

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027725.D
 Acq On : 02 Sep 2022 16:11
 Operator : SY/MD
 Sample : N4404-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVF5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	99	rBV	85169	97734	15.57%	2.174%
2	1.568	156	164	177	rBV	83881	100774	16.05%	2.241%
3	2.108	321	332	345	rBV	172349	246449	39.26%	5.481%
4	3.896	877	888	909	rBV	34882	120331	19.17%	2.676%
5	4.346	1012	1028	1062	rBV2	112512	286976	45.71%	6.383%
6	5.043	1229	1245	1279	rBV2	239581	627801	100.00%	13.963%
7	5.616	1411	1423	1451	rBV	141756	300344	47.84%	6.680%
8	5.912	1505	1515	1529	rVB7	3131	7279	1.16%	0.162%
9	6.066	1548	1563	1593	rBV2	139484	303201	48.30%	6.744%
10	6.986	1838	1849	1871	rBV2	50470	102153	16.27%	2.272%
11	7.313	1939	1951	1969	rBV	259192	471850	75.16%	10.495%
12	7.394	1971	1976	1989	rVB2	9371	18099	2.88%	0.403%
13	7.622	2038	2047	2062	rBV	29735	57193	9.11%	1.272%
14	8.092	2182	2193	2234	rBV	195247	488778	77.86%	10.871%
15	8.850	2417	2429	2460	rBV	219273	370316	58.99%	8.236%
16	10.214	2838	2853	2870	rBV	89081	145933	23.25%	3.246%
17	11.249	3164	3175	3195	rBV	200446	318904	50.80%	7.093%
18	11.532	3253	3263	3280	rBV2	16286	30942	4.93%	0.688%
19	11.622	3280	3291	3314	rVB	242124	380206	60.56%	8.456%
20	12.349	3507	3517	3526	rBV7	6939	11011	1.75%	0.245%
21	12.580	3579	3589	3599	rBV5	4796	9880	1.57%	0.220%




Sum of corrected areas: 4496154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027725.D
Acq On : 02 Sep 2022 16:11
Operator : SY/MD
Sample : N4404-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

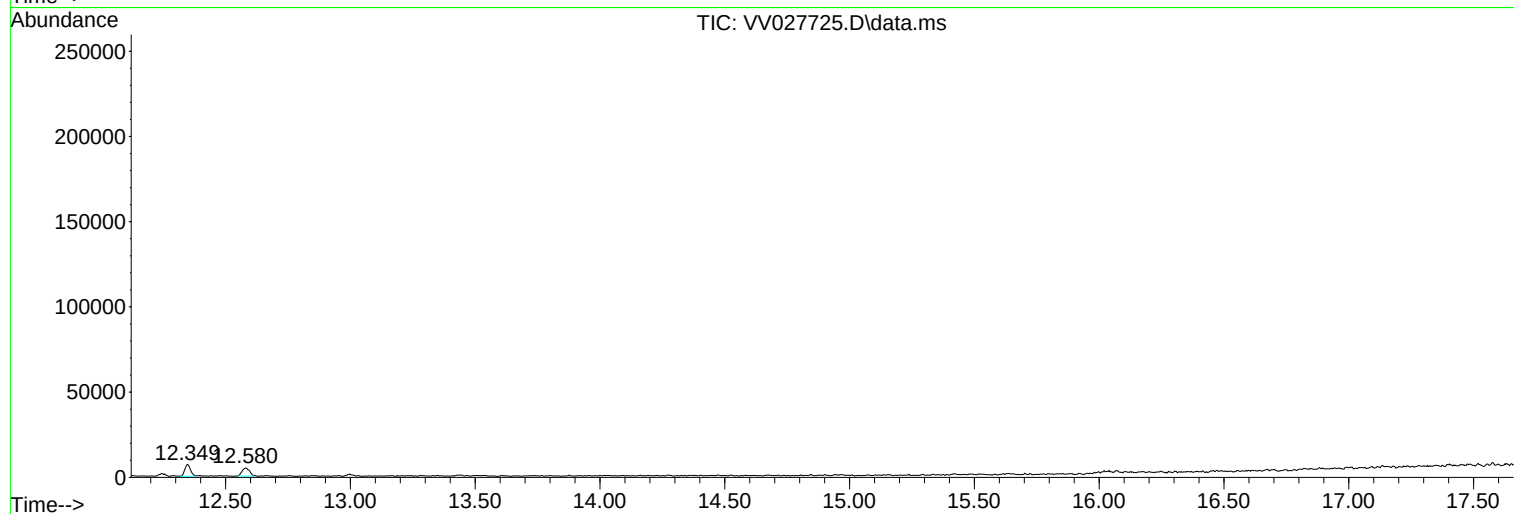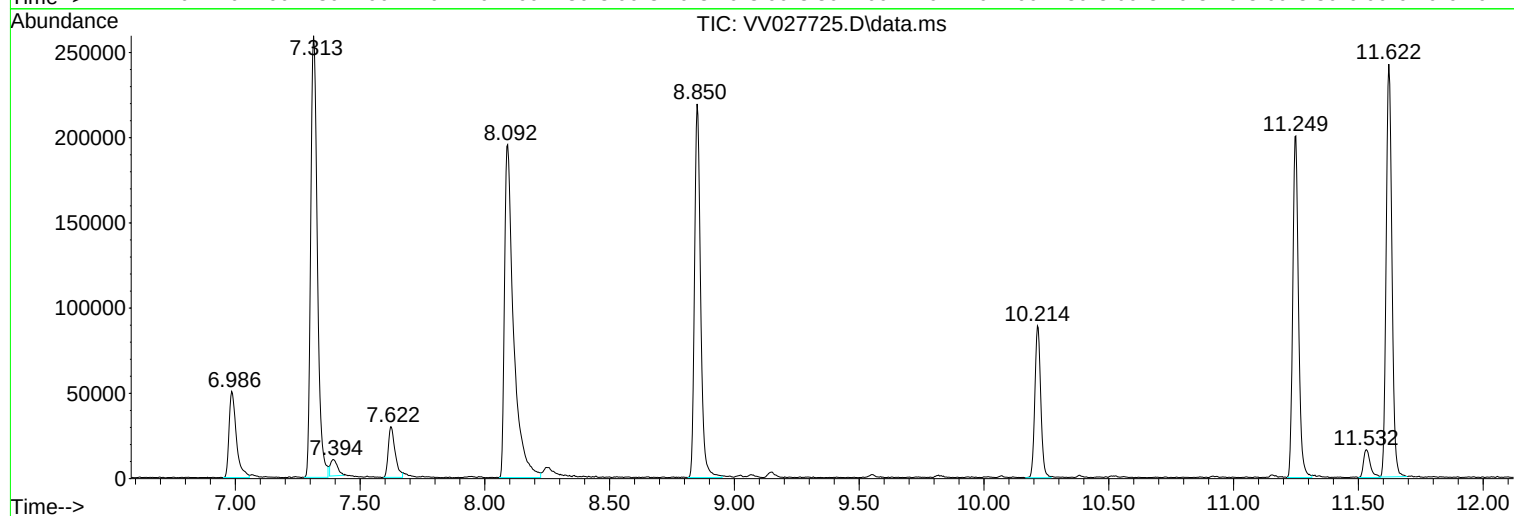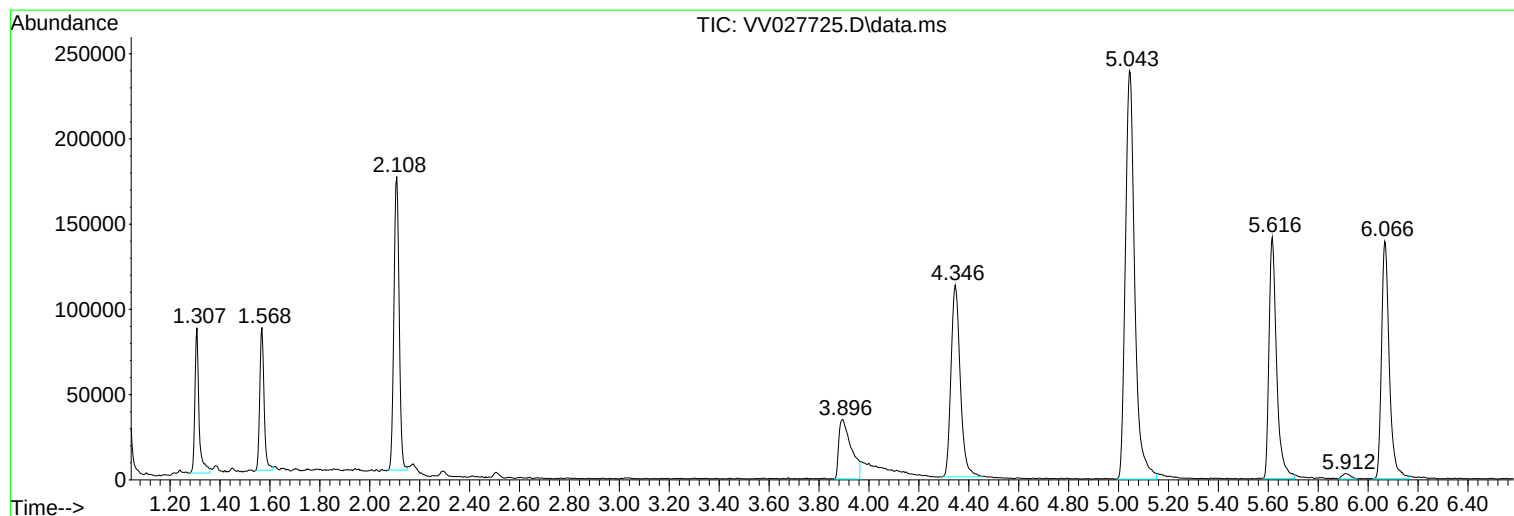

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027725.D
Acq On : 02 Sep 2022 16:11
Operator : SY/MD
Sample : N4404-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027725.D
Acq On : 02 Sep 2022 16:11
Operator : SY/MD
Sample : N4404-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc