

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027726.D
 Acq On : 02 Sep 2022 16:36
 Operator : SY/MD
 Sample : N4402-05 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	18	28	40	rVB2	4970	9873	1.54%	0.241%
2	1.565	155	163	178	rBV	87742	103770	16.23%	2.534%
3	2.105	322	331	342	rVB	32617	48825	7.64%	1.192%
4	2.503	444	455	467	rBV	14309	24624	3.85%	0.601%
5	3.899	875	889	913	rBV2	37800	140788	22.02%	3.437%
6	4.346	1012	1028	1060	rVB	120369	312517	48.87%	7.630%
7	5.043	1229	1245	1272	rBV2	250954	639474	100.00%	15.613%
8	5.616	1411	1423	1447	rBV	128429	274088	42.86%	6.692%
9	6.066	1550	1563	1585	rBV	145046	307111	48.03%	7.498%
10	7.313	1940	1951	1973	rBV	254829	457101	71.48%	11.160%
11	8.088	2180	2192	2225	rBV	193901	491613	76.88%	12.003%
12	8.850	2418	2429	2458	rBV	195852	352107	55.06%	8.597%
13	8.973	2458	2467	2481	rVB3	23861	40641	6.36%	0.992%
14	10.214	2843	2853	2873	rBV2	93244	152544	23.85%	3.724%
15	11.246	3162	3174	3195	rBV	185566	302903	47.37%	7.396%
16	11.548	3259	3268	3278	rVB7	5600	9168	1.43%	0.224%
17	11.622	3280	3291	3315	rBV	246336	409794	64.08%	10.005%
18	12.345	3507	3516	3530	rBV5	11091	18763	2.93%	0.458%




Sum of corrected areas: 4095704

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027726.D
Acq On : 02 Sep 2022 16:36
Operator : SY/MD
Sample : N4402-05 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

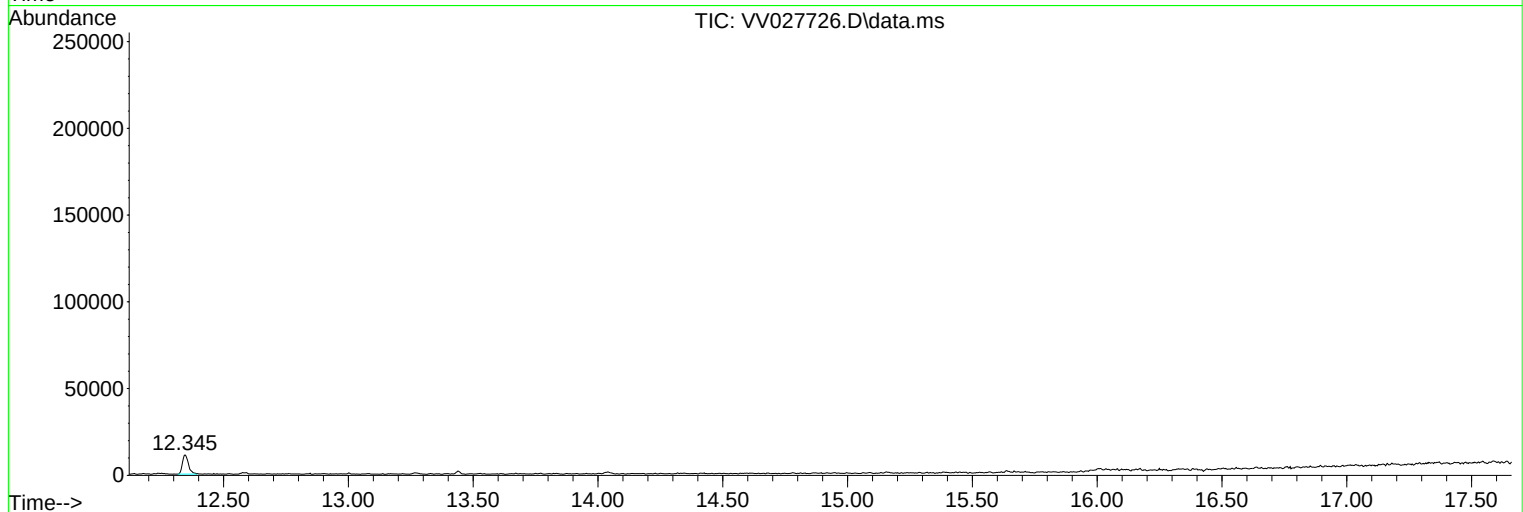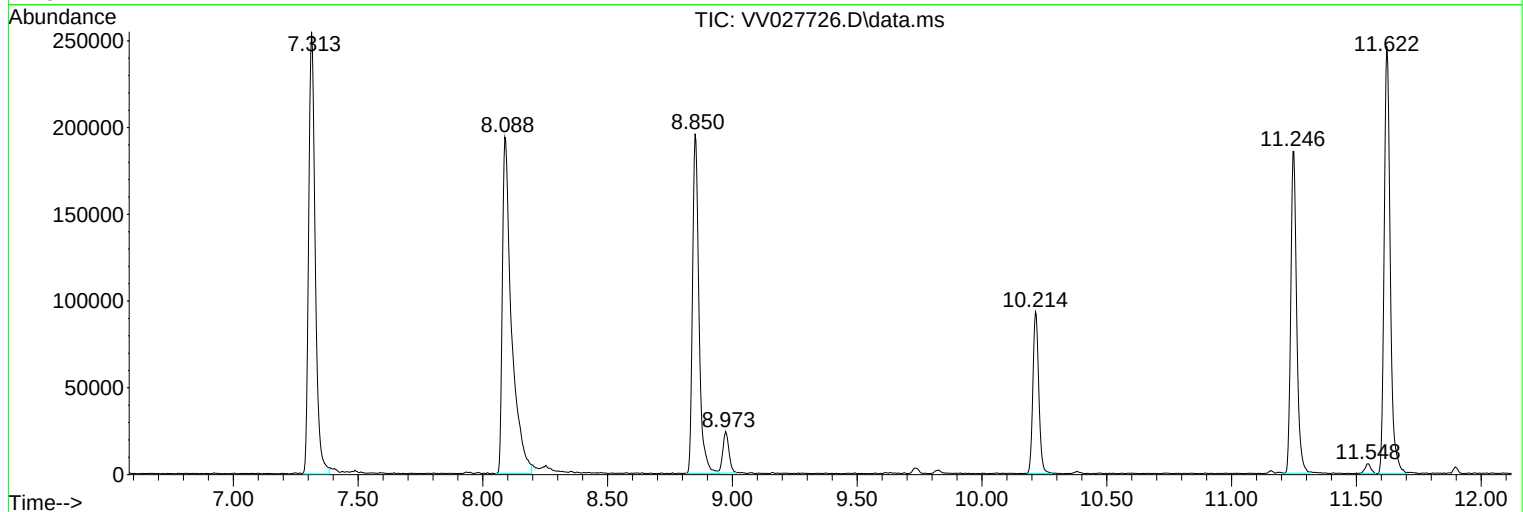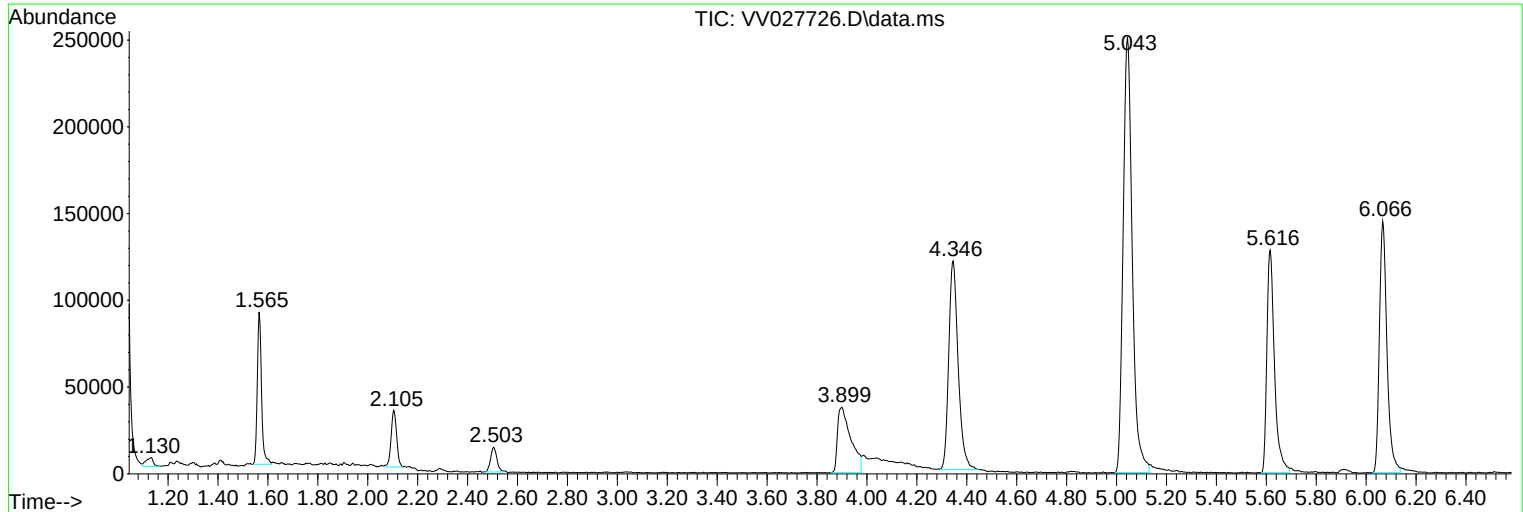

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027726.D
Acq On : 02 Sep 2022 16:36
Operator : SY/MD
Sample : N4402-05 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,1,1,2-tetrachloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.973	0.58 ug/L	40641	Chlorobenzene-d5	8.850

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	86
2			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	72
3			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	59
4			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	43
5			4-Chloro-3-fluoropyridine	131	C5H3ClFN	002546-56-7	10

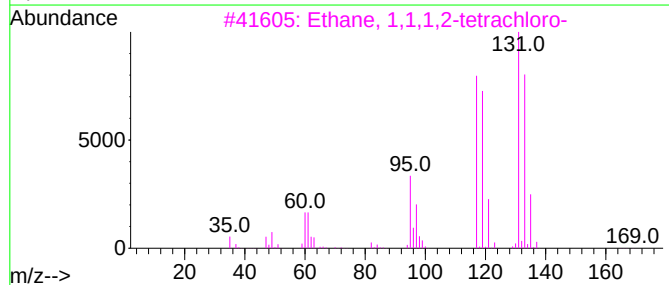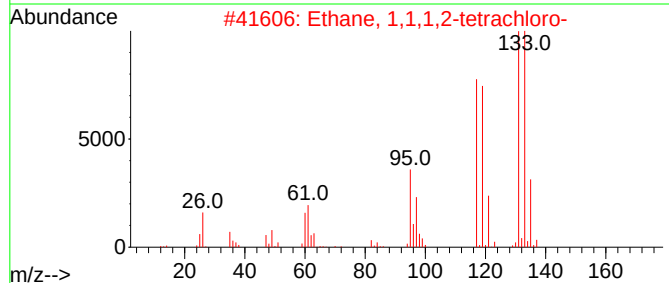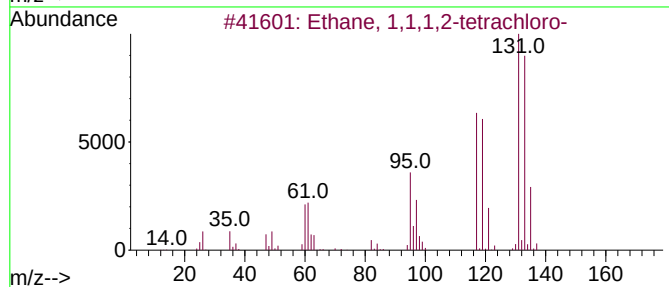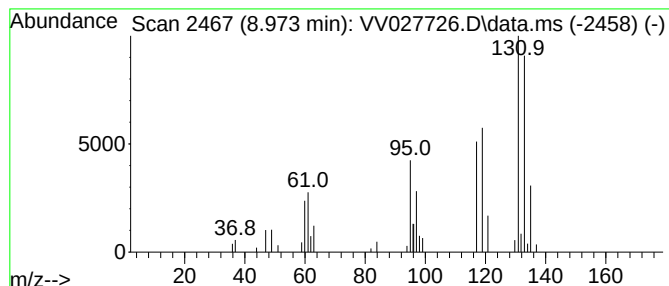

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027726.D
Acq On : 02 Sep 2022 16:36
Operator : SY/MD
Sample : N4402-05 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,1,1,2...	8.973	0.6	ug/L	40641	2	8.850	352107	5.0