

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027732.D
 Acq On : 02 Sep 2022 19:02
 Operator : SY/MD
 Sample : N4418-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	102	rBV2	144369	179423	5.52%	1.443%
2	1.568	155	164	174	rBV	83066	98332	3.03%	0.791%
3	2.108	321	332	346	rBV	170625	253101	7.79%	2.035%
4	2.761	526	535	548	rBV3	24231	44302	1.36%	0.356%
5	3.905	875	891	948	rBV	922465	2409829	74.20%	19.378%
6	4.346	1013	1028	1069	rVB	113661	295380	9.09%	2.375%
7	5.043	1229	1245	1283	rBV2	235002	618665	19.05%	4.975%
8	5.616	1411	1423	1447	rBV	134969	281834	8.68%	2.266%
9	5.908	1501	1514	1548	rBV	1168765	2351300	72.39%	18.907%
10	6.069	1551	1564	1593	rVB	139616	303340	9.34%	2.439%
11	6.985	1838	1849	1878	rBV	57218	116041	3.57%	0.933%
12	7.313	1940	1951	1976	rBV	259533	467806	14.40%	3.762%
13	7.625	2039	2048	2073	rBV2	32307	63059	1.94%	0.507%
14	7.973	2139	2156	2181	rBV	1936417	3247927	100.00%	26.117%
15	8.088	2183	2192	2228	rVB	218725	499246	15.37%	4.015%
16	8.850	2418	2429	2451	rBV	204519	341714	10.52%	2.748%
17	10.214	2841	2853	2874	rBV	89622	144544	4.45%	1.162%
18	11.246	3164	3174	3200	rBV	185305	299361	9.22%	2.407%
19	11.529	3254	3262	3279	rBV2	25915	45738	1.41%	0.368%
20	11.622	3279	3291	3307	rVV	236688	375041	11.55%	3.016%




Sum of corrected areas: 12435983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027732.D
Acq On : 02 Sep 2022 19:02
Operator : SY/MD
Sample : N4418-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

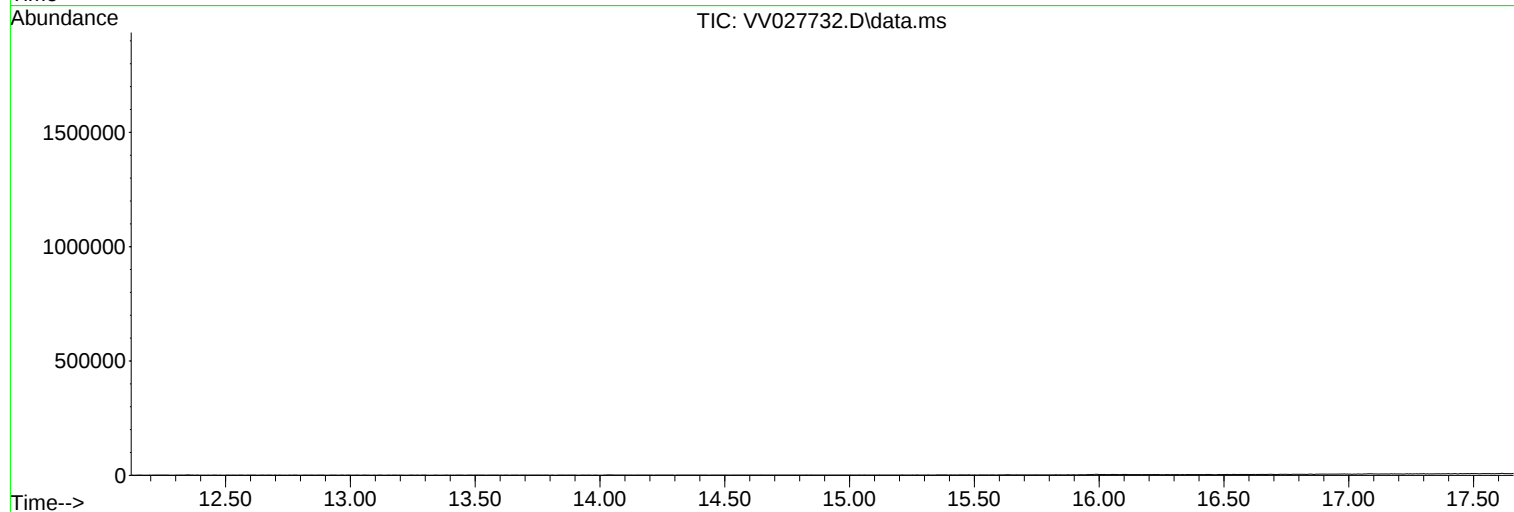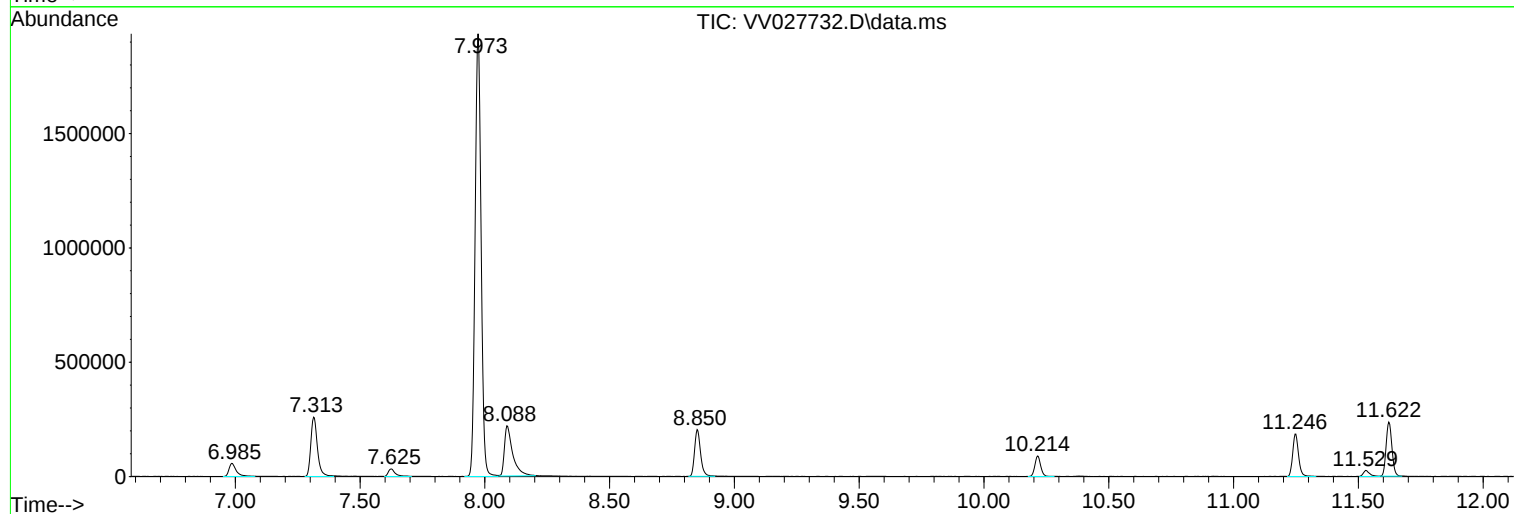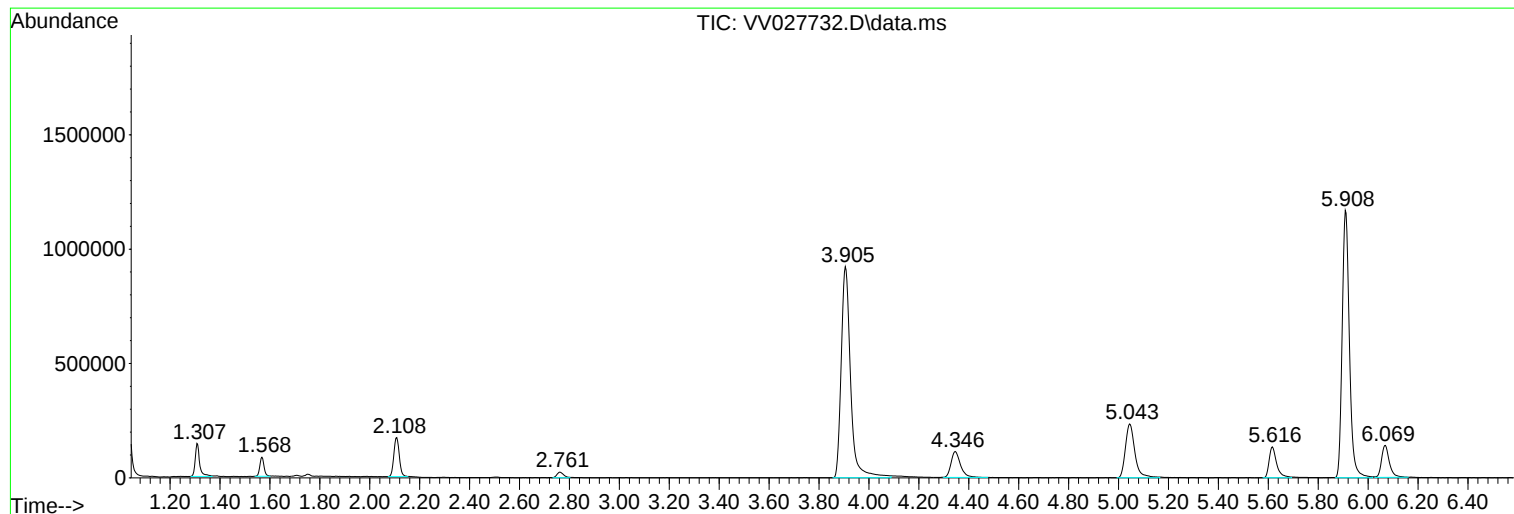

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027732.D
Acq On : 02 Sep 2022 19:02
Operator : SY/MD
Sample : N4418-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.529	0.76 ug/L	45738	1,4-Dichlorobenzene-d4	11.249

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	90
2		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	83
3		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	83
4		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	78
5		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	64

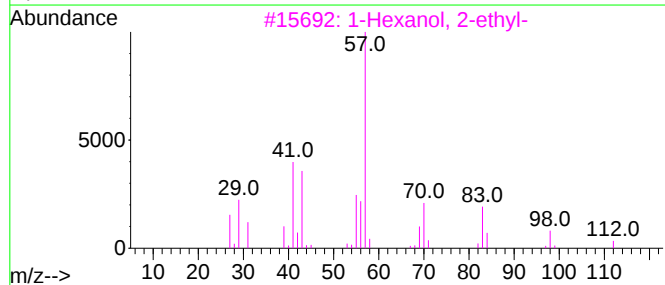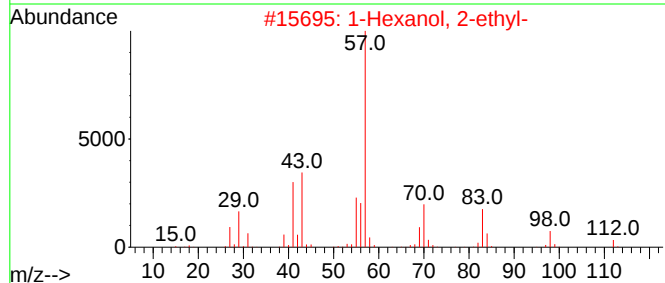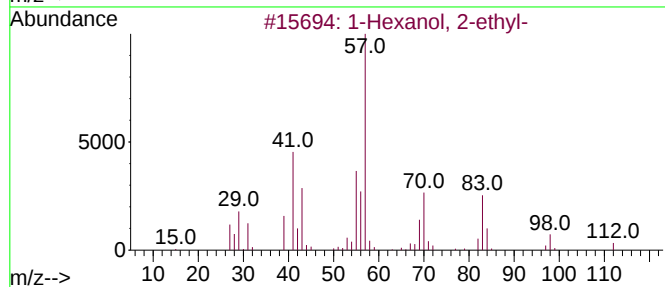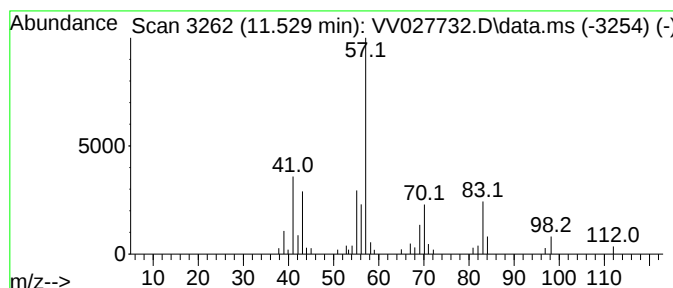

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
Data File : VV027732.D
Acq On : 02 Sep 2022 19:02
Operator : SY/MD
Sample : N4418-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	11.529	0.8	ug/L	45738	3	11.249	299361	5.0