
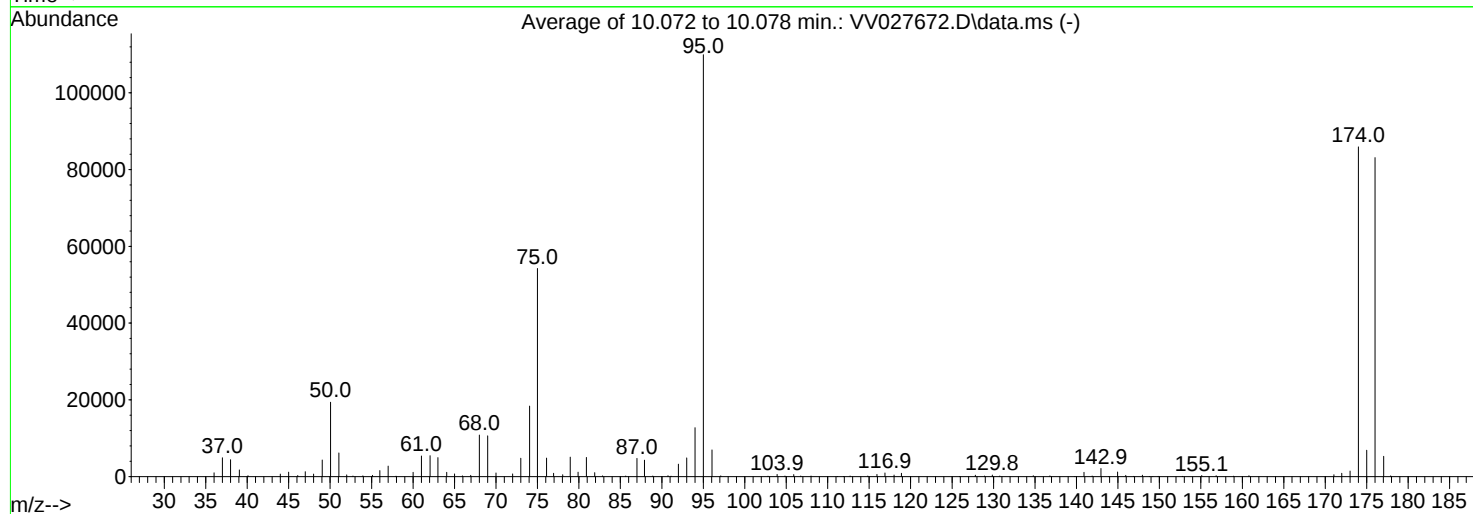


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090122\
 Data File : VV027672.D
 Acq On : 01 Sep 2022 16:19
 Operator : SY/MD
 Sample : BFB366
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB366

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR083122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Sep 03 05:30:57 2022

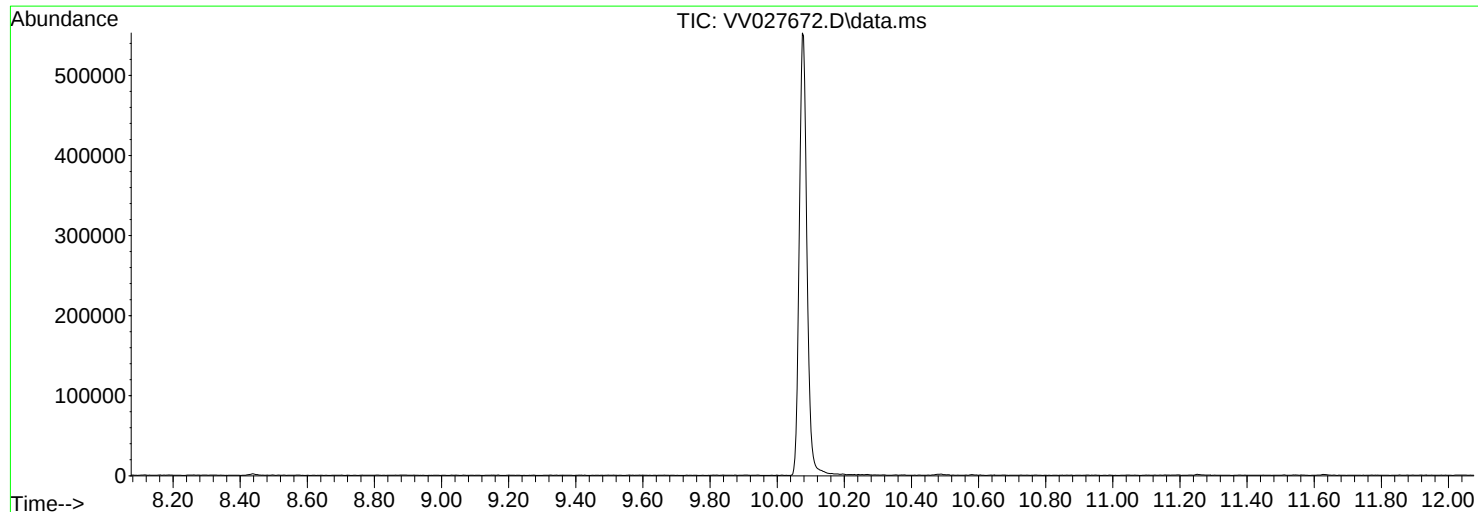

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	19352	PASS
75	95	30	80	49.3	54248	PASS
95	95	100	100	100.0	109931	PASS
96	95	5	9	6.3	6950	PASS
173	174	0.00	2	1.7	1432	PASS
174	95	50	120	78.2	85917	PASS
175	174	5	9	8.0	6877	PASS
176	174	95	105	96.8	83155	PASS
177	176	5	10	6.3	5257	PASS

m/z	Abundance
39.80	227.0
44.00	322.0

Instrument :
MSVOA_V
ClientSampleId :
BFB366

m/z	Abundance
36.00	973.0
37.00	4810.0
38.00	4208.0
39.00	1663.0
44.00	954.0
45.00	1088.0
46.10	287.0
47.00	1313.0
48.00	677.0
49.00	4133.0
50.00	18912.0
51.10	5865.0
52.00	337.0
52.70	135.0
53.90	167.0
55.10	316.0
56.00	1514.0
57.00	2707.0
58.00	146.0
60.00	1148.0
61.00	5157.0
62.00	5189.0
63.00	4714.0
64.10	944.0
65.00	597.0
65.90	148.0
67.00	277.0
68.00	10443.0
69.00	10140.0
70.00	876.0
72.00	655.0
73.00	4624.0
74.10	17680.0
75.00	51160.0
76.10	4739.0
76.90	881.0
78.10	480.0
79.00	4715.0
79.90	1069.0
80.90	4672.0
81.90	904.0
82.90	199.0
85.60	123.0
87.00	4572.0
87.90	4021.0
88.90	143.0
91.10	272.0
92.00	2951.0
93.00	4710.0
94.00	12018.0
95.00	103960.0
96.00	6611.0
97.10	195.0
103.90	543.0
104.80	140.0
105.90	479.0
106.80	161.0
108.10	112.0
112.70	103.0
114.80	129.0
115.90	472.0
116.90	871.0
118.00	402.0
118.90	826.0
127.80	298.0
128.90	102.0
129.90	376.0
130.70	166.0
134.80	195.0
136.90	177.0
140.90	1060.0
141.90	142.0
143.00	2057.0
145.00	1194.0
145.90	252.0
147.90	328.0
148.80	114.0
155.10	219.0
156.80	200.0
158.90	111.0
160.80	203.0
171.00	479.0
172.00	664.0
173.00	1246.0
174.00	79056.0
175.00	6354.0
176.00	76248.0
177.00	4931.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB366

m/z	Abundance
36.00	1002.0
37.00	5033.0
38.00	4510.0
39.00	1768.0
40.10	310.0
44.00	982.0
45.00	1199.0
46.10	312.0
46.90	1324.0
48.10	669.0
49.00	4460.0
50.10	20016.0
51.00	6316.0
52.00	438.0
52.70	160.0
54.00	206.0
55.10	339.0
56.00	1635.0
57.00	2855.0
58.00	120.0
60.00	1117.0
61.00	5560.0
62.10	5553.0
63.00	5168.0
64.00	1173.0
65.00	707.0
66.00	189.0
66.90	302.0
68.00	11223.0
69.00	10920.0
70.00	990.0
72.00	686.0
73.00	4962.0
74.00	18896.0
75.00	56136.0
76.10	5011.0
77.00	900.0
78.00	501.0
78.90	5296.0
79.90	1171.0
80.90	5144.0
81.90	1050.0
82.80	214.0
85.70	172.0
87.00	4867.0
87.90	4410.0
88.90	154.0
90.70	312.0
92.00	3371.0
93.00	5079.0
94.00	13207.0
95.00	113904.0
96.10	7130.0
97.10	207.0
102.80	129.0
103.90	579.0
104.90	168.0
105.90	555.0
106.80	165.0
108.00	128.0
112.70	132.0
114.90	147.0
116.00	586.0
116.90	992.0
118.00	421.0
118.90	898.0
127.80	354.0
128.90	148.0
129.90	422.0
130.70	142.0
134.80	218.0
136.80	194.0
140.90	1132.0
141.90	176.0
142.90	2207.0
143.90	129.0
144.90	1216.0
146.00	315.0
146.90	125.0
148.00	350.0
149.80	119.0
152.80	115.0
155.10	290.0
156.80	238.0
159.00	116.0
160.80	238.0
171.10	509.0
172.00	922.0
173.00	1486.0
174.00	88984.0
175.00	7189.0
176.00	85952.0

Instrument :
MSVOA_V
ClientSampleId :
BFB366

177.105384.0

177.90185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB366

m/z	Abundance
36.00	942.0
37.00	4921.0
38.00	4508.0
39.10	1759.0
40.10	386.0
44.00	968.0
45.00	1110.0
46.10	286.0
47.10	1182.0
47.90	605.0
49.10	4405.0
50.10	19128.0
51.00	6320.0
52.00	513.0
52.80	195.0
54.00	219.0
55.10	307.0
56.00	1589.0
57.00	2695.0
57.90	103.0
60.00	1039.0
61.00	5357.0
62.10	5565.0
63.00	4993.0
64.00	1249.0
65.00	788.0
66.00	181.0
66.90	319.0
68.00	10856.0
69.00	10770.0
70.00	917.0
72.00	676.0
73.00	4747.0
74.00	18496.0
75.00	55448.0
76.10	4702.0
77.00	802.0
78.00	475.0
78.90	5258.0
79.90	1178.0
80.90	5151.0
81.90	1085.0
82.80	182.0
85.70	201.0
87.00	4801.0
87.90	4434.0
88.90	123.0
90.80	333.0
92.00	3356.0
93.00	4857.0
94.00	13050.0
95.00	111928.0
96.10	7110.0
97.10	210.0
102.80	158.0
103.90	577.0
104.90	170.0
105.90	583.0
106.70	170.0
107.90	158.0
111.20	121.0
111.90	109.0
112.70	163.0
114.90	140.0
116.00	606.0
116.90	1006.0
118.00	410.0
118.90	907.0
125.90	110.0
127.80	454.0
128.90	190.0
129.80	427.0
130.80	156.0
134.80	226.0
136.70	184.0
139.80	112.0
140.90	1094.0
141.90	187.0
142.90	2086.0
144.90	1181.0
146.00	321.0
146.90	123.0
148.00	334.0
149.20	107.0
149.90	138.0
152.80	122.0
155.10	314.0
156.90	230.0
159.00	129.0
160.80	204.0
170.00	100.0
171.10	501.0

Instrument :
MSVOA_V
ClientSampleId :
BFB366

172.00	988.0
173.00	1564.0
174.00	89712.0
175.00	7089.0
176.00	87264.0
177.00	5457.0
177.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB366