


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092019\
 Data File : VV012915.D
 Acq On : 20 Sep 2019 08:57
 Operator : SY/MD
 Sample : BFB13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB131

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR070819SIM.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 13 06:44:17 2019

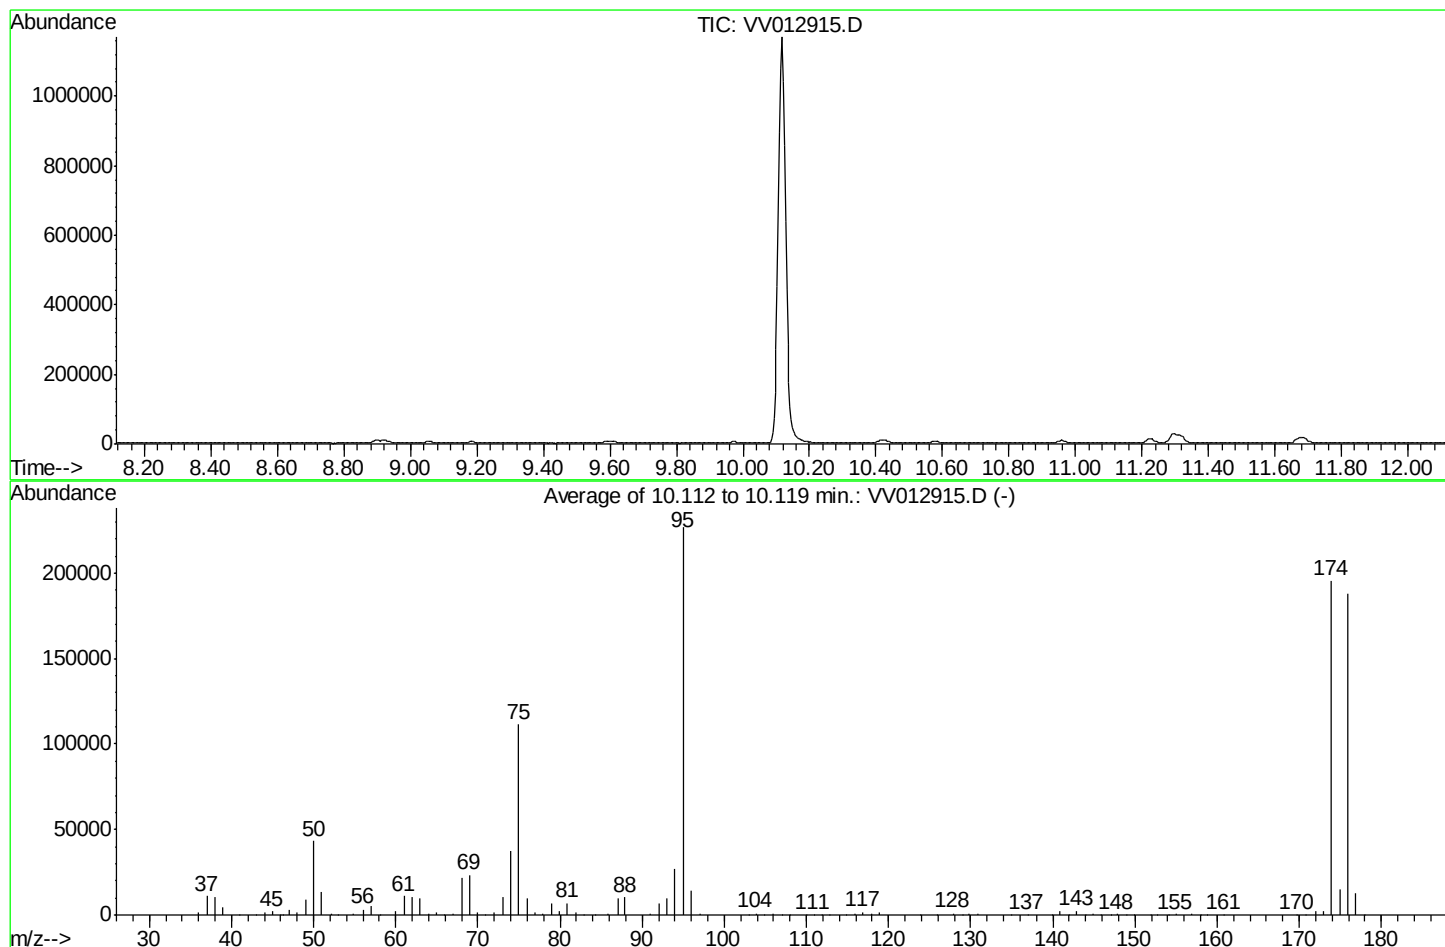

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	43341	PASS
75	95	30	80	49.2	111565	PASS
95	95	100	100	100.0	226794	PASS
96	95	5	9	6.4	14604	PASS
173	174	0.00	2	1.1	2230	PASS
174	95	50	120	86.3	195690	PASS
175	174	5	9	7.6	14904	PASS
176	174	95	101	96.2	188330	PASS
177	176	5	9	6.6	12439	PASS