

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092822\
 Data File : VW028167.D
 Acq On : 28 Sep 2022 18:29
 Operator : SY/MD
 Sample : N4871-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H61

Quant Time: Sep 29 01:30:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	163621	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	168397	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	80807	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	47836	2.820	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	56.400%
7) Chloroethane-d5	1.561	69	48676	3.609	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.200%
11) 1,1-Dichloroethene-d2	2.101	63	67556	2.296	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	46.000%#
20) 2-Butanone-d5	3.886	46	163410	57.061	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.120%
24) Chloroform-d	4.343	84	120701	4.459	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
26) 1,2-Dichloroethane-d4	5.027	65	59781	4.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	5.043	84	211795	3.836	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.800%
36) 1,2-Dichloropropane-d6	6.066	67	70953	4.122	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.400%
41) Toluene-d8	7.313	98	166531	3.332	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.600%#
43) trans-1,3-Dichloroprop...	7.622	79	21766	3.501	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%
46) 2-Hexanone-d5	8.085	63	131341	50.610	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.220%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	58847	5.001	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	75595	4.769	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.400%
Target Compounds					Qvalue	
13) Acetone	2.175	43	9923	4.498	ug/L	90
14) Carbon disulfide	2.288	76	7599	0.350	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028167.D
Acq On : 28 Sep 2022 18:29
Operator : SY/MD
Sample : N4871-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H61

Quant Time: Sep 29 01:30:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

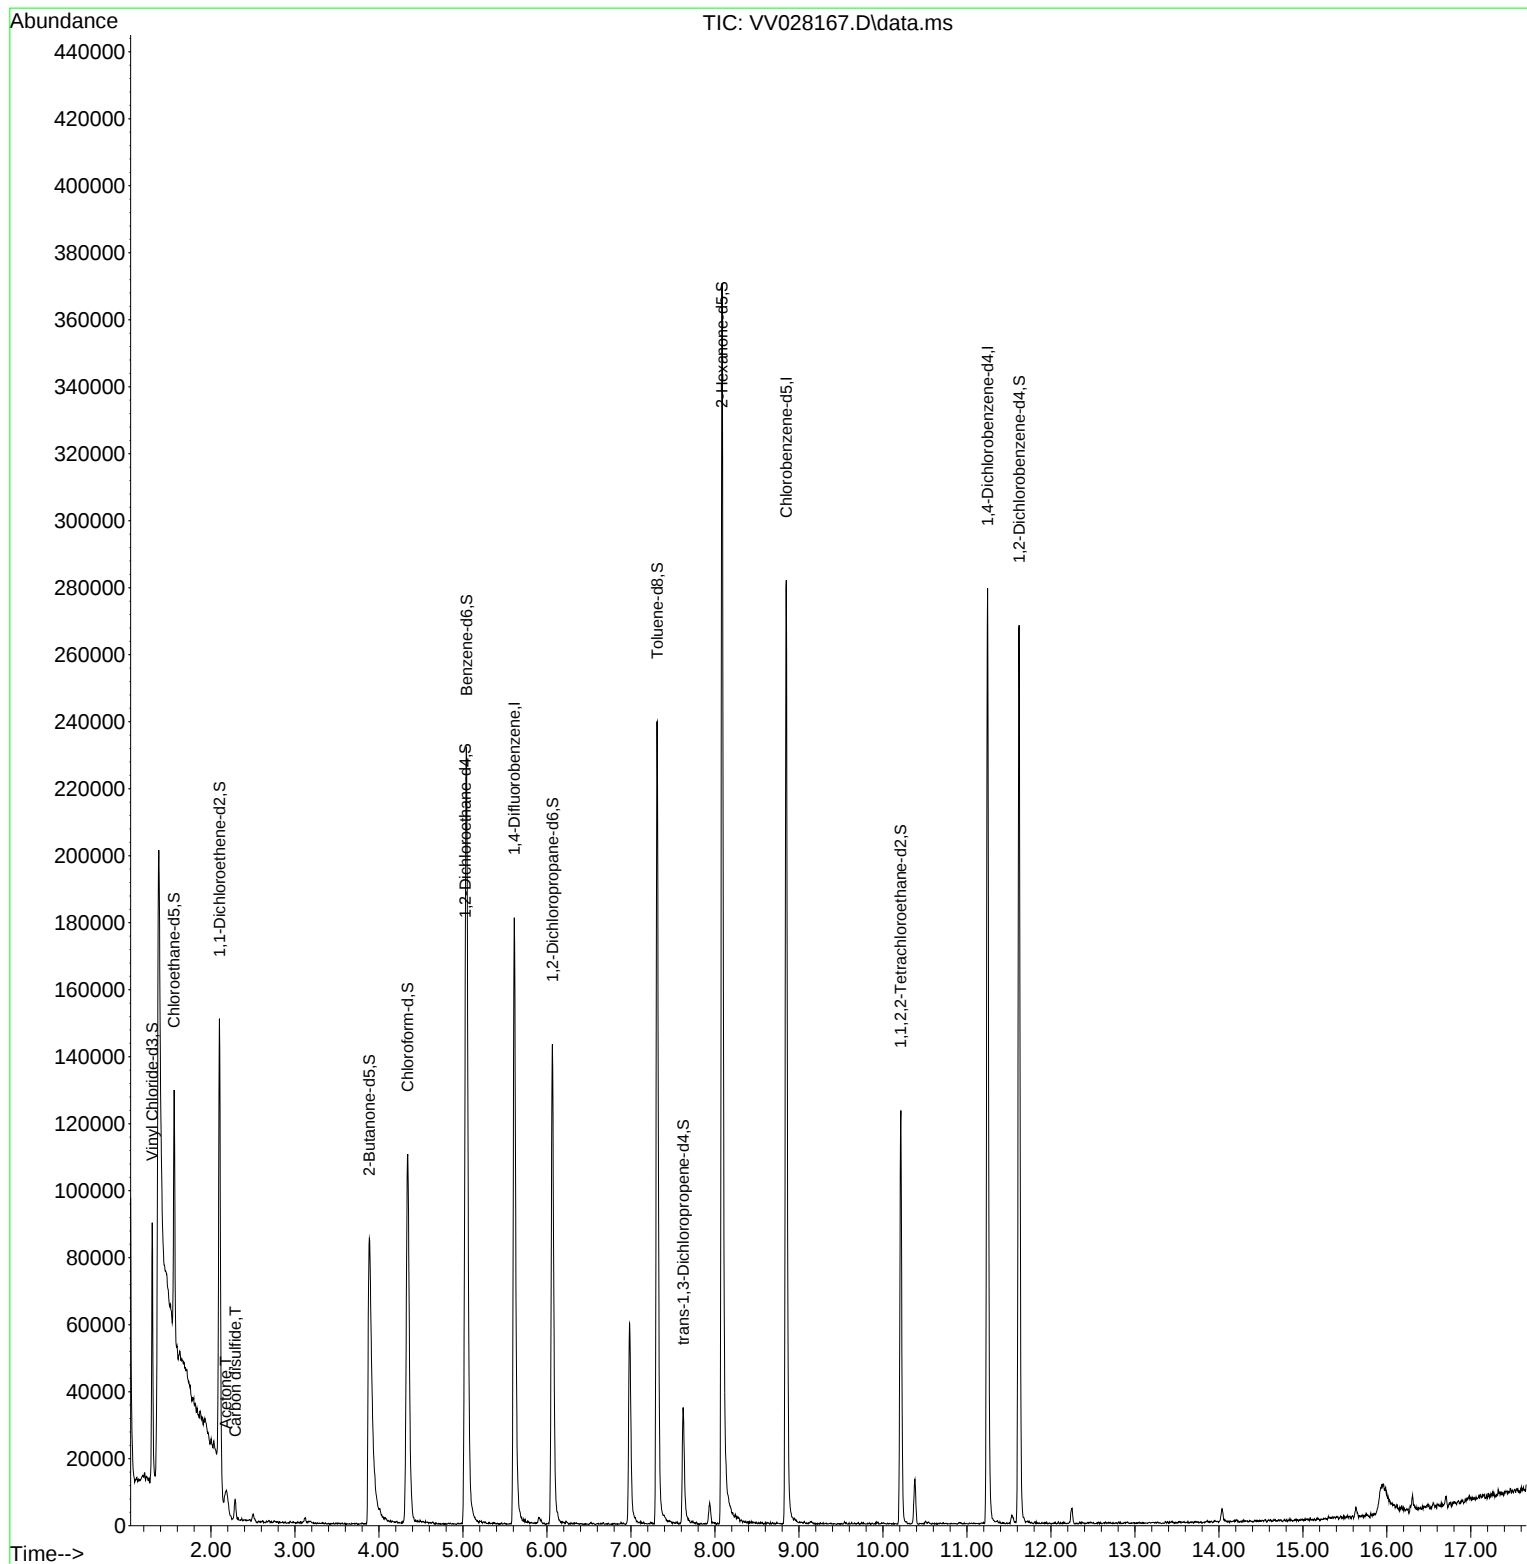

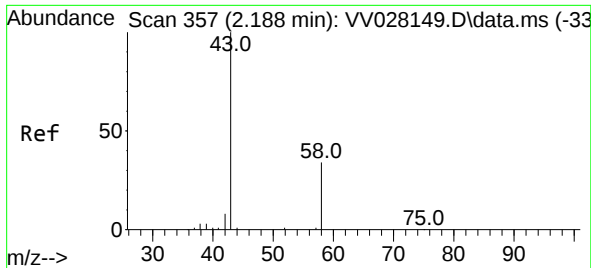

#13

Acetone

Concen: 4.498 ug/L

RT: 2.175 min Scan# 31

Delta R.T. -0.013 min

Lab File: VV028167.D

Acq: 28 Sep 2022 18:29

Instrument :

MSVOA_V

ClientSampleId :





F5H61

Tgt Ion: 43 Resp: 9923

Ion Ratio Lower Upper

43 100

58 38.6 0.0 65.6

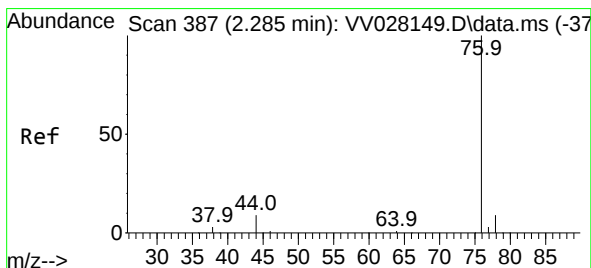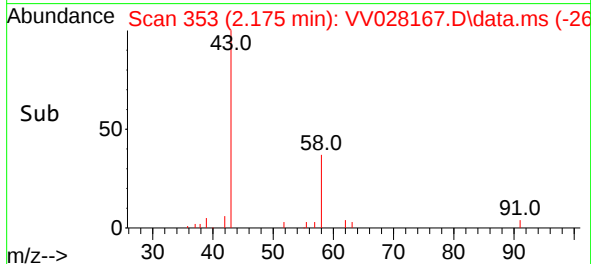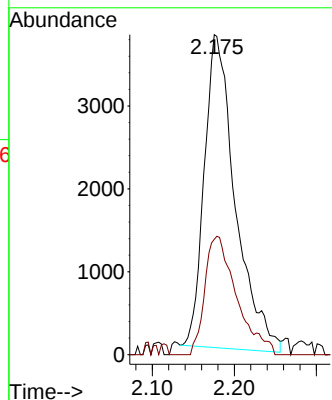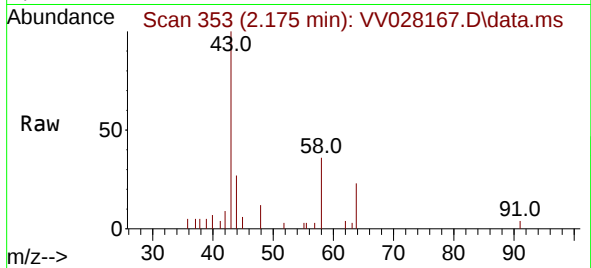

#14

Carbon disulfide

Concen: 0.350 ug/L

RT: 2.288 min Scan# 388

Delta R.T. 0.003 min

Lab File: VV028167.D

Acq: 28 Sep 2022 18:29

Tgt Ion: 76 Resp: 7599

Ion Ratio Lower Upper

76 100

78 9.4 7.6 11.4

