

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
 Data File : VV028151.D
 Acq On : 28 Sep 2022 12:01
 Operator : SY/MD
 Sample : N4856-04DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H30DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	90	rVB	93934	91934	13.19%	1.533%
2	1.561	155	162	177	rVB	84998	99845	14.33%	1.665%
3	2.098	319	329	347	rVB	160218	234516	33.66%	3.912%
4	2.500	444	454	467	rBV2	15380	26238	3.77%	0.438%
5	3.896	874	888	932	rBV2	63352	312308	44.82%	5.209%
6	4.336	1008	1025	1049	rBV	119717	306315	43.96%	5.109%
7	5.037	1226	1243	1278	rBV3	261505	649284	93.18%	10.830%
8	5.606	1407	1420	1447	rBV	193432	402831	57.81%	6.719%
9	6.060	1549	1561	1586	rBV	155019	323961	46.49%	5.403%
10	6.982	1836	1848	1867	rBV2	65822	128843	18.49%	2.149%
11	7.310	1938	1950	1975	rBV	256411	461787	66.27%	7.702%
12	7.619	2036	2046	2061	rBV	40500	75191	10.79%	1.254%
13	7.969	2133	2155	2175	rBV	307040	527747	75.74%	8.803%
14	8.085	2180	2191	2225	rBV	352522	696807	100.00%	11.622%
15	8.847	2413	2428	2449	rBV	306757	511421	73.39%	8.530%
16	10.211	2841	2852	2875	rBV	122417	196272	28.17%	3.274%
17	10.378	2892	2904	2918	rBV3	8748	14825	2.13%	0.247%
18	11.246	3163	3174	3197	rBV	298971	474513	68.10%	7.915%
19	11.619	3278	3290	3309	rBV	280813	451391	64.78%	7.529%
20	14.037	4030	4042	4055	rVB	5598	9367	1.34%	0.156%




Sum of corrected areas: 5995396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028151.D
Acq On : 28 Sep 2022 12:01
Operator : SY/MD
Sample : N4856-04DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

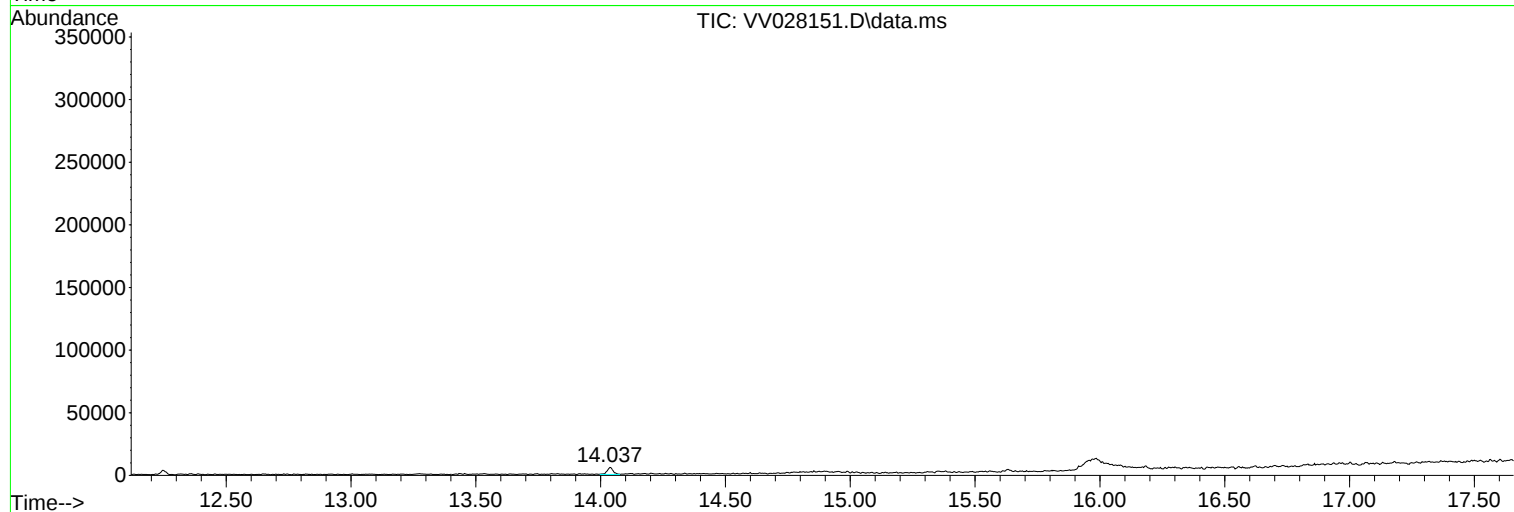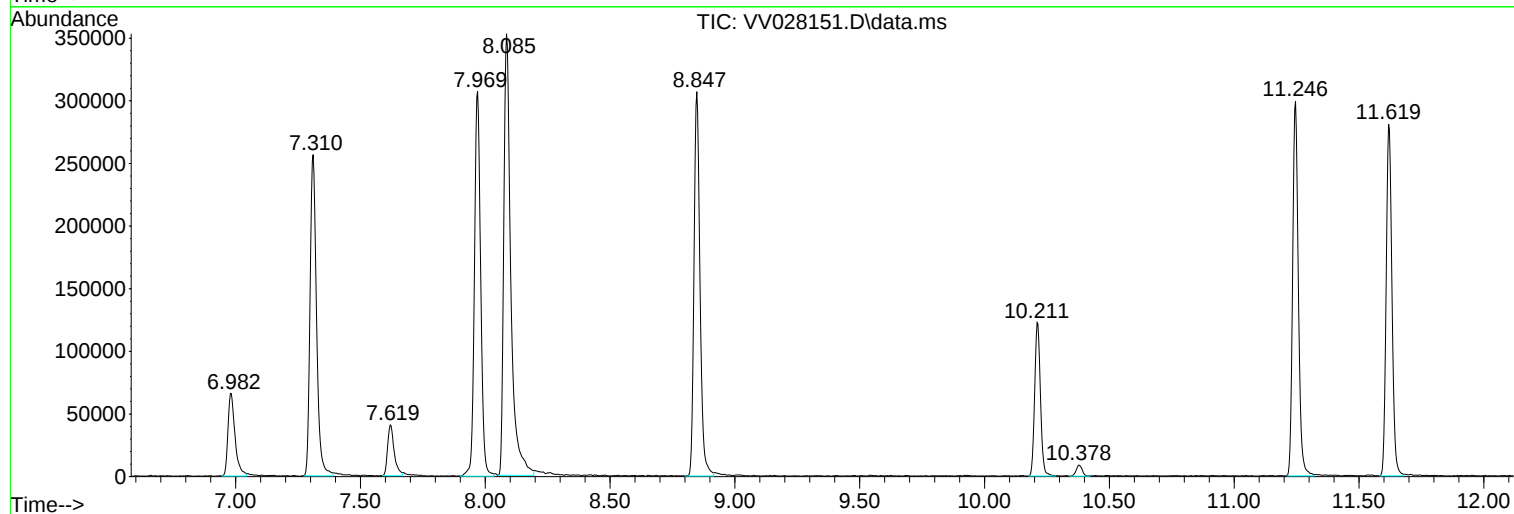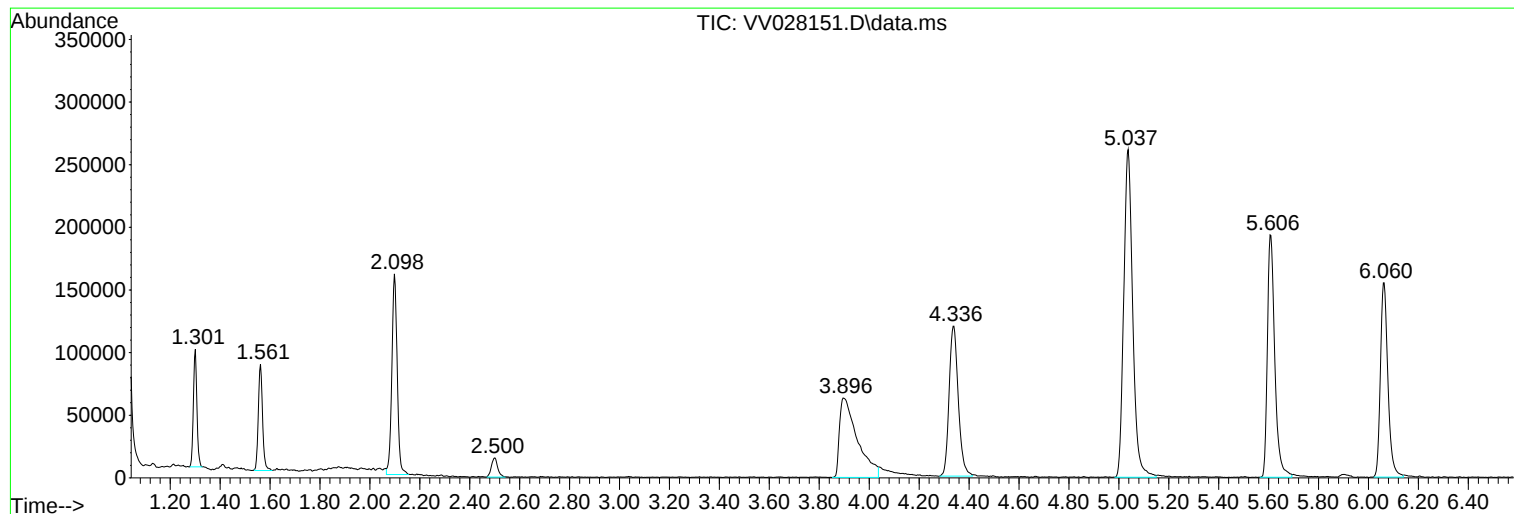

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028151.D
Acq On : 28 Sep 2022 12:01
Operator : SY/MD
Sample : N4856-04DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028151.D
Acq On : 28 Sep 2022 12:01
Operator : SY/MD
Sample : N4856-04DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H30DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc