

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
 Data File : VV028160.D
 Acq On : 28 Sep 2022 15:38
 Operator : SY/MD
 Sample : N4871-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	93	rVB	73802	75808	14.55%	1.743%
2	1.410	110	115	122	rBV2	7800	8321	1.60%	0.191%
3	1.565	155	163	174	rVV	72708	88560	17.00%	2.036%
4	2.101	320	330	347	rVB	134352	196246	37.68%	4.511%
5	3.889	875	886	922	rBV	69134	242521	46.56%	5.575%
6	4.343	1007	1027	1053	rBV	96854	247909	47.59%	5.699%
7	5.040	1228	1244	1273	rBV2	199346	504479	96.85%	11.597%
8	5.613	1409	1422	1442	rBV2	164489	331583	63.66%	7.623%
9	6.066	1549	1563	1587	rBV	114901	237144	45.53%	5.452%
10	6.986	1836	1849	1867	rBV2	50046	94828	18.21%	2.180%
11	7.313	1940	1951	1976	rBV	200007	360578	69.22%	8.289%
12	7.622	2038	2047	2066	rBV	30681	55500	10.65%	1.276%
13	7.937	2133	2145	2153	rBV2	3381	5948	1.14%	0.137%
14	8.085	2181	2191	2218	rBV	288600	520888	100.00%	11.975%
15	8.850	2418	2429	2456	rBV	268898	441455	84.75%	10.149%
16	10.214	2842	2853	2869	rBV	106960	169754	32.59%	3.902%
17	10.384	2893	2906	2919	rVB2	7182	11724	2.25%	0.270%
18	11.246	3161	3174	3194	rBV	247134	386233	74.15%	8.879%
19	11.622	3278	3291	3310	rBV	220387	351906	67.56%	8.090%
20	12.249	3472	3486	3495	rVB4	3094	5284	1.01%	0.121%
21	14.037	4032	4042	4053	rVB3	4768	7762	1.49%	0.178%
22	15.631	4528	4538	4544	rBV5	3661	5509	1.06%	0.127%




Sum of corrected areas: 4349940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028160.D
Acq On : 28 Sep 2022 15:38
Operator : SY/MD
Sample : N4871-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

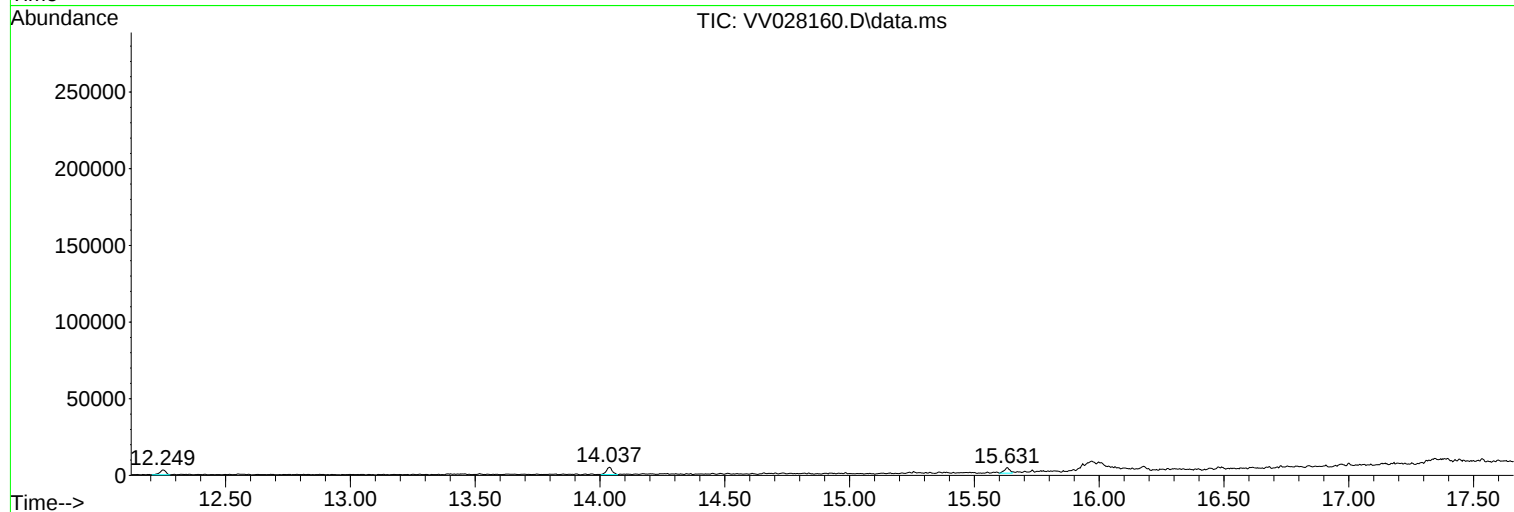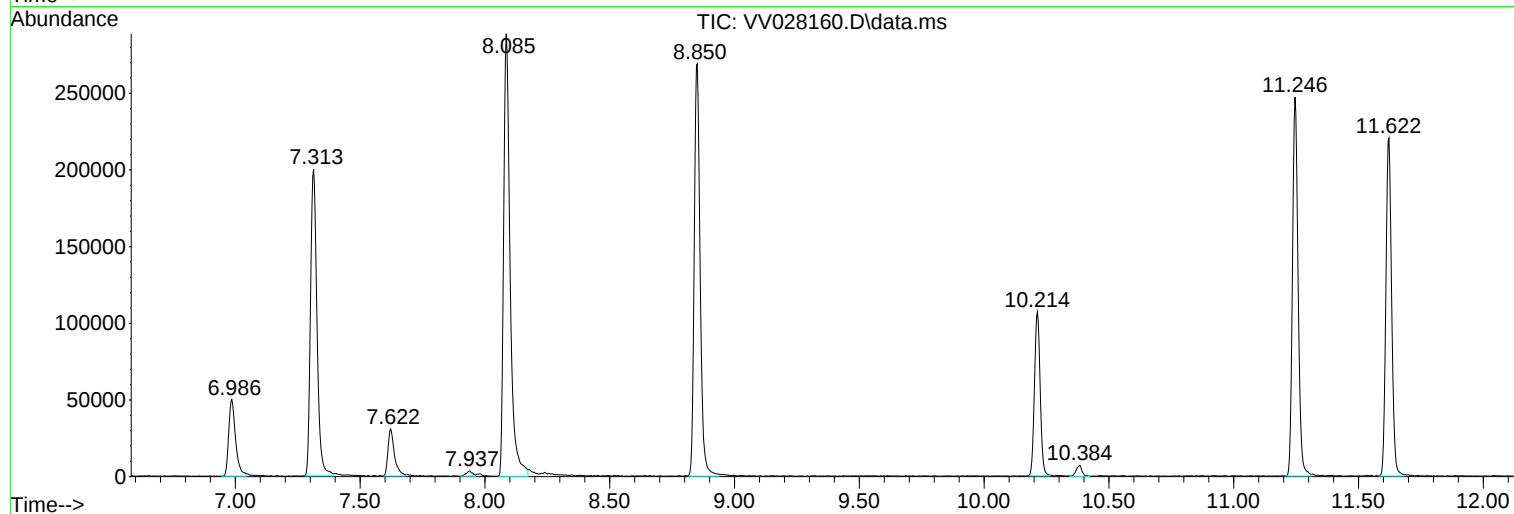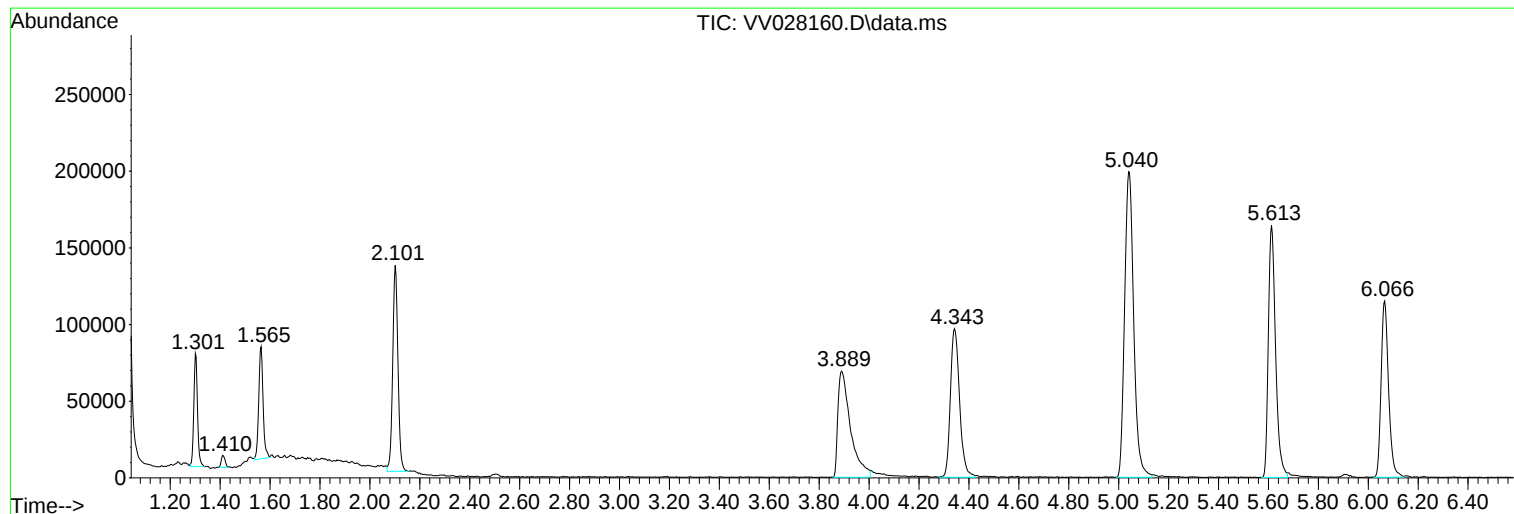

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028160.D
Acq On : 28 Sep 2022 15:38
Operator : SY/MD
Sample : N4871-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028160.D
Acq On : 28 Sep 2022 15:38
Operator : SY/MD
Sample : N4871-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
