

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
 Data File : VV028162.D
 Acq On : 28 Sep 2022 16:27
 Operator : SY/MD
 Sample : N4871-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H25

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	93	rVB	75274	76540	14.46%	1.793%
2	1.561	156	162	179	rVB	72629	85240	16.10%	1.996%
3	2.101	321	330	349	rVB	131210	191239	36.13%	4.479%
4	3.889	876	886	926	rBV	61128	215057	40.62%	5.037%
5	4.342	1011	1027	1059	rBV	92120	228015	43.07%	5.340%
6	5.040	1229	1244	1278	rBV3	184678	474621	89.66%	11.116%
7	5.612	1411	1422	1445	rBV	144703	292286	55.21%	6.846%
8	6.066	1546	1563	1590	rBV2	118902	247011	46.66%	5.785%
9	6.985	1838	1849	1875	rBV2	53193	108146	20.43%	2.533%
10	7.313	1939	1951	1978	rBV	207834	366613	69.25%	8.586%
11	7.622	2037	2047	2062	rBV2	31298	54760	10.34%	1.283%
12	7.972	2134	2156	2176	rBV3	60498	109032	20.60%	2.554%
13	8.085	2181	2191	2216	rBV	295296	529372	100.00%	12.398%
14	8.850	2417	2429	2457	rBV	228688	378269	71.46%	8.859%
15	10.214	2840	2853	2870	rBV	107346	173953	32.86%	4.074%
16	10.378	2895	2904	2916	rBV2	8900	14607	2.76%	0.342%
17	11.246	3162	3174	3195	rBV	225397	353885	66.85%	8.288%
18	11.622	3279	3291	3310	rBV	222488	355521	67.16%	8.327%
19	14.040	4033	4043	4053	rVB3	4921	8550	1.62%	0.200%
20	15.943	4628	4635	4639	rBV8	4870	7011	1.32%	0.164%




Sum of corrected areas: 4269728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028162.D
Acq On : 28 Sep 2022 16:27
Operator : SY/MD
Sample : N4871-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

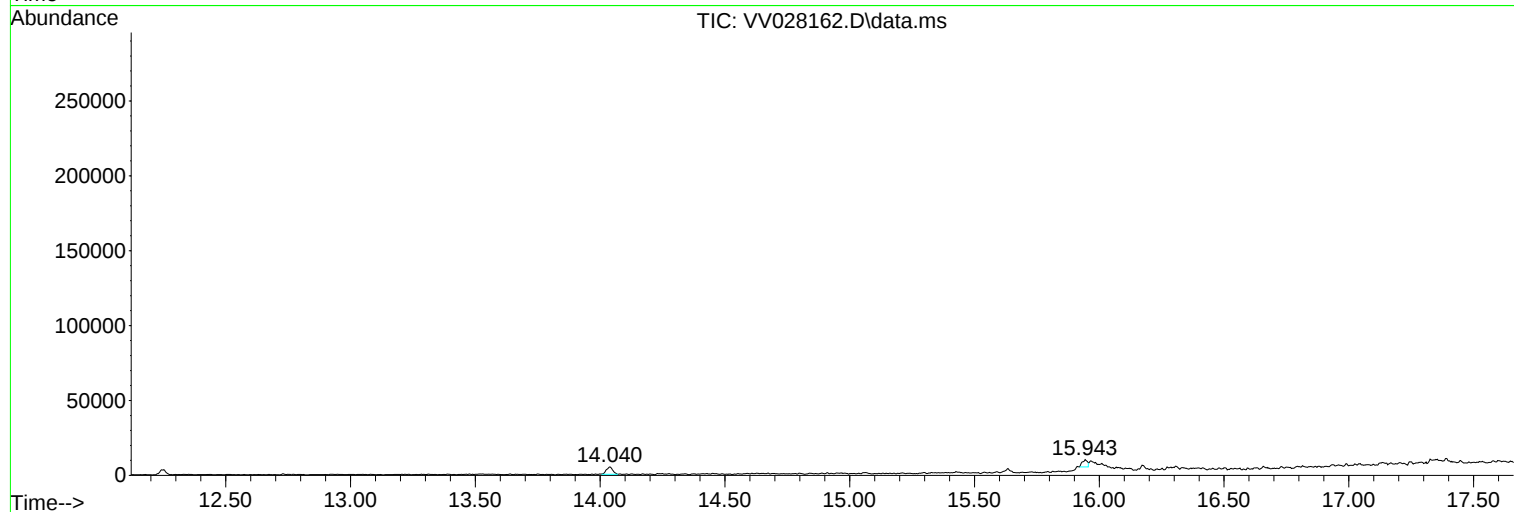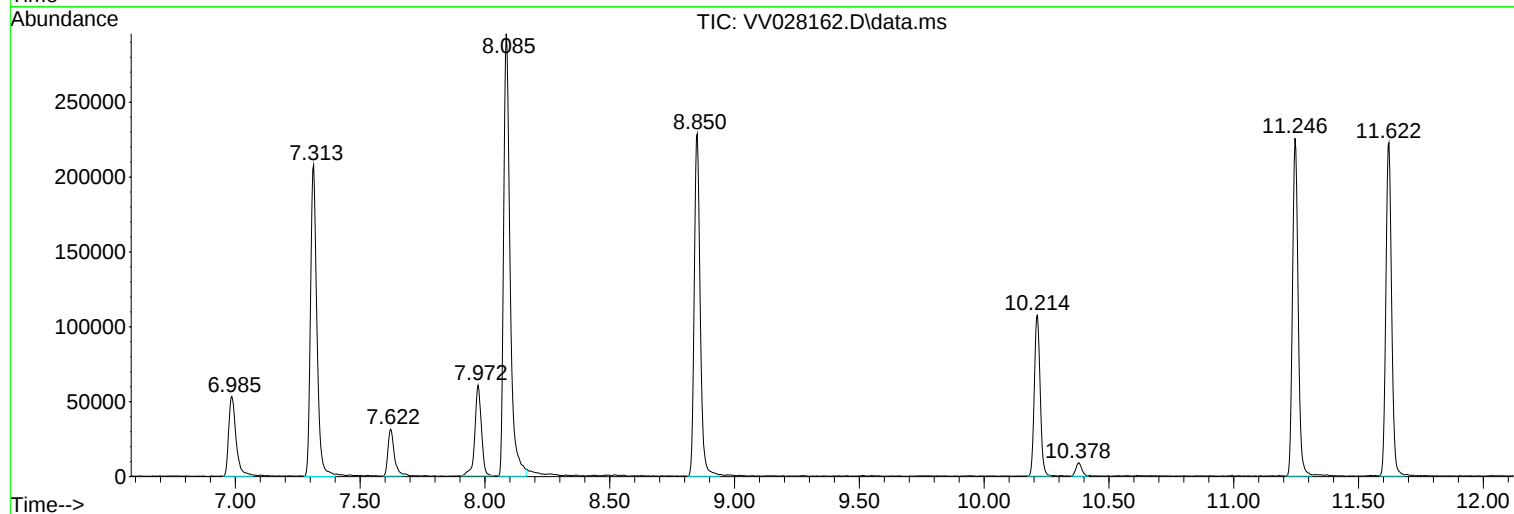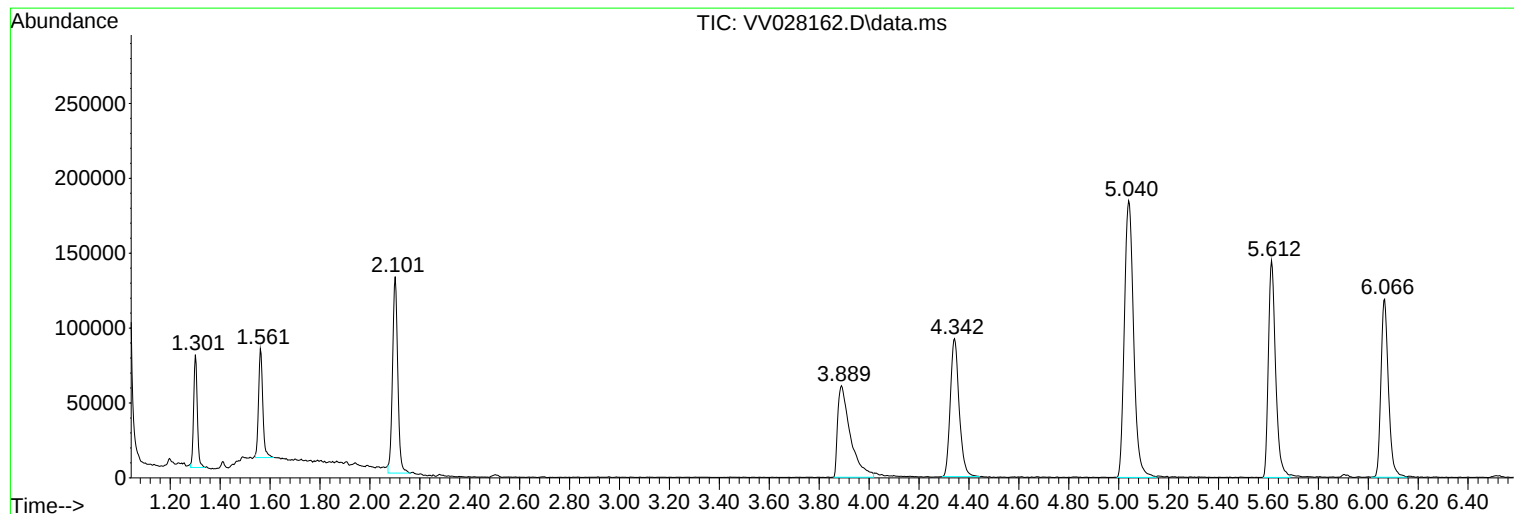

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028162.D
Acq On : 28 Sep 2022 16:27
Operator : SY/MD
Sample : N4871-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028162.D
Acq On : 28 Sep 2022 16:27
Operator : SY/MD
Sample : N4871-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc