

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
 Data File : VV028163.D
 Acq On : 28 Sep 2022 16:51
 Operator : SY/MD
 Sample : N4871-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H26

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	79779	83072	14.59%	1.619%
2	1.410	109	115	123	rVB2	7055	8431	1.48%	0.164%
3	1.561	154	162	173	rBV	76111	94813	16.65%	1.848%
4	2.101	321	330	344	rVB	133035	194540	34.16%	3.792%
5	3.892	876	887	922	rBV	71127	271292	47.64%	5.288%
6	4.342	1009	1027	1052	rBV	107907	272712	47.89%	5.316%
7	5.040	1228	1244	1267	rBV2	228016	569513	100.00%	11.101%
8	5.612	1410	1422	1450	rBV	172507	357469	62.77%	6.968%
9	6.066	1548	1563	1590	rBV	137624	285381	50.11%	5.562%
10	6.985	1839	1849	1871	rBV	56109	106127	18.63%	2.069%
11	7.313	1939	1951	1977	rBV	219672	389323	68.36%	7.588%
12	7.622	2038	2047	2062	rBV2	32842	59904	10.52%	1.168%
13	7.969	2133	2155	2177	rBV	308912	530640	93.17%	10.343%
14	8.085	2181	2191	2214	rBV	302470	548426	96.30%	10.690%
15	8.847	2418	2428	2450	rBV	253875	419962	73.74%	8.186%
16	10.214	2841	2853	2870	rBV	99505	158120	27.76%	3.082%
17	10.381	2895	2905	2914	rVB2	11579	18482	3.25%	0.360%
18	11.246	3163	3174	3194	rBV	239155	377810	66.34%	7.364%
19	11.622	3278	3291	3313	rBV	231526	371677	65.26%	7.245%
20	12.246	3475	3485	3495	rBV4	3613	5994	1.05%	0.117%
21	14.033	4035	4041	4051	rVB2	4388	6767	1.19%	0.132%




Sum of corrected areas: 5130455

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028163.D
Acq On : 28 Sep 2022 16:51
Operator : SY/MD
Sample : N4871-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

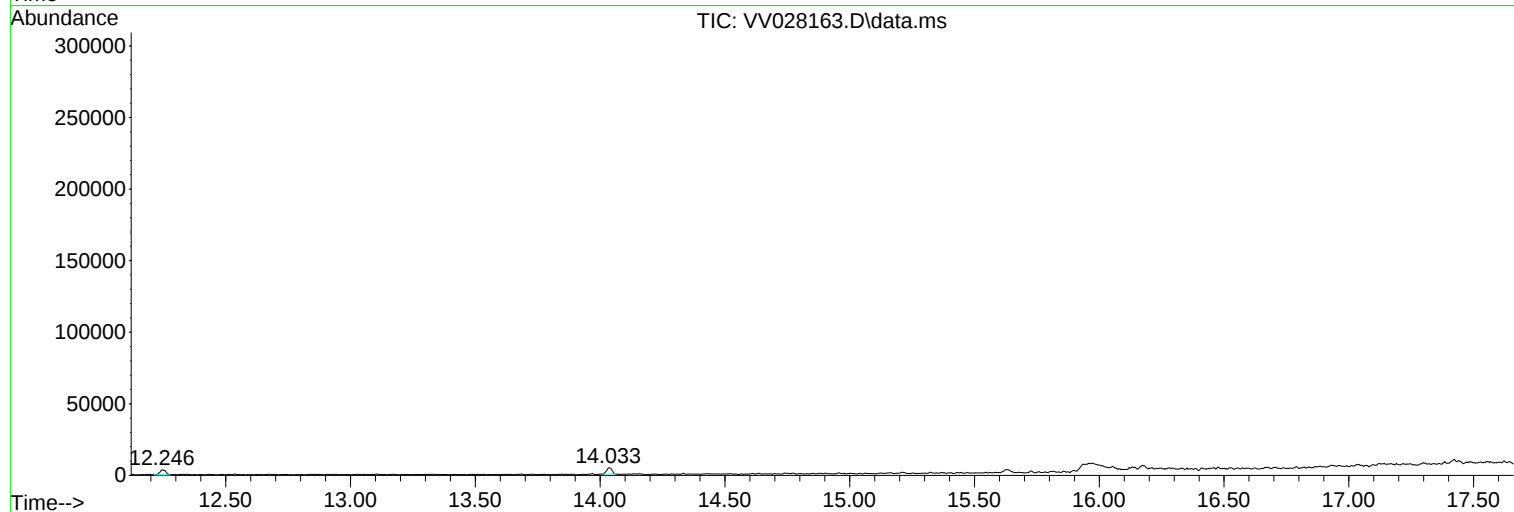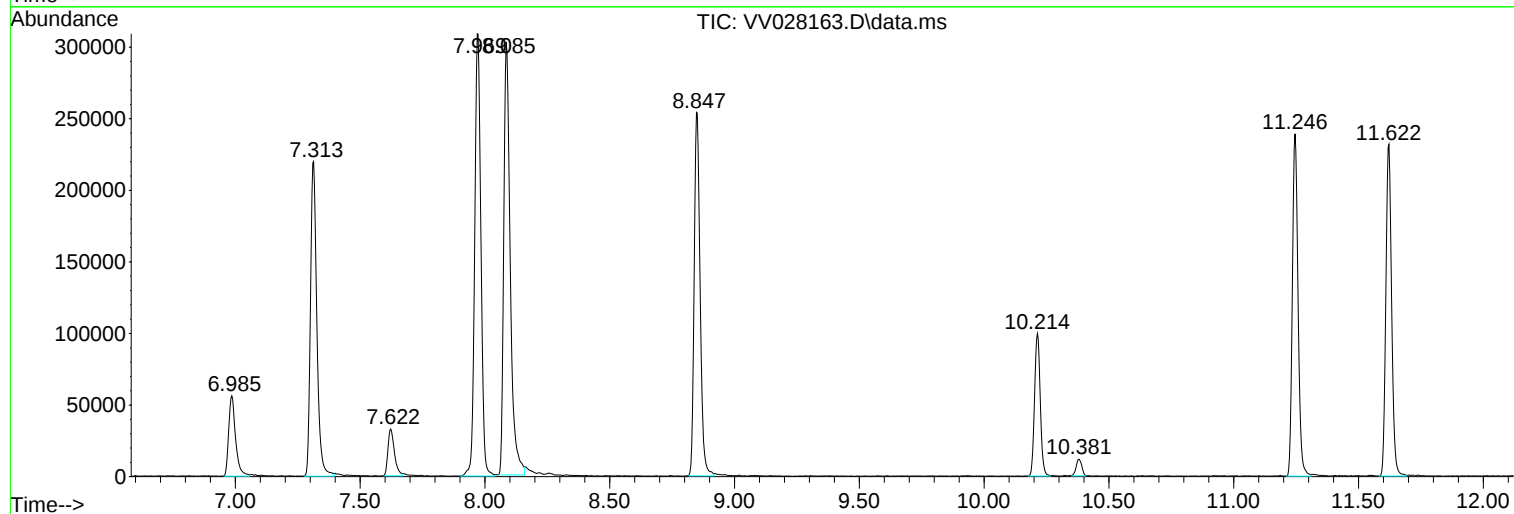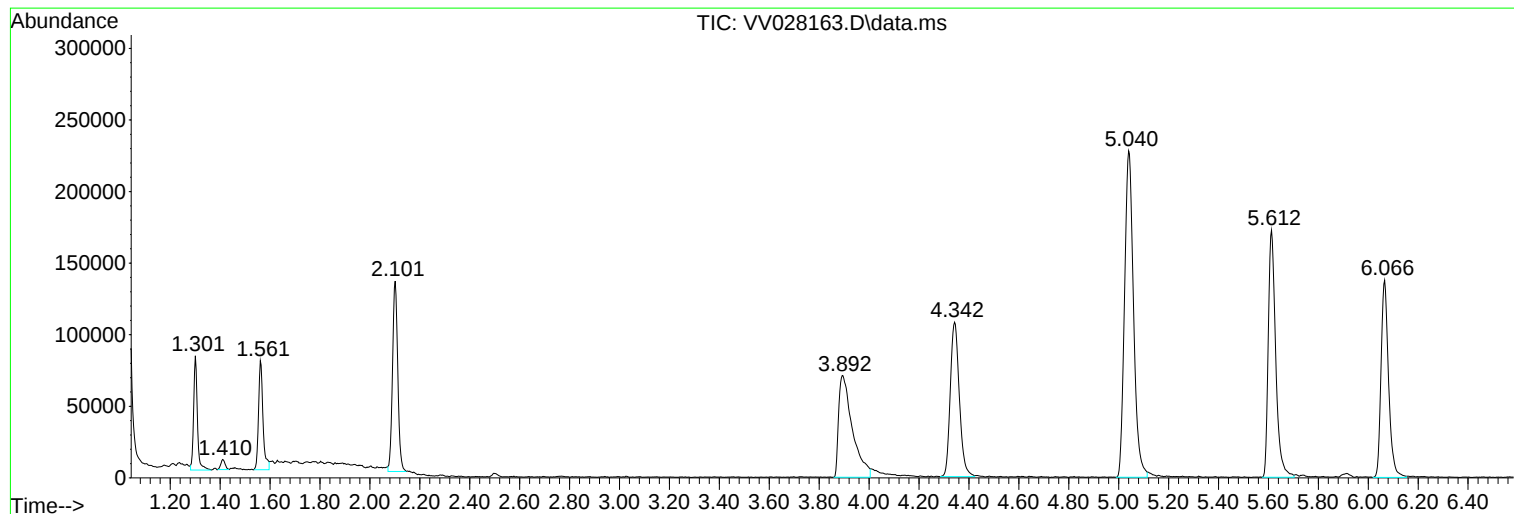

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028163.D
Acq On : 28 Sep 2022 16:51
Operator : SY/MD
Sample : N4871-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092822\
Data File : VV028163.D
Acq On : 28 Sep 2022 16:51
Operator : SY/MD
Sample : N4871-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc