
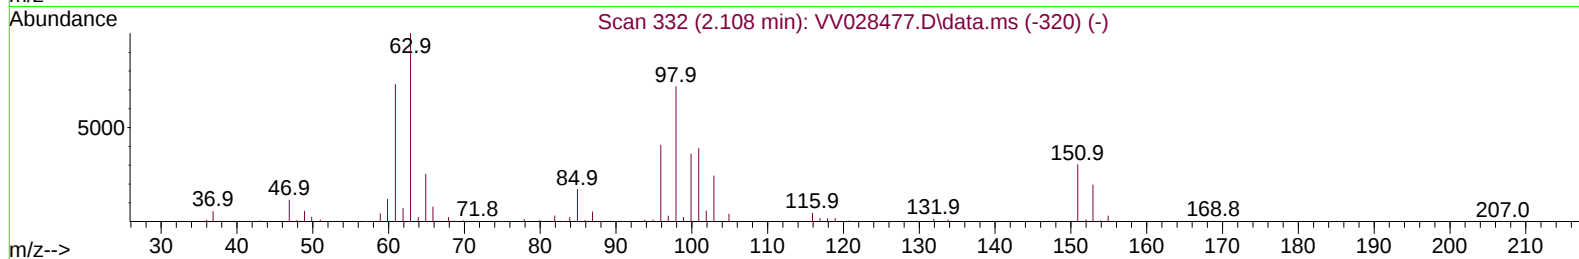
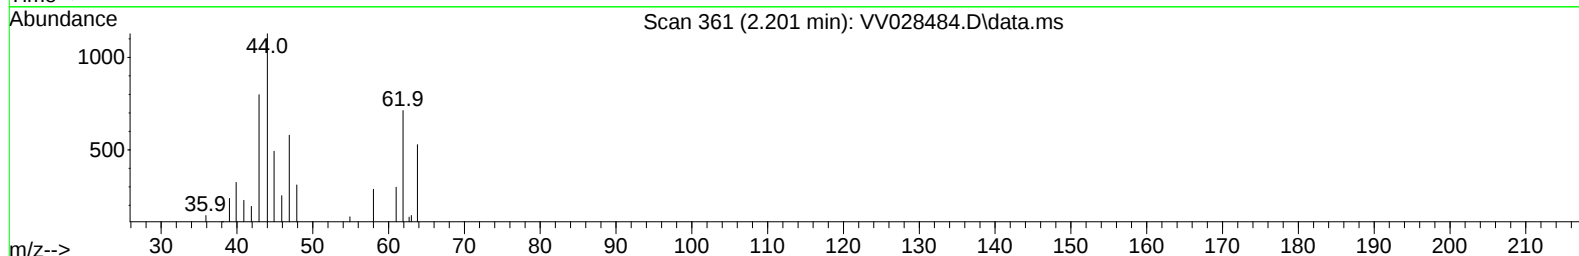


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028484.D
 Acq On : 09 Oct 2022 14:18
 Operator : SY/MD
 Sample : N4923-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Quant Time: Oct 10 05:27:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 10 05:21:45 2022
 Response via : Initial Calibration

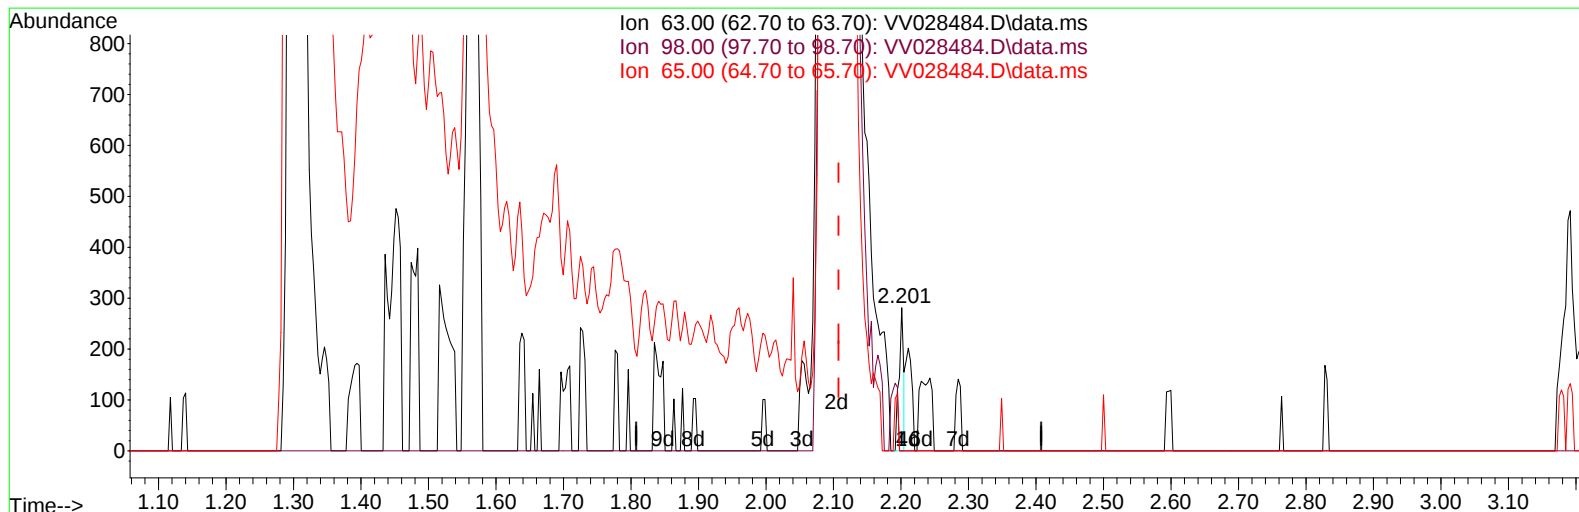

TIC: VV028484.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.201min (+ 0.093) 0.03 ug/L

response	135	
Ion	Exp%	Act%
63.00	100.00	100.00
98.00	70.50	68.89
65.00	24.00	30.37
0.00	0.00	0.00