

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028442.D
 Acq On : 08 Oct 2022 17:25
 Operator : SY/MD
 Sample : VV1008WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	145274	152003	11.57%	1.524%
2	1.564	156	163	176	rVB	116236	132449	10.08%	1.328%
3	2.105	321	331	349	rVB	239890	343891	26.17%	3.448%
4	2.899	571	578	581	rBV5	1106	1064	0.08%	0.011%
5	3.059	625	628	632	rBV4	601	503	0.04%	0.005%
6	3.082	632	635	639	rVB3	874	486	0.04%	0.005%
7	3.159	654	659	664	rBV5	911	1138	0.09%	0.011%
8	3.400	732	734	737	rBV4	537	319	0.02%	0.003%
9	3.571	785	787	792	rVB3	703	503	0.04%	0.005%
10	3.616	799	801	804	rBV3	294	185	0.01%	0.002%
11	3.693	823	825	826	rBV	338	166	0.01%	0.002%
12	3.744	839	841	843	rVB2	592	215	0.02%	0.002%
13	3.757	843	845	847	rBV2	501	212	0.02%	0.002%
14	3.899	879	889	916	rBV	65591	246535	18.76%	2.472%
15	4.342	1014	1027	1058	rVB	196042	500984	38.12%	5.024%
16	4.799	1167	1169	1172	rBV3	516	327	0.02%	0.003%
17	4.895	1197	1199	1204	rVB5	420	284	0.02%	0.003%
18	4.918	1204	1206	1209	rBV3	574	417	0.03%	0.004%
19	5.043	1227	1245	1278	rBV2	507548	1314262	100.00%	13.179%
20	5.612	1411	1422	1454	rBV	404138	826618	62.90%	8.289%
21	6.066	1550	1563	1589	rBV	285905	591044	44.97%	5.927%
22	6.323	1640	1643	1645	rBV2	528	317	0.02%	0.003%
23	6.355	1651	1653	1654	rBV	454	168	0.01%	0.002%
24	6.513	1699	1702	1704	rBV3	592	379	0.03%	0.004%
25	6.545	1709	1712	1715	rBV3	701	442	0.03%	0.004%
26	6.609	1729	1732	1733	rBV2	488	292	0.02%	0.003%
27	6.815	1793	1796	1801	rBV5	730	669	0.05%	0.007%
28	6.899	1820	1822	1826	rBV3	592	407	0.03%	0.004%
29	6.982	1838	1848	1882	rBV	177509	336427	25.60%	3.373%
30	7.310	1939	1950	1975	rBV	607070	1069688	81.39%	10.726%
31	7.619	2036	2046	2067	rBV	120223	219441	16.70%	2.200%
32	8.034	2172	2175	2180	rBV5	604	680	0.05%	0.007%
33	8.085	2181	2191	2225	rBV	335762	714638	54.38%	7.166%
34	8.529	2326	2329	2330	rBV	493	257	0.02%	0.003%
35	8.702	2381	2383	2385	rBV	404	226	0.02%	0.002%
36	8.847	2416	2428	2452	rBV	590020	977839	74.40%	9.805%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028442.D
 Acq On : 08 Oct 2022 17:25
 Operator : SY/MD
 Sample : VV1008WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	9.046	2488	2490	2494	rBV4	934	591	0.04%	0.006%
38	9.204	2532	2539	2543	rBV7	786	992	0.08%	0.010%
39	9.223	2543	2545	2552	rVB4	830	605	0.05%	0.006%
40	9.255	2552	2555	2557	rBV	730	429	0.03%	0.004%
41	9.297	2566	2568	2571	rVB3	563	243	0.02%	0.002%
42	9.333	2576	2579	2581	rBV3	802	468	0.04%	0.005%
43	9.403	2594	2601	2605	rVB4	505	607	0.05%	0.006%
44	9.426	2606	2608	2611	rVB3	523	266	0.02%	0.003%
45	9.452	2614	2616	2619	rBV2	387	209	0.02%	0.002%
46	9.474	2619	2623	2625	rBV3	766	546	0.04%	0.005%
47	9.490	2625	2628	2630	rBV2	425	212	0.02%	0.002%
48	9.802	2722	2725	2727	rBV2	366	236	0.02%	0.002%
49	9.866	2739	2745	2746	rBV4	914	812	0.06%	0.008%
50	9.931	2761	2765	2770	rBV5	785	773	0.06%	0.008%
51	10.075	2807	2810	2811	rBV3	547	287	0.02%	0.003%
52	10.210	2840	2852	2878	rBV	370967	601691	45.78%	6.033%
53	10.381	2903	2905	2908	rBV3	700	550	0.04%	0.006%
54	10.426	2916	2919	2920	rBV2	537	301	0.02%	0.003%
55	10.574	2962	2965	2967	rBV3	759	425	0.03%	0.004%
56	10.821	3032	3042	3043	rBV4	1105	1573	0.12%	0.016%
57	10.886	3054	3062	3064	rBV3	812	893	0.07%	0.009%
58	10.931	3072	3076	3078	rBV4	890	604	0.05%	0.006%
59	11.085	3121	3124	3127	rBV2	506	382	0.03%	0.004%
60	11.242	3161	3173	3197	rBV	619092	981014	74.64%	9.837%
61	11.551	3267	3269	3271	rBV	880	471	0.04%	0.005%
62	11.615	3277	3289	3311	rBV	588608	936096	71.23%	9.387%
63	11.828	3353	3355	3359	rVB3	803	386	0.03%	0.004%
64	11.847	3359	3361	3364	rVB2	613	399	0.03%	0.004%
65	11.863	3364	3366	3367	rBV2	341	135	0.01%	0.001%
66	11.988	3401	3405	3406	rBV3	787	500	0.04%	0.005%
67	12.130	3447	3449	3451	rBV2	420	186	0.01%	0.002%
68	12.143	3451	3453	3457	rVB3	482	363	0.03%	0.004%
69	12.181	3463	3465	3467	rBV2	608	312	0.02%	0.003%
70	12.291	3495	3499	3503	rBV4	676	599	0.05%	0.006%
71	12.374	3523	3525	3527	rBV2	604	306	0.02%	0.003%
72	12.403	3532	3534	3536	rBV3	463	212	0.02%	0.002%
73	12.574	3585	3587	3589	rBV2	456	193	0.01%	0.002%
74	12.869	3675	3679	3680	rBV	723	530	0.04%	0.005%
75	13.365	3828	3833	3835	rBV3	845	818	0.06%	0.008%
76	13.467	3863	3865	3868	rBV2	604	355	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028442.D
Acq On : 08 Oct 2022 17:25
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Title : VOC Analysis

77	13.895	3996	3998	4001	rBV3	631	291	0.02%	0.003%
78	15.024	4347	4349	4350	rBV2	919	407	0.03%	0.004%




Sum of corrected areas: 9972743

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028442.D
Acq On : 08 Oct 2022 17:25
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

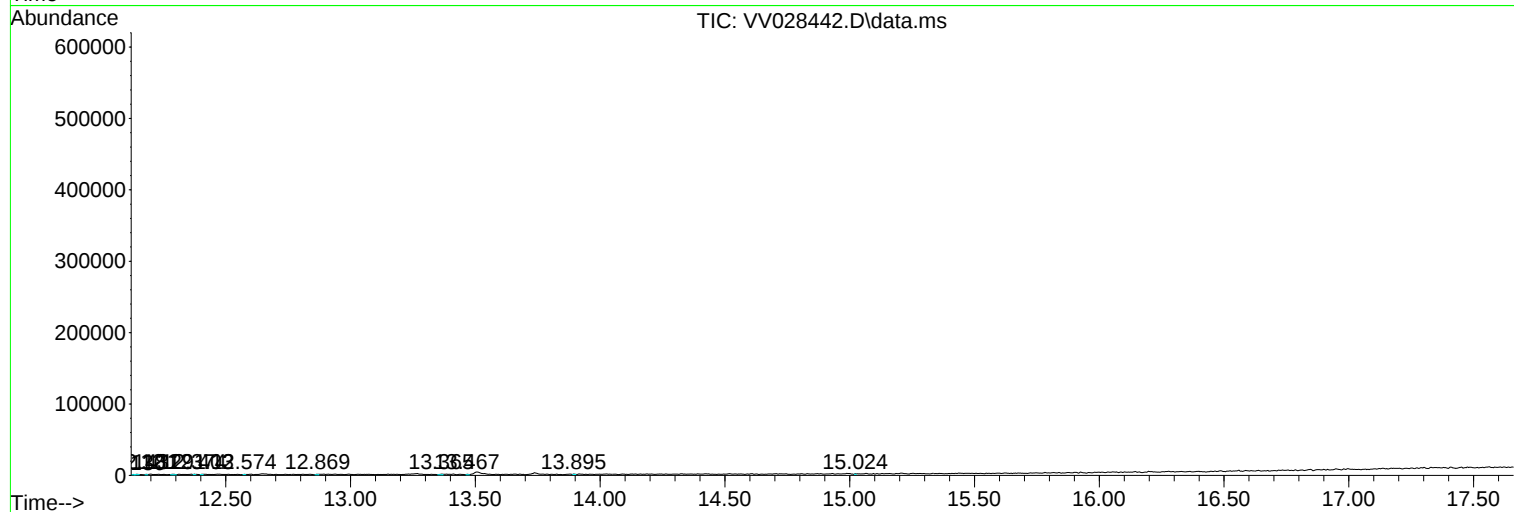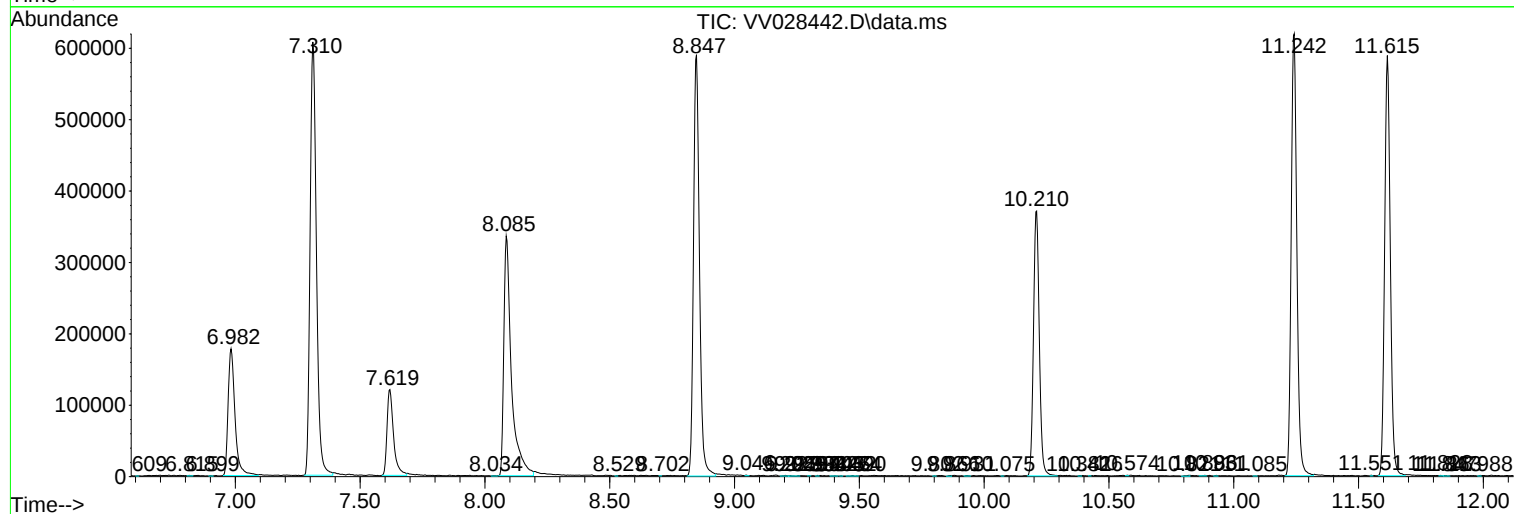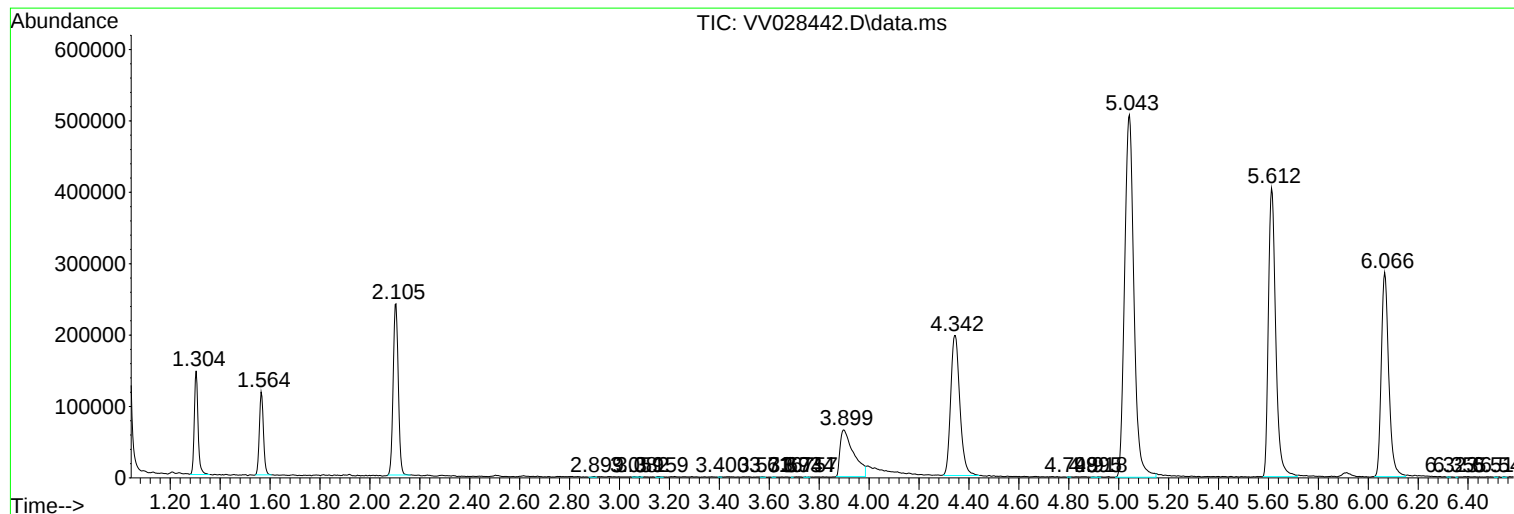

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028442.D
Acq On : 08 Oct 2022 17:25
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028442.D
Acq On : 08 Oct 2022 17:25
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc