

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028443.D
 Acq On : 08 Oct 2022 17:49
 Operator : SY/MD
 Sample : VV1008WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	196340	208167	14.60%	1.978%
2	1.564	156	163	174	rVB	145376	161226	11.31%	1.532%
3	2.105	320	331	350	rBV	363179	530932	37.24%	5.046%
4	2.503	449	455	465	rVB7	3391	5768	0.40%	0.055%
5	2.564	471	474	478	rBV3	685	638	0.04%	0.006%
6	2.593	481	483	485	rBV3	753	411	0.03%	0.004%
7	2.732	523	526	527	rBV2	353	171	0.01%	0.002%
8	2.844	559	561	563	rBV	371	223	0.02%	0.002%
9	2.886	571	574	575	rBV2	421	217	0.02%	0.002%
10	3.021	611	616	618	rBV4	758	735	0.05%	0.007%
11	3.166	659	661	664	rBV2	371	210	0.01%	0.002%
12	3.182	664	666	669	rVV3	664	255	0.02%	0.002%
13	3.404	733	735	739	rBV4	429	346	0.02%	0.003%
14	3.458	750	752	754	rBV3	570	289	0.02%	0.003%
15	3.523	770	772	775	rBV2	478	277	0.02%	0.003%
16	3.539	775	777	779	rBV	333	200	0.01%	0.002%
17	3.593	791	794	797	rBV2	883	479	0.03%	0.005%
18	3.699	824	827	829	rBV2	652	397	0.03%	0.004%
19	3.761	843	846	847	rBV	370	223	0.02%	0.002%
20	3.796	855	857	860	rBV3	383	281	0.02%	0.003%
21	3.847	869	873	874	rBV2	527	337	0.02%	0.003%
22	3.899	880	889	931	rBV	56101	275932	19.36%	2.622%
23	4.342	1013	1027	1061	rVB	210452	539821	37.87%	5.130%
24	4.838	1178	1181	1184	rBV4	650	428	0.03%	0.004%
25	4.908	1201	1203	1206	rBV2	681	325	0.02%	0.003%
26	5.040	1223	1244	1275	rBV2	550962	1425633	100.00%	13.549%
27	5.535	1396	1398	1400	rBV	1076	530	0.04%	0.005%
28	5.551	1400	1403	1406	rVB4	594	504	0.04%	0.005%
29	5.613	1406	1422	1448	rBV	386380	789904	55.41%	7.507%
30	5.873	1501	1503	1505	rBV2	784	326	0.02%	0.003%
31	5.908	1505	1514	1525	rBV9	5863	12795	0.90%	0.122%
32	6.063	1550	1562	1586	rBV	307341	634986	44.54%	6.035%
33	6.256	1620	1622	1627	rVB5	755	460	0.03%	0.004%
34	6.320	1638	1642	1643	rBV3	497	263	0.02%	0.002%
35	6.503	1695	1699	1703	rBV3	707	520	0.04%	0.005%
36	6.545	1708	1712	1713	rBV3	525	385	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028443.D
 Acq On : 08 Oct 2022 17:49
 Operator : SY/MD
 Sample : VV1008WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.616	1731	1734	1735	rBV	377	223	0.02%	0.002%
38	6.625	1735	1737	1739	rBV2	367	227	0.02%	0.002%
39	6.661	1745	1748	1749	rBV2	479	331	0.02%	0.003%
40	6.789	1786	1788	1791	rVV3	476	291	0.02%	0.003%
41	6.921	1827	1829	1833	rVB3	801	454	0.03%	0.004%
42	6.944	1833	1836	1837	rBV2	437	244	0.02%	0.002%
43	6.982	1837	1848	1877	rBV	193731	366039	25.68%	3.479%
44	7.310	1937	1950	1983	rBV	668187	1169569	82.04%	11.115%
45	7.616	2036	2045	2067	rBV	129178	236768	16.61%	2.250%
46	8.085	2182	2191	2230	rBV	319500	690629	48.44%	6.564%
47	8.503	2316	2321	2327	rVB	8306	6070	0.43%	0.058%
48	8.532	2327	2330	2333	rBV2	456	293	0.02%	0.003%
49	8.641	2362	2364	2366	rBV2	453	241	0.02%	0.002%
50	8.693	2375	2380	2384	rVB3	1190	1223	0.09%	0.012%
51	8.719	2384	2388	2391	rBV3	760	624	0.04%	0.006%
52	8.754	2396	2399	2402	rBV3	668	433	0.03%	0.004%
53	8.844	2416	2427	2457	rBV	554227	925096	64.89%	8.792%
54	9.101	2505	2507	2510	rBV2	785	468	0.03%	0.004%
55	9.288	2563	2565	2567	rBV2	630	306	0.02%	0.003%
56	9.310	2567	2572	2574	rBV4	732	690	0.05%	0.007%
57	9.378	2590	2593	2595	rBV	627	405	0.03%	0.004%
58	9.590	2658	2659	2662	rBV2	454	288	0.02%	0.003%
59	9.651	2674	2678	2683	rBV5	649	620	0.04%	0.006%
60	9.680	2685	2687	2689	rBV2	426	179	0.01%	0.002%
61	9.709	2694	2696	2703	rVB2	519	455	0.03%	0.004%
62	9.741	2703	2706	2710	rBV2	690	553	0.04%	0.005%
63	9.760	2710	2712	2713	rBV2	422	200	0.01%	0.002%
64	9.895	2751	2754	2757	rBV2	645	482	0.03%	0.005%
65	9.937	2765	2767	2768	rBV	563	236	0.02%	0.002%
66	9.960	2771	2774	2777	rBV3	815	521	0.04%	0.005%
67	10.018	2789	2792	2794	rBV2	395	229	0.02%	0.002%
68	10.040	2798	2799	2803	rBV2	568	262	0.02%	0.002%
69	10.146	2830	2832	2834	rBV	387	158	0.01%	0.002%
70	10.162	2835	2837	2839	rVB2	655	259	0.02%	0.002%
71	10.207	2839	2851	2874	rBV	385179	616354	43.23%	5.858%
72	10.407	2911	2913	2914	rBV	420	150	0.01%	0.001%
73	10.464	2929	2931	2934	rVB3	557	238	0.02%	0.002%
74	10.484	2934	2937	2939	rBV	425	347	0.02%	0.003%
75	10.542	2952	2955	2957	rVB3	547	324	0.02%	0.003%
76	10.567	2960	2963	2964	rBV3	606	383	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028443.D
 Acq On : 08 Oct 2022 17:49
 Operator : SY/MD
 Sample : VV1008WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.825	3042	3043	3046	rBV2	582	198	0.01%	0.002%
78	10.915	3069	3071	3072	rBV2	437	189	0.01%	0.002%
79	10.953	3081	3083	3085	rBV2	305	174	0.01%	0.002%
80	10.969	3085	3088	3091	rBV4	783	547	0.04%	0.005%
81	11.066	3116	3118	3121	rVB3	474	206	0.01%	0.002%
82	11.130	3135	3138	3141	rVB4	728	401	0.03%	0.004%
83	11.149	3141	3144	3145	rBV2	372	215	0.02%	0.002%
84	11.239	3160	3172	3194	rBV	584152	921566	64.64%	8.758%
85	11.500	3251	3253	3254	rBV	397	173	0.01%	0.002%
86	11.616	3277	3289	3311	rBV	621687	976530	68.50%	9.281%
87	11.988	3403	3405	3408	rVB2	526	191	0.01%	0.002%
88	12.165	3456	3460	3464	rVB4	465	454	0.03%	0.004%
89	12.326	3509	3510	3512	rBV2	372	186	0.01%	0.002%
90	12.400	3526	3533	3535	rBV3	822	862	0.06%	0.008%
91	12.622	3600	3602	3604	rBV3	353	165	0.01%	0.002%
92	12.635	3604	3606	3607	rBV3	508	202	0.01%	0.002%
93	12.644	3607	3609	3610	rBV2	466	185	0.01%	0.002%
94	12.866	3677	3678	3683	rVB4	566	304	0.02%	0.003%
95	12.911	3690	3692	3694	rVB3	691	230	0.02%	0.002%
96	12.969	3708	3710	3713	rVB	916	425	0.03%	0.004%
97	13.214	3783	3786	3790	rBV3	634	509	0.04%	0.005%
98	13.641	3916	3919	3920	rBV2	570	235	0.02%	0.002%
99	13.792	3965	3966	3969	rBV3	578	222	0.02%	0.002%
100	14.062	4048	4050	4051	rBV2	479	232	0.02%	0.002%




Sum of corrected areas: 10522057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028443.D
Acq On : 08 Oct 2022 17:49
Operator : SY/MD
Sample : VV1008WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

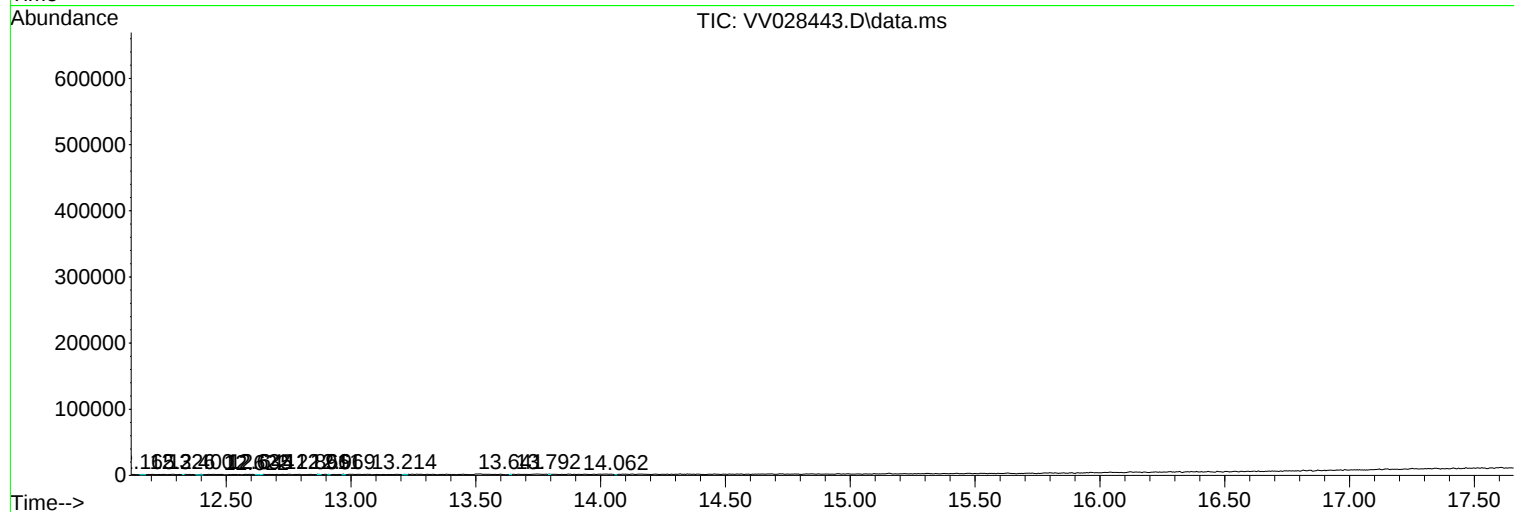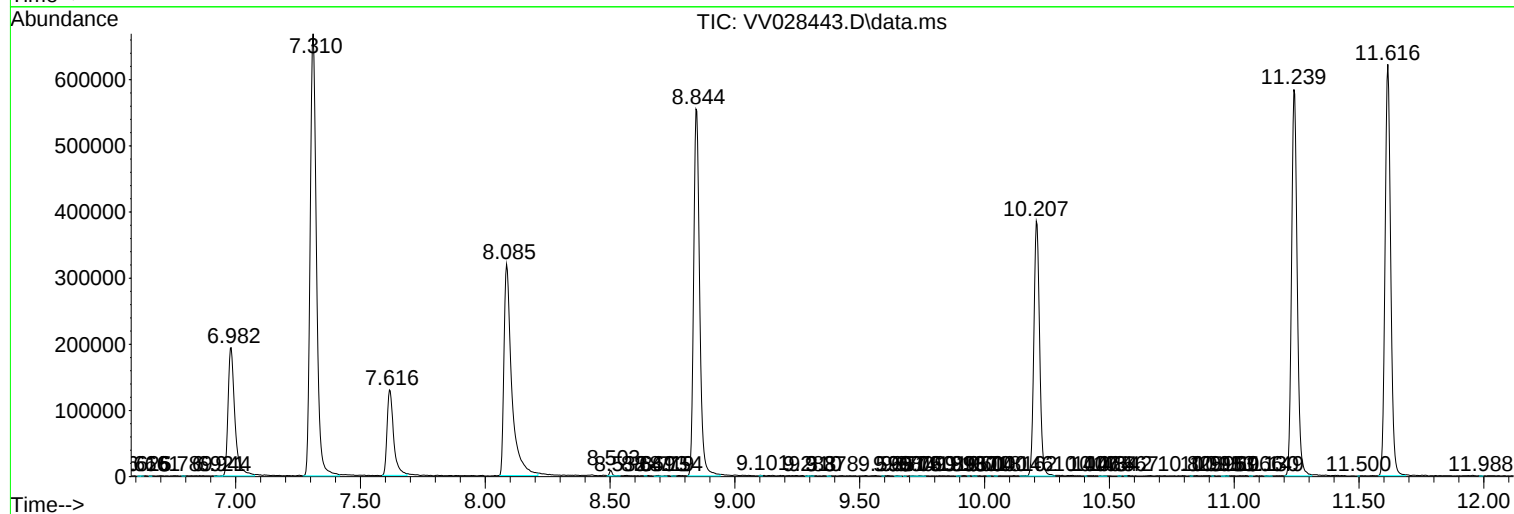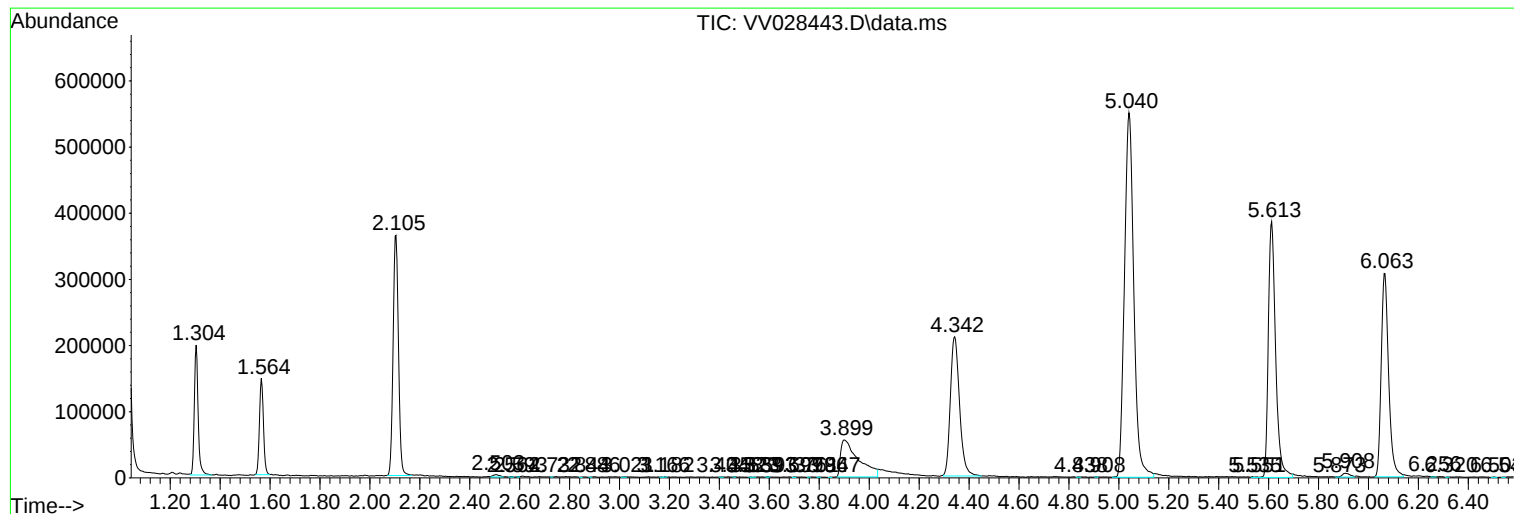

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028443.D
Acq On : 08 Oct 2022 17:49
Operator : SY/MD
Sample : VV1008WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028443.D
Acq On : 08 Oct 2022 17:49
Operator : SY/MD
Sample : VV1008WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc