

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028445.D
 Acq On : 08 Oct 2022 18:36
 Operator : SY/MD
 Sample : N4893-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	132802	141689	11.58%	1.470%
2	1.564	156	163	175	rVB	107274	121378	9.92%	1.260%
3	2.101	321	330	344	rVB	228213	322872	26.39%	3.351%
4	2.953	592	595	597	rBV2	800	467	0.04%	0.005%
5	3.114	643	645	647	rVB3	774	269	0.02%	0.003%
6	3.166	657	661	664	rBV3	428	421	0.03%	0.004%
7	3.326	709	711	715	rBV3	670	448	0.04%	0.005%
8	3.387	726	730	734	rVB3	743	807	0.07%	0.008%
9	3.426	734	742	744	rBV5	866	935	0.08%	0.010%
10	3.474	755	757	759	rBV2	364	226	0.02%	0.002%
11	3.516	768	770	773	rBV2	545	415	0.03%	0.004%
12	3.596	792	795	797	rBV3	649	303	0.02%	0.003%
13	3.680	816	821	824	rBV4	673	749	0.06%	0.008%
14	3.735	834	838	841	rBV5	629	508	0.04%	0.005%
15	3.767	845	848	852	rBV2	659	499	0.04%	0.005%
16	3.905	879	891	914	rBV2	52952	212214	17.35%	2.202%
17	4.342	1013	1027	1056	rVB	187751	471585	38.55%	4.894%
18	4.535	1085	1087	1089	rBV3	647	222	0.02%	0.002%
19	4.616	1110	1112	1115	rBV3	459	261	0.02%	0.003%
20	4.751	1149	1154	1155	rBV5	631	409	0.03%	0.004%
21	4.780	1160	1163	1165	rBV3	629	463	0.04%	0.005%
22	4.886	1192	1196	1199	rVB6	752	548	0.04%	0.006%
23	4.953	1215	1217	1218	rBV2	477	238	0.02%	0.002%
24	5.040	1229	1244	1275	rBV3	479052	1223245	100.00%	12.694%
25	5.313	1327	1329	1333	rVB4	768	415	0.03%	0.004%
26	5.571	1407	1409	1410	rBV	566	232	0.02%	0.002%
27	5.612	1411	1422	1453	rVV	382231	768891	62.86%	7.979%
28	5.908	1504	1514	1532	rBV	8085	19798	1.62%	0.205%
29	6.066	1549	1563	1593	rBV	269965	559477	45.74%	5.806%
30	6.391	1662	1664	1668	rBV4	634	433	0.04%	0.004%
31	6.773	1781	1783	1786	rBV	450	335	0.03%	0.003%
32	6.815	1794	1796	1801	rVB4	572	472	0.04%	0.005%
33	6.837	1801	1803	1807	rBV2	570	519	0.04%	0.005%
34	6.873	1812	1814	1817	rBV2	729	418	0.03%	0.004%
35	6.927	1828	1831	1834	rBV4	626	448	0.04%	0.005%
36	6.982	1837	1848	1873	rBV2	165746	310728	25.40%	3.225%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100822\
 Data File : VW028445.D
 Acq On : 08 Oct 2022 18:36
 Operator : SY/MD
 Sample : N4893-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.310	1938	1950	1973	rBV	566241	991958	81.09%	10.294%
38	7.619	2036	2046	2066	rBV	115127	206217	16.86%	2.140%
39	7.911	2135	2137	2139	rBV3	382	224	0.02%	0.002%
40	7.969	2143	2155	2173	rVV	253587	431601	35.28%	4.479%
41	8.088	2182	2192	2226	rBV	293740	622883	50.92%	6.464%
42	8.368	2276	2279	2284	rBV4	543	560	0.05%	0.006%
43	8.474	2308	2312	2314	rBV3	699	511	0.04%	0.005%
44	8.561	2336	2339	2341	rBV3	514	395	0.03%	0.004%
45	8.596	2347	2350	2353	rBV3	645	517	0.04%	0.005%
46	8.754	2395	2399	2402	rBV5	786	689	0.06%	0.007%
47	8.786	2407	2409	2411	rBV3	601	291	0.02%	0.003%
48	8.844	2416	2427	2450	rBV	531432	896159	73.26%	9.300%
49	9.117	2509	2512	2513	rBV2	472	328	0.03%	0.003%
50	9.172	2527	2529	2534	rBV4	544	478	0.04%	0.005%
51	9.265	2555	2558	2559	rBV	583	312	0.03%	0.003%
52	9.275	2559	2561	2567	rVB3	509	490	0.04%	0.005%
53	9.406	2598	2602	2605	rVB4	761	626	0.05%	0.006%
54	9.426	2605	2608	2613	rBV3	740	731	0.06%	0.008%
55	9.464	2618	2620	2622	rVB	583	245	0.02%	0.003%
56	9.513	2632	2635	2637	rVB	662	347	0.03%	0.004%
57	9.542	2641	2644	2645	rBV2	471	278	0.02%	0.003%
58	9.570	2651	2653	2656	rVB2	556	270	0.02%	0.003%
59	9.593	2656	2660	2664	rBV4	731	569	0.05%	0.006%
60	9.722	2695	2700	2702	rBV4	957	670	0.05%	0.007%
61	9.895	2752	2754	2756	rBV2	722	448	0.04%	0.005%
62	9.979	2777	2780	2784	rBV6	547	445	0.04%	0.005%
63	10.027	2793	2795	2796	rBV2	626	231	0.02%	0.002%
64	10.101	2816	2818	2821	rVB3	823	371	0.03%	0.004%
65	10.123	2821	2825	2827	rBV2	391	248	0.02%	0.003%
66	10.207	2840	2851	2870	rBV	345760	557790	45.60%	5.789%
67	10.320	2885	2886	2889	rBV2	486	299	0.02%	0.003%
68	10.432	2918	2921	2924	rBV2	543	408	0.03%	0.004%
69	10.487	2937	2938	2941	rBV2	773	360	0.03%	0.004%
70	10.561	2957	2961	2965	rBV4	797	801	0.07%	0.008%
71	10.699	3000	3004	3006	rBV3	456	409	0.03%	0.004%
72	10.828	3040	3044	3045	rBV2	327	235	0.02%	0.002%
73	10.898	3063	3066	3068	rBV3	564	380	0.03%	0.004%
74	11.175	3150	3152	3155	rVB2	1035	667	0.05%	0.007%
75	11.239	3155	3172	3196	rBV	560981	882886	72.18%	9.162%
76	11.535	3260	3264	3269	rBV6	661	766	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028445.D
 Acq On : 08 Oct 2022 18:36
 Operator : SY/MD
 Sample : N4893-11DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J10DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.615	3277	3289	3309	rBV	537983	859183	70.24%	8.916%
78	11.924	3382	3385	3387	rBV2	563	298	0.02%	0.003%
79	11.956	3391	3395	3397	rBV4	549	396	0.03%	0.004%
80	11.975	3399	3401	3403	rBV2	584	304	0.02%	0.003%
81	12.046	3419	3423	3425	rBV5	487	360	0.03%	0.004%
82	12.204	3470	3472	3478	rVB4	391	359	0.03%	0.004%
83	12.477	3555	3557	3560	rBV3	431	356	0.03%	0.004%
84	12.647	3607	3610	3612	rBV2	642	249	0.02%	0.003%
85	12.693	3621	3624	3629	rBV4	609	686	0.06%	0.007%
86	12.866	3676	3678	3680	rBV2	435	230	0.02%	0.002%
87	12.934	3696	3699	3701	rBV2	626	329	0.03%	0.003%
88	12.998	3715	3719	3721	rBV	436	321	0.03%	0.003%
89	13.165	3765	3771	3773	rBV3	622	651	0.05%	0.007%
90	13.287	3806	3809	3815	rBV5	637	571	0.05%	0.006%
91	13.319	3815	3819	3822	rBV3	641	476	0.04%	0.005%
92	13.429	3851	3853	3857	rVB5	673	412	0.03%	0.004%
93	13.493	3871	3873	3876	rBV2	534	385	0.03%	0.004%
94	13.593	3899	3904	3909	rBV6	663	760	0.06%	0.008%
95	13.786	3961	3964	3966	rBV3	658	372	0.03%	0.004%
96	14.123	4066	4069	4072	rBV2	915	519	0.04%	0.005%
97	14.252	4107	4109	4111	rBV3	565	235	0.02%	0.002%
98	14.313	4124	4128	4129	rBV2	668	424	0.03%	0.004%
99	14.454	4170	4172	4175	rBV2	684	342	0.03%	0.004%
100	14.554	4201	4203	4205	rBV2	737	383	0.03%	0.004%




Sum of corrected areas: 9636031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028445.D
Acq On : 08 Oct 2022 18:36
Operator : SY/MD
Sample : N4893-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

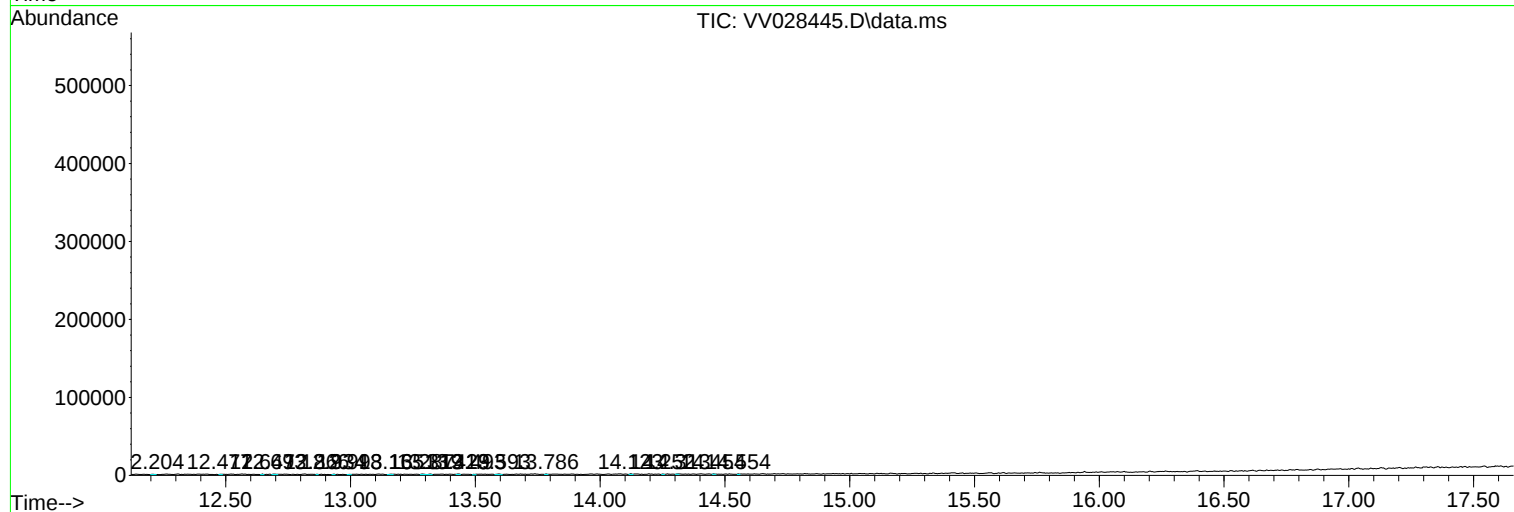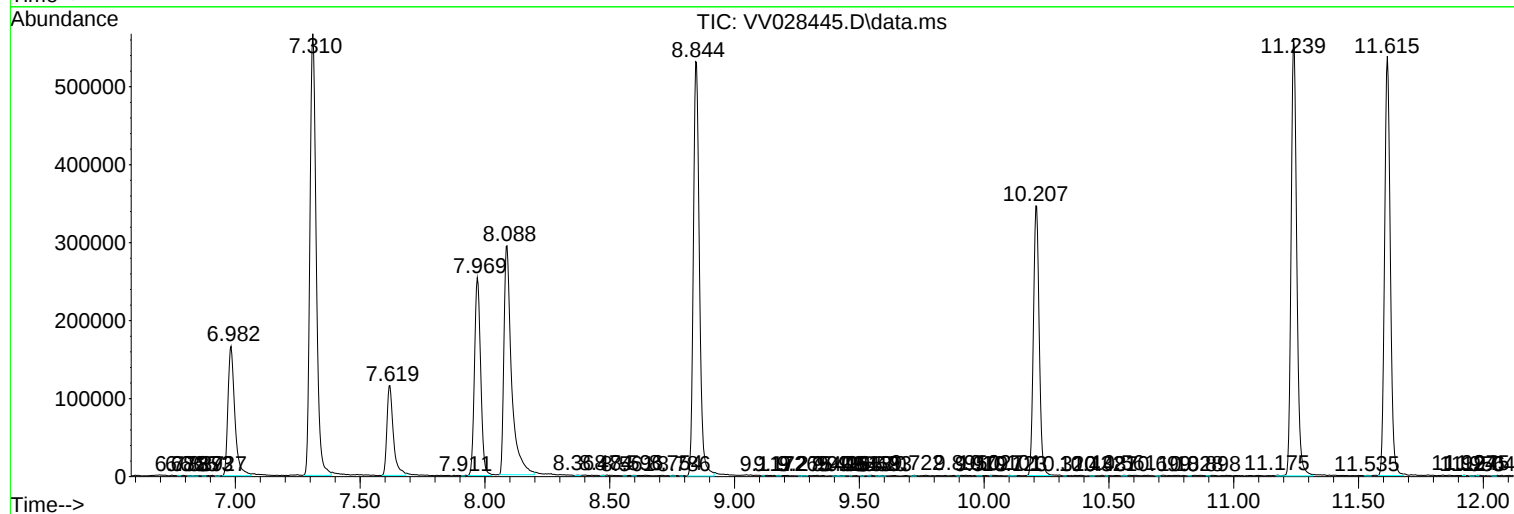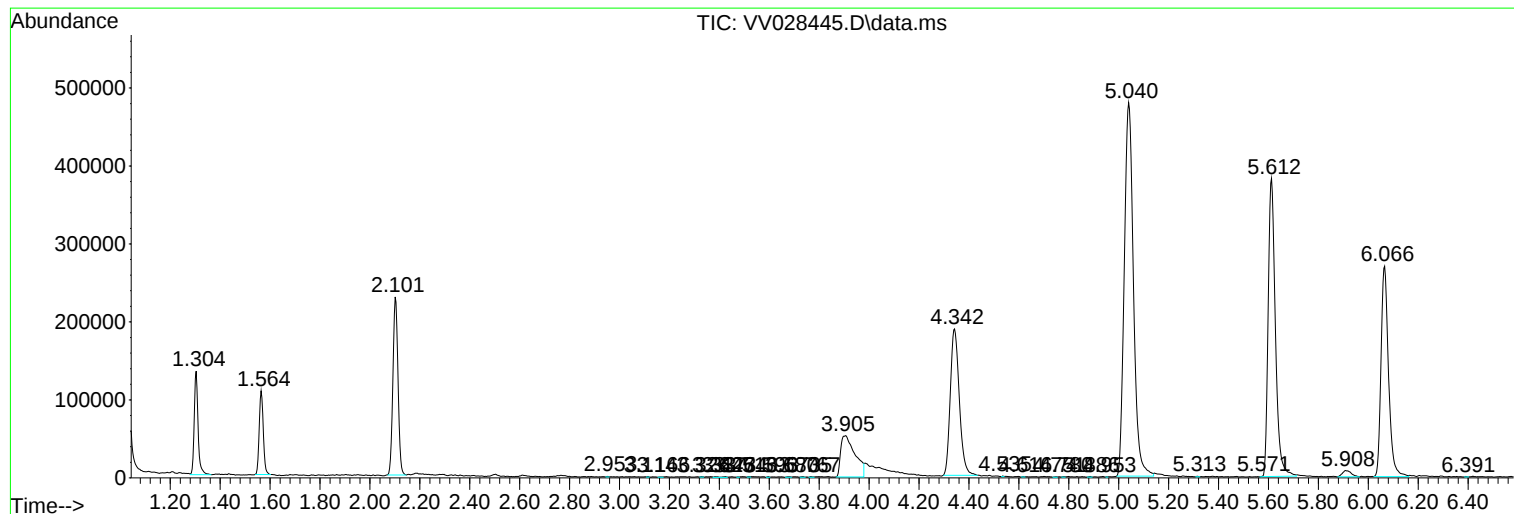

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028445.D
Acq On : 08 Oct 2022 18:36
Operator : SY/MD
Sample : N4893-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028445.D
Acq On : 08 Oct 2022 18:36
Operator : SY/MD
Sample : N4893-11DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J10DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc