

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028446.D
 Acq On : 08 Oct 2022 19:00
 Operator : SY/MD
 Sample : N4893-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	201753	212167	14.23%	2.009%
2	1.564	156	163	176	rVB	145556	166156	11.15%	1.574%
3	2.105	321	331	349	rVB	298639	432566	29.02%	4.097%
4	2.577	476	478	480	rBV2	556	186	0.01%	0.002%
5	2.773	537	539	540	rBV2	467	216	0.01%	0.002%
6	3.108	641	643	645	rVB	603	225	0.02%	0.002%
7	3.613	796	800	806	rBV4	593	787	0.05%	0.007%
8	3.754	843	844	846	rVB	542	168	0.01%	0.002%
9	3.780	849	852	856	rBV4	857	675	0.05%	0.006%
10	3.860	873	877	879	rBV3	529	404	0.03%	0.004%
11	3.902	879	890	931	rBV2	68616	318261	21.35%	3.014%
12	4.342	1012	1027	1055	rBV	221160	557223	37.38%	5.277%
13	4.706	1138	1140	1141	rBV	608	258	0.02%	0.002%
14	4.735	1146	1149	1151	rVB2	433	240	0.02%	0.002%
15	4.773	1159	1161	1165	rBV5	789	632	0.04%	0.006%
16	4.818	1173	1175	1177	rBV2	437	231	0.02%	0.002%
17	4.899	1192	1200	1204	rVB7	758	1047	0.07%	0.010%
18	5.040	1228	1244	1287	rBV2	582385	1490642	100.00%	14.117%
19	5.339	1333	1337	1341	rBV4	807	701	0.05%	0.007%
20	5.362	1341	1344	1345	rBV3	759	472	0.03%	0.004%
21	5.484	1380	1382	1386	rBV5	712	546	0.04%	0.005%
22	5.529	1393	1396	1397	rBV2	656	458	0.03%	0.004%
23	5.612	1410	1422	1458	rBV	361659	745477	50.01%	7.060%
24	5.908	1505	1514	1529	rVB6	6047	13104	0.88%	0.124%
25	6.063	1548	1562	1592	rBV	318169	661648	44.39%	6.266%
26	6.339	1642	1648	1651	rBV5	811	818	0.05%	0.008%
27	6.510	1697	1701	1705	rBV4	805	700	0.05%	0.007%
28	6.686	1754	1756	1758	rVB	478	246	0.02%	0.002%
29	6.699	1758	1760	1762	rBV2	452	173	0.01%	0.002%
30	6.860	1806	1810	1813	rBV3	599	493	0.03%	0.005%
31	6.905	1820	1824	1827	rBV4	709	598	0.04%	0.006%
32	6.928	1827	1831	1837	rVB6	553	598	0.04%	0.006%
33	6.982	1837	1848	1876	rBV	200657	378493	25.39%	3.584%
34	7.227	1923	1924	1926	rBV2	682	291	0.02%	0.003%
35	7.255	1931	1933	1938	rBV4	846	682	0.05%	0.006%
36	7.310	1938	1950	1979	rBV	679728	1195363	80.19%	11.320%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028446.D
 Acq On : 08 Oct 2022 19:00
 Operator : SY/MD
 Sample : N4893-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.616	2036	2045	2066	rBV	137315	241078	16.17%	2.283%
38	7.931	2137	2143	2144	rBV4	610	586	0.04%	0.006%
39	7.976	2155	2157	2160	rVB2	865	368	0.02%	0.003%
40	8.008	2165	2167	2168	rBV	595	209	0.01%	0.002%
41	8.085	2181	2191	2224	rBV	377453	756952	50.78%	7.169%
42	8.445	2301	2303	2305	rBV3	882	395	0.03%	0.004%
43	8.680	2373	2376	2379	rVB4	587	274	0.02%	0.003%
44	8.699	2379	2382	2384	rBV2	479	270	0.02%	0.003%
45	8.847	2416	2428	2461	rBV	518650	867314	58.18%	8.214%
46	9.082	2499	2501	2503	rVB2	1088	402	0.03%	0.004%
47	9.165	2523	2527	2531	rBV6	740	512	0.03%	0.005%
48	9.230	2545	2547	2550	rBV2	831	483	0.03%	0.005%
49	9.284	2562	2564	2567	rVB	526	215	0.01%	0.002%
50	9.304	2567	2570	2571	rBV	562	296	0.02%	0.003%
51	9.326	2575	2577	2580	rBV3	521	301	0.02%	0.003%
52	9.345	2580	2583	2589	rBV4	369	468	0.03%	0.004%
53	9.461	2616	2619	2621	rBV2	543	356	0.02%	0.003%
54	9.567	2649	2652	2657	rBV4	853	437	0.03%	0.004%
55	9.612	2664	2666	2669	rVB3	489	251	0.02%	0.002%
56	9.635	2669	2673	2675	rBV3	417	303	0.02%	0.003%
57	9.757	2707	2711	2712	rBV3	582	391	0.03%	0.004%
58	9.783	2716	2719	2721	rBV2	648	472	0.03%	0.004%
59	9.805	2724	2726	2728	rVB3	553	234	0.02%	0.002%
60	9.824	2729	2732	2735	rBV2	740	427	0.03%	0.004%
61	9.960	2771	2774	2777	rBV2	601	391	0.03%	0.004%
62	10.011	2789	2790	2794	rBV4	483	305	0.02%	0.003%
63	10.085	2810	2813	2816	rBV4	844	619	0.04%	0.006%
64	10.140	2825	2830	2834	rBV3	864	849	0.06%	0.008%
65	10.207	2840	2851	2872	rBV	406805	647817	43.46%	6.135%
66	10.361	2896	2899	2900	rBV2	648	277	0.02%	0.003%
67	10.381	2902	2905	2909	rVB5	617	510	0.03%	0.005%
68	10.419	2915	2917	2920	rBV	883	488	0.03%	0.005%
69	10.558	2953	2960	2962	rBV4	864	890	0.06%	0.008%
70	10.574	2962	2965	2967	rBV3	868	627	0.04%	0.006%
71	10.667	2991	2994	2997	rBV4	708	416	0.03%	0.004%
72	10.686	2997	3000	3001	rBV2	513	256	0.02%	0.002%
73	10.850	3045	3051	3055	rBV5	1124	1166	0.08%	0.011%
74	10.918	3064	3072	3074	rBV5	1073	1076	0.07%	0.010%
75	10.931	3074	3076	3078	rVV	368	182	0.01%	0.002%
76	11.017	3101	3103	3106	rVB2	531	250	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028446.D
 Acq On : 08 Oct 2022 19:00
 Operator : SY/MD
 Sample : N4893-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.062	3114	3117	3118	rBV2	347	199	0.01%	0.002%
78	11.178	3149	3153	3156	rBV2	448	410	0.03%	0.004%
79	11.239	3162	3172	3194	rBV	536324	847315	56.84%	8.024%
80	11.461	3238	3241	3242	rBV	566	319	0.02%	0.003%
81	11.615	3277	3289	3312	rBV	629228	992231	66.56%	9.397%
82	11.818	3350	3352	3353	rBV2	607	314	0.02%	0.003%
83	11.924	3383	3385	3387	rBV3	325	193	0.01%	0.002%
84	12.043	3420	3422	3425	rBV2	426	293	0.02%	0.003%
85	12.217	3474	3476	3479	rBV3	505	333	0.02%	0.003%
86	12.590	3589	3592	3594	rBV3	517	372	0.02%	0.004%
87	12.786	3650	3653	3655	rVB3	823	445	0.03%	0.004%
88	12.840	3668	3670	3672	rVB3	517	199	0.01%	0.002%
89	12.895	3685	3687	3690	rBV2	534	250	0.02%	0.002%
90	13.049	3733	3735	3740	rVB4	500	293	0.02%	0.003%
91	13.210	3782	3785	3787	rVB2	858	448	0.03%	0.004%
92	13.230	3787	3791	3792	rBV2	588	396	0.03%	0.004%
93	13.606	3906	3908	3912	rVB3	515	245	0.02%	0.002%
94	13.657	3922	3924	3927	rBV4	554	428	0.03%	0.004%
95	13.754	3951	3954	3956	rBV2	807	515	0.03%	0.005%
96	14.223	4097	4100	4101	rBV2	616	404	0.03%	0.004%
97	14.355	4139	4141	4143	rBV3	512	279	0.02%	0.003%
98	14.393	4152	4153	4156	rBV2	535	346	0.02%	0.003%
99	14.734	4257	4259	4260	rBV	670	290	0.02%	0.003%
100	14.991	4335	4339	4341	rBV4	814	710	0.05%	0.007%




Sum of corrected areas: 10559285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028446.D
Acq On : 08 Oct 2022 19:00
Operator : SY/MD
Sample : N4893-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

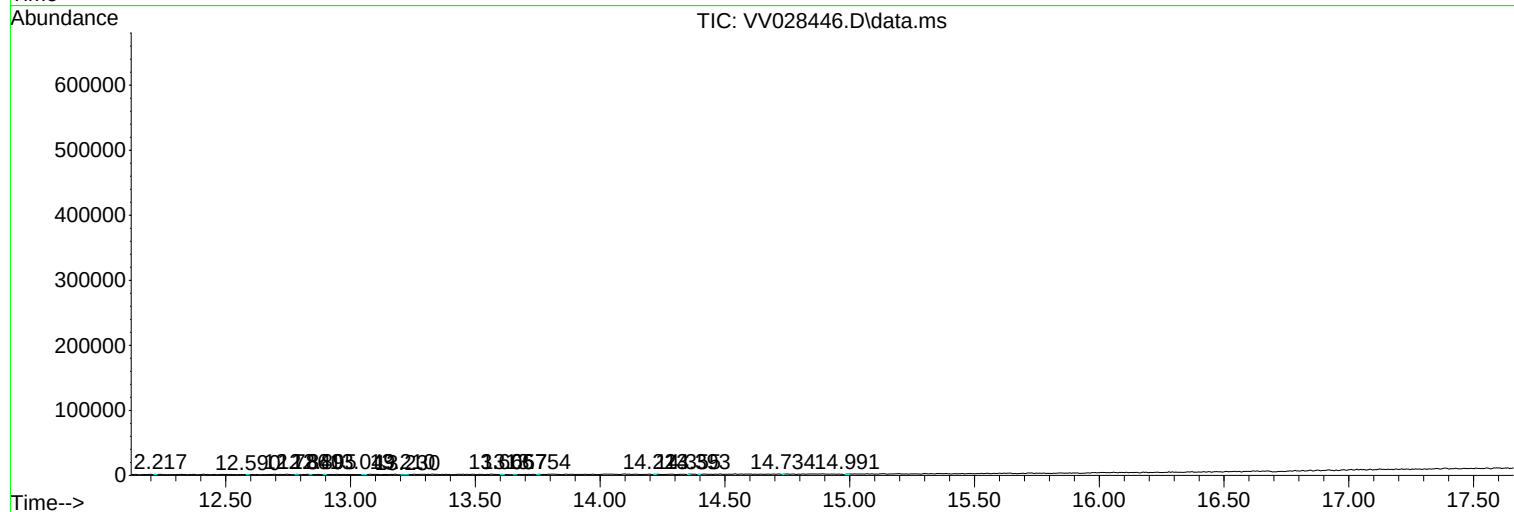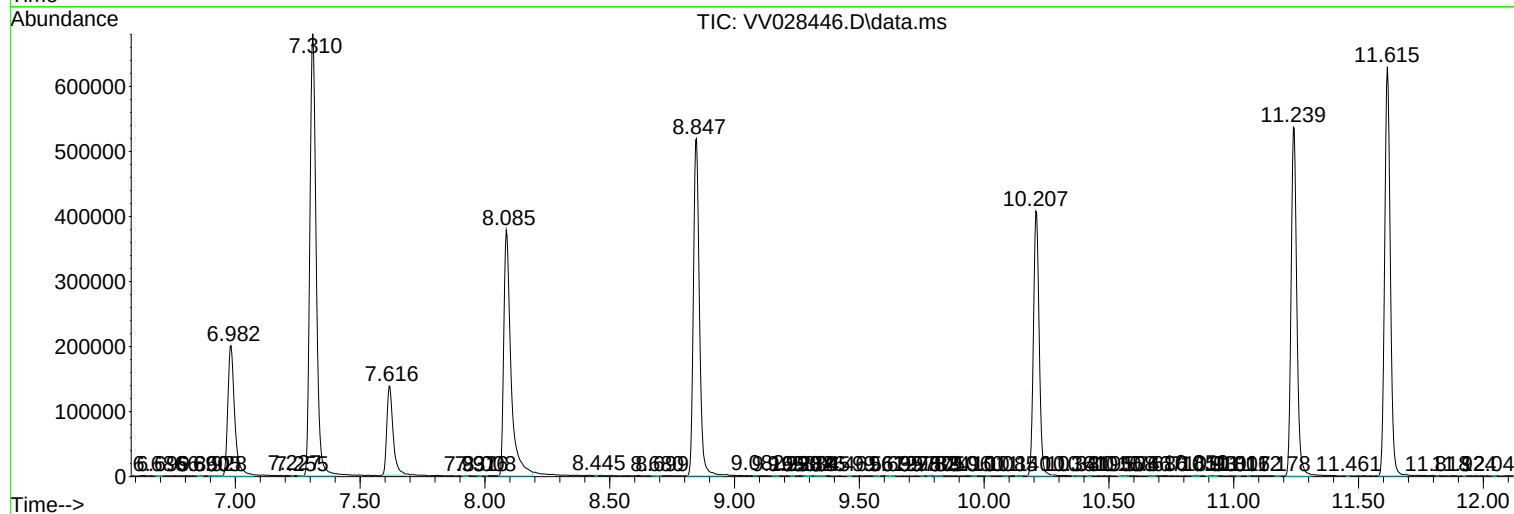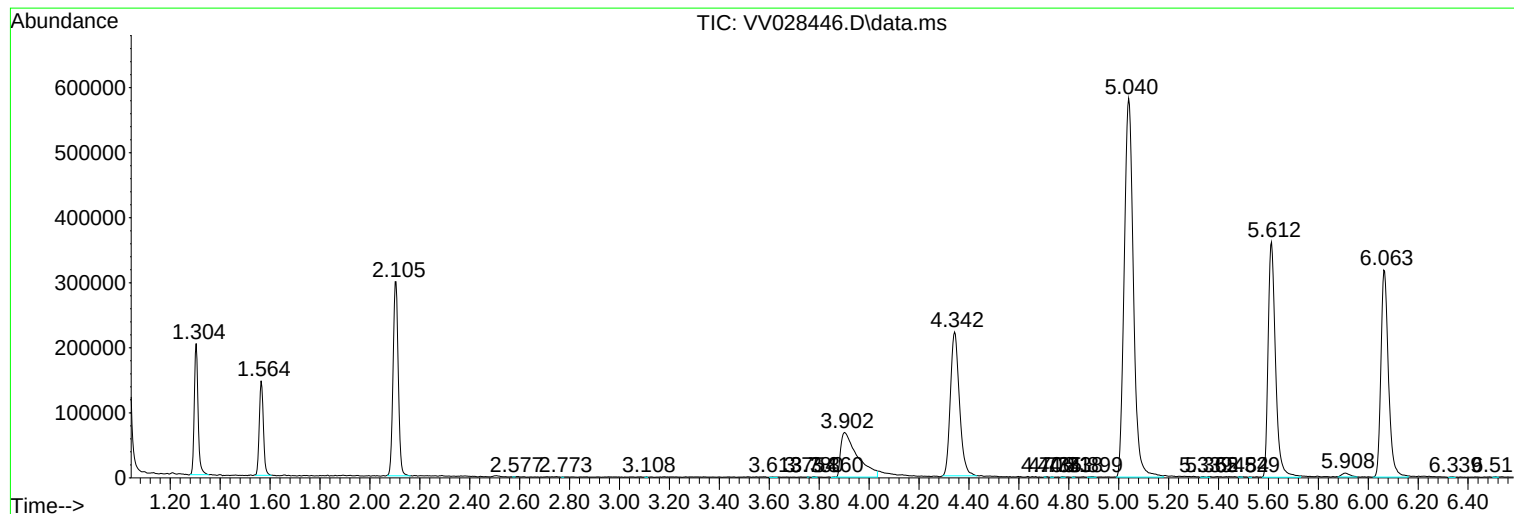

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028446.D
Acq On : 08 Oct 2022 19:00
Operator : SY/MD
Sample : N4893-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028446.D
Acq On : 08 Oct 2022 19:00
Operator : SY/MD
Sample : N4893-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc