

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028450.D
 Acq On : 08 Oct 2022 20:37
 Operator : SY/MD
 Sample : N4889-05DL 2000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ63DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	135074	146637	5.99%	1.220%
2	1.564	156	163	177	rBV	108573	126164	5.15%	1.050%
3	2.105	321	331	351	rVB	224917	326656	13.34%	2.719%
4	2.552	468	470	475	rBV4	597	457	0.02%	0.004%
5	3.249	683	687	690	rBV3	613	452	0.02%	0.004%
6	3.333	709	713	715	rBV4	489	409	0.02%	0.003%
7	3.388	726	730	734	rBV4	662	623	0.03%	0.005%
8	3.420	738	740	744	rBV2	502	281	0.01%	0.002%
9	3.474	754	757	759	rBV3	450	299	0.01%	0.002%
10	3.510	766	768	771	rBV3	847	550	0.02%	0.005%
11	3.568	783	786	790	rVV4	431	351	0.01%	0.003%
12	3.587	790	792	796	rVB	506	349	0.01%	0.003%
13	3.732	835	837	841	rBV4	494	406	0.02%	0.003%
14	3.896	878	888	926	rBV2	63084	266175	10.87%	2.215%
15	4.343	1015	1027	1057	rVB	188710	470164	19.20%	3.913%
16	4.867	1188	1190	1193	rBV4	357	301	0.01%	0.003%
17	4.896	1196	1199	1202	rBV4	754	587	0.02%	0.005%
18	4.973	1219	1223	1226	rBV2	619	497	0.02%	0.004%
19	5.040	1227	1244	1275	rBV2	478870	1235456	50.45%	10.283%
20	5.365	1343	1345	1348	rBV2	692	369	0.02%	0.003%
21	5.532	1393	1397	1399	rBV3	604	484	0.02%	0.004%
22	5.613	1410	1422	1450	rVV	375910	757792	30.95%	6.307%
23	5.870	1498	1502	1503	rBV3	424	260	0.01%	0.002%
24	5.908	1504	1514	1532	rVB9	5871	12951	0.53%	0.108%
25	5.986	1534	1538	1541	rBV3	641	598	0.02%	0.005%
26	6.063	1548	1562	1596	rBV	266250	568312	23.21%	4.730%
27	6.481	1688	1692	1694	rBV4	787	592	0.02%	0.005%
28	6.661	1744	1748	1749	rBV3	501	313	0.01%	0.003%
29	6.670	1749	1751	1753	rVV3	670	377	0.02%	0.003%
30	6.693	1756	1758	1761	rBV2	589	357	0.01%	0.003%
31	6.719	1764	1766	1770	rBV4	529	345	0.01%	0.003%
32	6.793	1785	1789	1792	rBV3	654	433	0.02%	0.004%
33	6.847	1799	1806	1807	rBV4	789	683	0.03%	0.006%
34	6.982	1836	1848	1877	rBV	162871	311548	12.72%	2.593%
35	7.310	1939	1950	1962	rBV	579412	994795	40.62%	8.280%
36	7.381	1962	1972	2003	rVB	1430019	2448762	100.00%	20.382%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028450.D
 Acq On : 08 Oct 2022 20:37
 Operator : SY/MD
 Sample : N4889-05DL 2000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ63DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.619	2037	2046	2071	rBV	111318	194856	7.96%	1.622%
38	7.905	2133	2135	2140	rVB3	905	643	0.03%	0.005%
39	8.005	2164	2166	2168	rBV2	652	340	0.01%	0.003%
40	8.034	2173	2175	2176	rBV2	596	265	0.01%	0.002%
41	8.085	2182	2191	2231	rBV	304069	646806	26.41%	5.383%
42	8.352	2272	2274	2276	rBV3	672	325	0.01%	0.003%
43	8.503	2319	2321	2324	rBV	605	351	0.01%	0.003%
44	8.538	2328	2332	2335	rVB3	684	561	0.02%	0.005%
45	8.555	2335	2337	2340	rBV4	586	435	0.02%	0.004%
46	8.584	2340	2346	2350	rVB5	820	950	0.04%	0.008%
47	8.606	2350	2353	2356	rBV3	551	454	0.02%	0.004%
48	8.654	2366	2368	2372	rBV4	658	424	0.02%	0.004%
49	8.844	2414	2427	2445	rBV	530101	879475	35.92%	7.320%
50	9.011	2470	2479	2494	rBV	33228	55302	2.26%	0.460%
51	9.130	2506	2516	2539	rBV	109676	186011	7.60%	1.548%
52	9.288	2562	2565	2569	rVB2	773	492	0.02%	0.004%
53	9.439	2610	2612	2615	rVB3	684	335	0.01%	0.003%
54	9.538	2632	2643	2662	rBV2	36616	64226	2.62%	0.535%
55	9.657	2678	2680	2686	rVB5	936	749	0.03%	0.006%
56	9.683	2686	2688	2691	rBV3	698	603	0.02%	0.005%
57	9.895	2751	2754	2755	rBV2	479	260	0.01%	0.002%
58	9.908	2755	2758	2760	rBV3	515	366	0.01%	0.003%
59	10.075	2807	2810	2812	rBV3	528	414	0.02%	0.003%
60	10.120	2820	2824	2828	rBV4	820	547	0.02%	0.005%
61	10.156	2832	2835	2836	rBV2	492	255	0.01%	0.002%
62	10.207	2840	2851	2878	rVV	348853	559659	22.85%	4.658%
63	10.352	2894	2896	2902	rBV6	611	639	0.03%	0.005%
64	10.445	2917	2925	2930	rBV7	2088	3205	0.13%	0.027%
65	10.500	2940	2942	2945	rVB3	847	381	0.02%	0.003%
66	10.632	2980	2983	2986	rBV3	746	387	0.02%	0.003%
67	10.648	2986	2988	2995	rVB3	748	557	0.02%	0.005%
68	10.683	2995	2999	3001	rBV5	1083	953	0.04%	0.008%
69	10.911	3061	3070	3080	rBV4	4744	7935	0.32%	0.066%
70	10.950	3080	3082	3086	rVB2	483	287	0.01%	0.002%
71	11.027	3099	3106	3107	rBV4	508	497	0.02%	0.004%
72	11.056	3113	3115	3117	rVB3	572	277	0.01%	0.002%
73	11.095	3125	3127	3133	rVB4	1058	731	0.03%	0.006%
74	11.165	3146	3149	3155	rBV3	819	840	0.03%	0.007%
75	11.194	3155	3158	3160	rBV3	480	315	0.01%	0.003%
76	11.239	3160	3172	3193	rBV	553683	866405	35.38%	7.211%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028450.D
 Acq On : 08 Oct 2022 20:37
 Operator : SY/MD
 Sample : N4889-05DL 2000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ63DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.419	3225	3228	3230	rBV4	556	344	0.01%	0.003%
78	11.526	3257	3261	3263	rBV2	721	527	0.02%	0.004%
79	11.616	3277	3289	3311	rBV	530901	849943	34.71%	7.074%
80	11.783	3337	3341	3345	rVB3	686	536	0.02%	0.004%
81	11.805	3345	3348	3351	rBV3	753	553	0.02%	0.005%
82	11.831	3354	3356	3360	rVB4	864	521	0.02%	0.004%
83	11.863	3363	3366	3371	rVB3	624	464	0.02%	0.004%
84	11.931	3382	3387	3389	rBV3	529	506	0.02%	0.004%
85	12.075	3430	3432	3435	rVB4	775	338	0.01%	0.003%
86	12.114	3441	3444	3448	rBV3	810	659	0.03%	0.005%
87	12.255	3485	3488	3494	rBV5	604	731	0.03%	0.006%
88	12.577	3586	3588	3591	rVB2	706	302	0.01%	0.003%
89	12.612	3598	3599	3602	rVB2	672	261	0.01%	0.002%
90	12.870	3676	3679	3683	rBV5	1117	1116	0.05%	0.009%
91	12.956	3704	3706	3709	rVB2	621	350	0.01%	0.003%
92	12.982	3712	3714	3717	rBV2	410	281	0.01%	0.002%
93	13.181	3773	3776	3779	rBV2	520	297	0.01%	0.002%
94	13.326	3817	3821	3826	rBV2	653	729	0.03%	0.006%
95	13.506	3875	3877	3879	rBV3	598	330	0.01%	0.003%
96	13.635	3914	3917	3919	rBV2	526	276	0.01%	0.002%
97	13.648	3919	3921	3924	rBV3	479	269	0.01%	0.002%
98	13.792	3964	3966	3970	rBV3	522	393	0.02%	0.003%
99	14.731	4256	4258	4259	rBV3	651	326	0.01%	0.003%
100	14.992	4337	4339	4340	rBV	661	261	0.01%	0.002%




Sum of corrected areas: 12014611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028450.D
Acq On : 08 Oct 2022 20:37
Operator : SY/MD
Sample : N4889-05DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ63DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

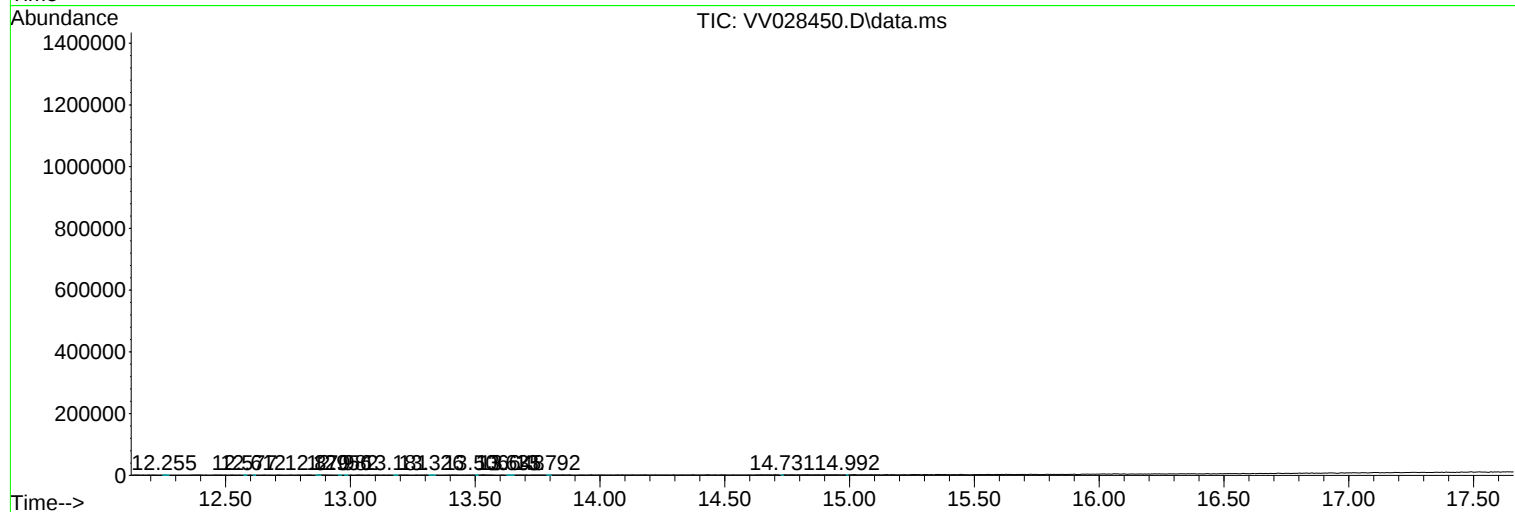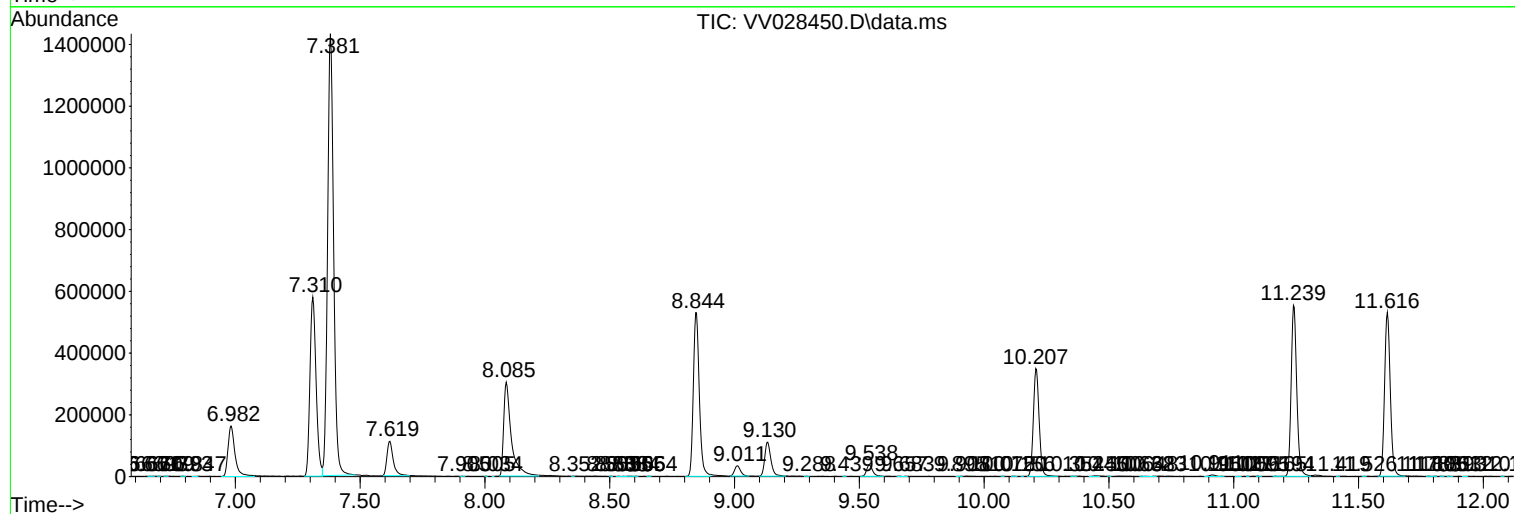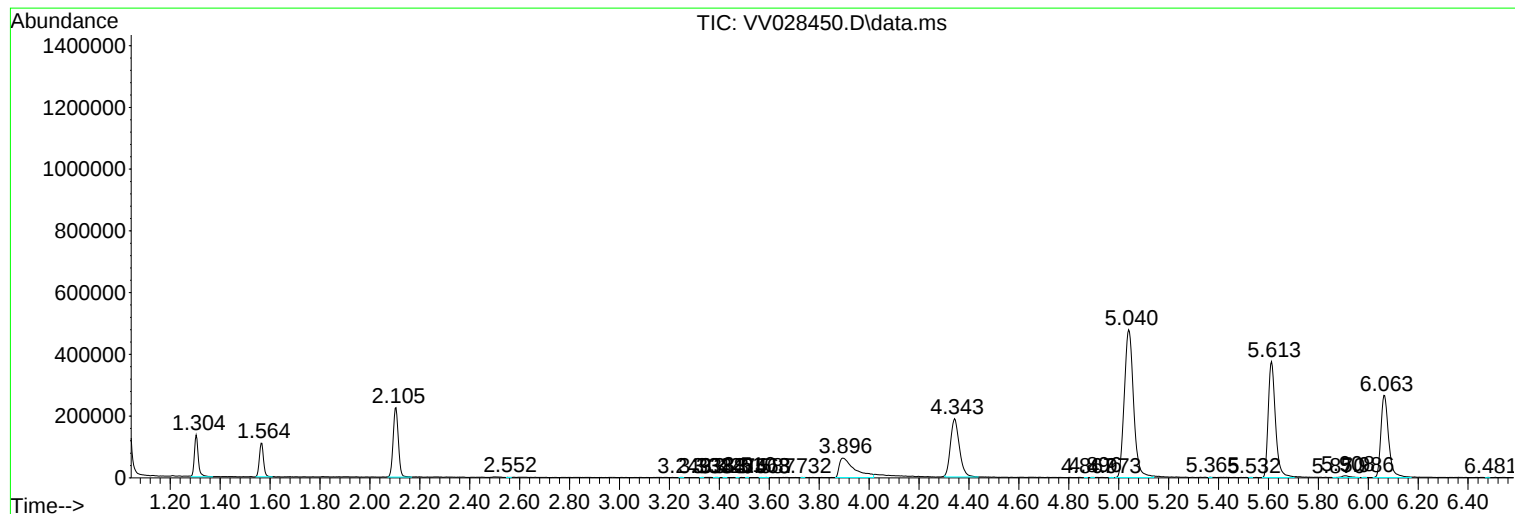

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028450.D
Acq On : 08 Oct 2022 20:37
Operator : SY/MD
Sample : N4889-05DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ63DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028450.D
Acq On : 08 Oct 2022 20:37
Operator : SY/MD
Sample : N4889-05DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ63DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc