

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028451.D
 Acq On : 08 Oct 2022 21:01
 Operator : SY/MD
 Sample : N4889-04DL 2000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ62DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	132594	138966	5.56%	1.158%
2	1.564	156	163	179	rVB	106313	123716	4.95%	1.031%
3	2.101	320	330	345	rBV	219353	315530	12.63%	2.629%
4	2.500	448	454	464	rBV8	2685	4388	0.18%	0.037%
5	2.767	534	537	539	rBV2	1052	723	0.03%	0.006%
6	2.834	556	558	562	rVB3	898	587	0.02%	0.005%
7	2.860	562	566	568	rBV2	543	276	0.01%	0.002%
8	2.876	568	571	575	rBV	813	524	0.02%	0.004%
9	2.931	585	588	592	rBV3	554	482	0.02%	0.004%
10	2.979	601	603	606	rBV3	488	342	0.01%	0.003%
11	3.047	622	624	627	rVB2	698	312	0.01%	0.003%
12	3.066	627	630	634	rBV4	519	424	0.02%	0.004%
13	3.217	674	677	678	rBV	547	272	0.01%	0.002%
14	3.265	688	692	695	rBV3	487	403	0.02%	0.003%
15	3.394	730	732	736	rVB4	813	351	0.01%	0.003%
16	3.420	738	740	742	rBV2	576	335	0.01%	0.003%
17	3.593	792	794	797	rVV	621	282	0.01%	0.002%
18	3.613	798	800	805	rVB3	743	442	0.02%	0.004%
19	3.638	805	808	810	rBV3	655	442	0.02%	0.004%
20	3.658	810	814	816	rBV3	422	350	0.01%	0.003%
21	3.757	842	845	848	rBV3	649	390	0.02%	0.003%
22	3.789	852	855	858	rBV3	781	372	0.01%	0.003%
23	3.812	859	862	865	rBV2	657	403	0.02%	0.003%
24	3.895	878	888	926	rBV	65694	267918	10.72%	2.232%
25	4.342	1013	1027	1057	rVB	184798	466377	18.67%	3.886%
26	4.648	1118	1122	1125	rBV4	632	642	0.03%	0.005%
27	4.738	1148	1150	1152	rBV3	546	367	0.01%	0.003%
28	4.860	1185	1188	1191	rBV	671	392	0.02%	0.003%
29	5.040	1228	1244	1274	rBV2	474232	1216920	48.71%	10.140%
30	5.384	1348	1351	1353	rBV3	513	303	0.01%	0.003%
31	5.410	1356	1359	1361	rBV4	698	402	0.02%	0.003%
32	5.442	1367	1369	1372	rVB3	600	306	0.01%	0.003%
33	5.465	1372	1376	1377	rBV2	663	345	0.01%	0.003%
34	5.490	1381	1384	1386	rBV2	519	309	0.01%	0.003%
35	5.612	1410	1422	1446	rBV	375626	759062	30.38%	6.325%
36	5.905	1504	1513	1520	rBV7	6039	10617	0.42%	0.088%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100822\
 Data File : VW028451.D
 Acq On : 08 Oct 2022 21:01
 Operator : SY/MD
 Sample : N4889-04DL 2000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ62DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.066	1549	1563	1591	rBV	267926	567003	22.69%	4.724%
38	6.320	1638	1642	1644	rBV4	503	335	0.01%	0.003%
39	6.458	1682	1685	1687	rBV4	618	362	0.01%	0.003%
40	6.490	1693	1695	1698	rBV4	517	255	0.01%	0.002%
41	6.526	1704	1706	1707	rBV	830	378	0.02%	0.003%
42	6.792	1786	1789	1792	rBV2	644	484	0.02%	0.004%
43	6.982	1836	1848	1875	rBV	163001	308249	12.34%	2.568%
44	7.194	1912	1914	1916	rBV2	808	467	0.02%	0.004%
45	7.310	1939	1950	1962	rBV	572688	983533	39.37%	8.195%
46	7.381	1962	1972	2001	rVB	1453545	2498388	100.00%	20.817%
47	7.619	2036	2046	2070	rBV	109532	196818	7.88%	1.640%
48	7.985	2155	2160	2161	rBV3	561	489	0.02%	0.004%
49	8.085	2182	2191	2230	rBV	301668	641178	25.66%	5.343%
50	8.497	2313	2319	2321	rBV6	803	883	0.04%	0.007%
51	8.574	2341	2343	2347	rVB2	704	298	0.01%	0.002%
52	8.606	2349	2353	2355	rVV4	606	394	0.02%	0.003%
53	8.625	2356	2359	2364	rVV3	795	480	0.02%	0.004%
54	8.728	2386	2391	2396	rBV5	1011	982	0.04%	0.008%
55	8.847	2416	2428	2447	rBV	542669	889041	35.58%	7.408%
56	9.011	2471	2479	2500	rVB	33942	58208	2.33%	0.485%
57	9.133	2507	2517	2532	rBV	109597	183598	7.35%	1.530%
58	9.406	2600	2602	2604	rVB2	966	457	0.02%	0.004%
59	9.497	2628	2630	2633	rBV2	380	272	0.01%	0.002%
60	9.538	2633	2643	2662	rBV	37714	65198	2.61%	0.543%
61	9.632	2670	2672	2675	rBV3	480	366	0.01%	0.003%
62	9.731	2700	2703	2704	rBV2	616	299	0.01%	0.002%
63	9.886	2749	2751	2754	rBV4	732	308	0.01%	0.003%
64	9.985	2778	2782	2784	rBV	454	387	0.02%	0.003%
65	10.050	2799	2802	2803	rBV2	543	260	0.01%	0.002%
66	10.207	2840	2851	2872	rBV	343664	549510	21.99%	4.579%
67	10.445	2918	2925	2931	rBV8	2283	3354	0.13%	0.028%
68	10.538	2950	2954	2957	rBV4	1458	1209	0.05%	0.010%
69	10.570	2962	2964	2967	rVB3	726	312	0.01%	0.003%
70	10.625	2979	2981	2991	rVB3	876	735	0.03%	0.006%
71	10.667	2991	2994	2997	rVB2	490	270	0.01%	0.002%
72	10.702	2997	3005	3009	rBV5	1543	2271	0.09%	0.019%
73	10.914	3067	3071	3080	rVB4	3985	4497	0.18%	0.037%
74	10.972	3087	3089	3091	rBV2	607	292	0.01%	0.002%
75	11.075	3118	3121	3122	rBV2	612	300	0.01%	0.002%
76	11.146	3140	3143	3145	rBV3	717	462	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028451.D
 Acq On : 08 Oct 2022 21:01
 Operator : SY/MD
 Sample : N4889-04DL 2000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ62DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.239	3161	3172	3196	rBV	555766	873337	34.96%	7.277%
78	11.429	3229	3231	3235	rBV3	615	402	0.02%	0.003%
79	11.455	3236	3239	3242	rVB4	898	448	0.02%	0.004%
80	11.493	3248	3251	3252	rBV	585	313	0.01%	0.003%
81	11.538	3262	3265	3268	rBV2	823	580	0.02%	0.005%
82	11.615	3277	3289	3308	rBV	528512	840649	33.65%	7.005%
83	11.802	3344	3347	3349	rBV3	495	343	0.01%	0.003%
84	11.930	3382	3387	3391	rBV3	782	1021	0.04%	0.009%
85	12.316	3501	3507	3509	rBV5	719	705	0.03%	0.006%
86	12.429	3540	3542	3547	rBV	488	386	0.02%	0.003%
87	12.612	3595	3599	3603	rVB4	647	493	0.02%	0.004%
88	12.686	3620	3622	3625	rBV	574	305	0.01%	0.003%
89	12.731	3633	3636	3639	rBV4	566	483	0.02%	0.004%
90	12.757	3641	3644	3646	rBV3	639	342	0.01%	0.003%
91	12.811	3656	3661	3662	rBV2	706	535	0.02%	0.004%
92	12.885	3683	3684	3689	rVB4	619	303	0.01%	0.003%
93	13.049	3733	3735	3738	rBV4	767	477	0.02%	0.004%
94	13.226	3787	3790	3792	rBV4	702	405	0.02%	0.003%
95	13.464	3861	3864	3866	rBV2	662	354	0.01%	0.003%
96	13.519	3878	3881	3883	rBV3	663	490	0.02%	0.004%
97	13.673	3926	3929	3934	rVB3	962	899	0.04%	0.007%
98	13.702	3934	3938	3941	rBV3	773	564	0.02%	0.005%
99	13.741	3947	3950	3952	rBV2	559	401	0.02%	0.003%
100	14.082	4053	4056	4058	rBV2	612	357	0.01%	0.003%




Sum of corrected areas: 12001446

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028451.D
Acq On : 08 Oct 2022 21:01
Operator : SY/MD
Sample : N4889-04DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ62DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

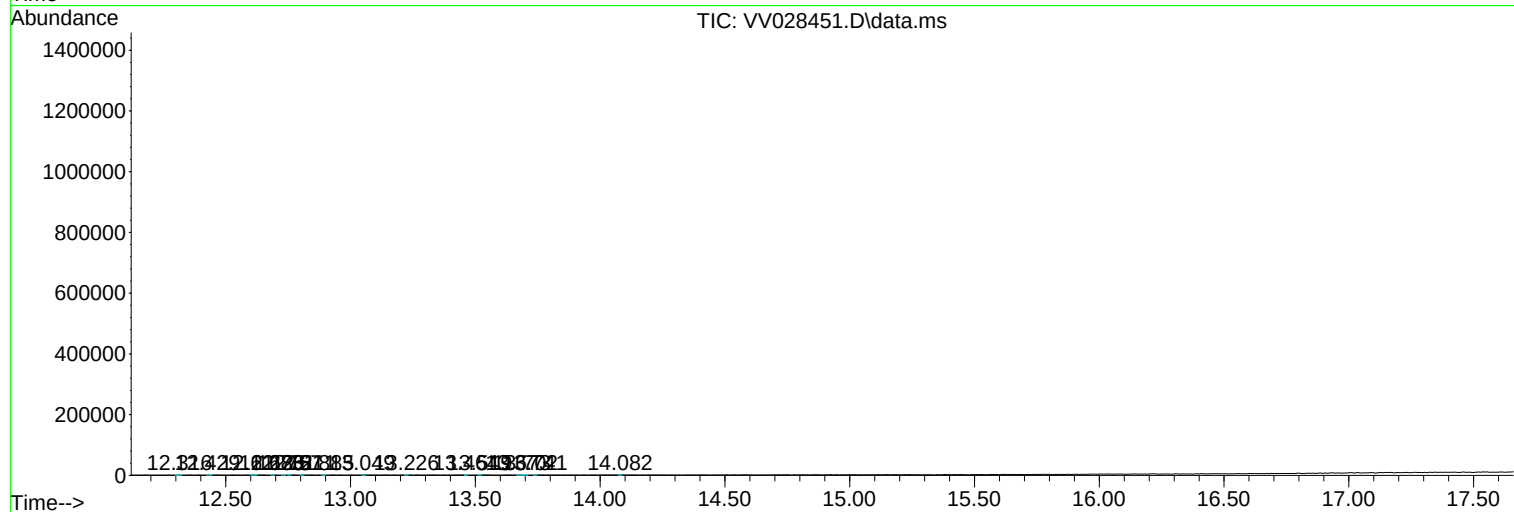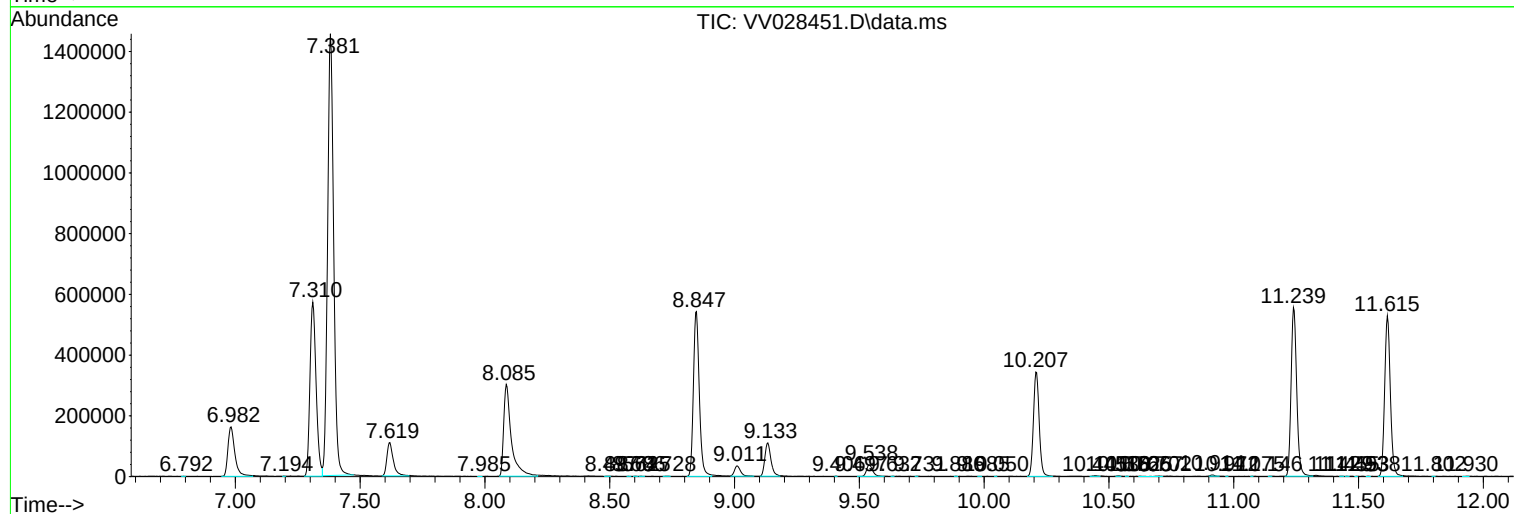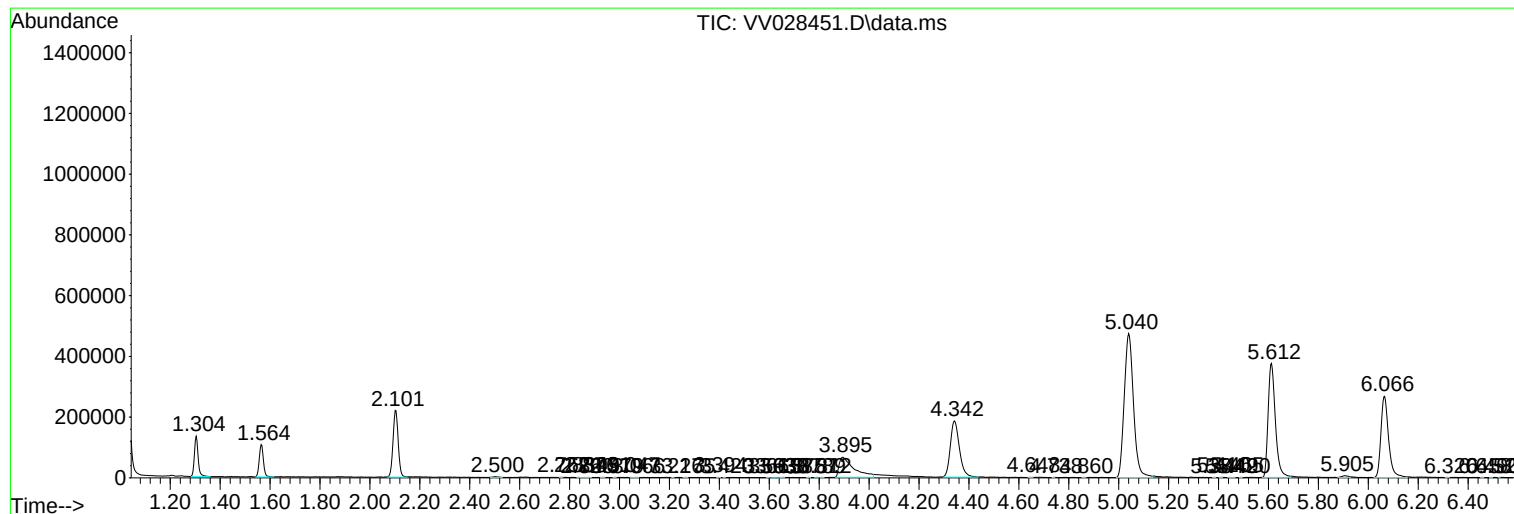

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028451.D
Acq On : 08 Oct 2022 21:01
Operator : SY/MD
Sample : N4889-04DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ62DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028451.D
Acq On : 08 Oct 2022 21:01
Operator : SY/MD
Sample : N4889-04DL 2000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ62DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc