

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028459.D
 Acq On : 09 Oct 2022 00:15
 Operator : SY/MD
 Sample : N4923-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10026

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	154159	162241	11.87%	1.343%
2	1.564	157	163	175	rVB	129395	145095	10.62%	1.201%
3	2.105	322	331	348	rVB	269074	391531	28.66%	3.240%
4	2.651	498	501	505	rBV3	659	426	0.03%	0.004%
5	2.908	578	581	583	rBV	724	419	0.03%	0.003%
6	3.002	606	610	613	rBV3	615	495	0.04%	0.004%
7	3.149	651	656	657	rBV3	689	541	0.04%	0.004%
8	3.207	672	674	678	rBV4	409	329	0.02%	0.003%
9	3.262	687	691	693	rBV2	508	390	0.03%	0.003%
10	3.342	714	716	717	rBV2	540	264	0.02%	0.002%
11	3.654	808	813	816	rBV3	505	555	0.04%	0.005%
12	3.789	853	855	859	rVB2	543	312	0.02%	0.003%
13	3.895	878	888	923	rBV	66475	257412	18.84%	2.130%
14	4.342	1014	1027	1054	rVB3	229002	669704	49.02%	5.542%
15	4.561	1092	1095	1099	rVB3	976	600	0.04%	0.005%
16	4.648	1116	1122	1123	rBV3	825	752	0.06%	0.006%
17	4.712	1140	1142	1144	rBV2	524	277	0.02%	0.002%
18	4.751	1150	1154	1155	rBV3	615	477	0.03%	0.004%
19	4.773	1159	1161	1164	rVB2	611	327	0.02%	0.003%
20	4.815	1171	1174	1176	rBV3	439	318	0.02%	0.003%
21	4.841	1179	1182	1184	rBV2	657	253	0.02%	0.002%
22	4.947	1212	1215	1217	rBV3	522	340	0.02%	0.003%
23	5.040	1225	1244	1273	rBV2	526215	1366270	100.00%	11.306%
24	5.368	1344	1346	1348	rBV2	766	456	0.03%	0.004%
25	5.468	1376	1377	1381	rVB3	941	614	0.04%	0.005%
26	5.500	1381	1387	1393	rVB7	815	918	0.07%	0.008%
27	5.538	1394	1399	1400	rBV3	704	536	0.04%	0.004%
28	5.612	1410	1422	1454	rBV	424067	858993	62.87%	7.108%
29	5.911	1505	1515	1527	rBV9	4183	8902	0.65%	0.074%
30	6.005	1542	1544	1548	rVB4	577	318	0.02%	0.003%
31	6.066	1549	1563	1597	rBV	302488	626993	45.89%	5.188%
32	6.429	1673	1676	1678	rBV4	572	307	0.02%	0.003%
33	6.452	1681	1683	1687	rBV3	497	337	0.02%	0.003%
34	6.513	1692	1702	1717	rBV3	8431	17814	1.30%	0.147%
35	6.731	1766	1770	1771	rBV4	651	455	0.03%	0.004%
36	6.783	1784	1786	1788	rBV3	528	240	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028459.D
 Acq On : 09 Oct 2022 00:15
 Operator : SY/MD
 Sample : N4923-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10026

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.821	1797	1798	1800	rBV	529	258	0.02%	0.002%
38	6.895	1816	1821	1823	rBV4	549	399	0.03%	0.003%
39	6.915	1825	1827	1832	rVB2	439	334	0.02%	0.003%
40	6.982	1837	1848	1879	rBV	177982	341599	25.00%	2.827%
41	7.310	1939	1950	1970	rBV	650227	1115106	81.62%	9.227%
42	7.616	2036	2045	2067	rBV	123148	221164	16.19%	1.830%
43	7.902	2130	2134	2136	rBV4	878	771	0.06%	0.006%
44	8.085	2181	2191	2229	rBV	348654	724013	52.99%	5.991%
45	8.661	2368	2370	2372	rBV2	555	345	0.03%	0.003%
46	8.725	2386	2390	2392	rBV2	718	527	0.04%	0.004%
47	8.770	2401	2404	2405	rBV2	819	446	0.03%	0.004%
48	8.847	2416	2428	2456	rBV	608359	1012328	74.09%	8.377%
49	9.085	2499	2502	2505	rVB3	1330	771	0.06%	0.006%
50	9.136	2509	2518	2532	rBV2	24150	44375	3.25%	0.367%
51	9.239	2548	2550	2553	rVV3	800	410	0.03%	0.003%
52	9.265	2555	2558	2563	rVB4	905	585	0.04%	0.005%
53	9.304	2563	2570	2572	rBV4	771	952	0.07%	0.008%
54	9.397	2595	2599	2600	rBV2	584	372	0.03%	0.003%
55	9.542	2633	2644	2664	rBV2	15007	29680	2.17%	0.246%
56	9.667	2681	2683	2687	rVB3	879	498	0.04%	0.004%
57	9.693	2689	2691	2694	rBV	526	298	0.02%	0.002%
58	9.738	2700	2705	2708	rBV4	549	485	0.04%	0.004%
59	9.792	2719	2722	2723	rBV	399	229	0.02%	0.002%
60	9.805	2723	2726	2731	rVV3	908	711	0.05%	0.006%
61	9.863	2742	2744	2746	rBV3	688	293	0.02%	0.002%
62	9.902	2751	2756	2758	rBV3	549	504	0.04%	0.004%
63	9.921	2759	2762	2765	rBV2	455	235	0.02%	0.002%
64	9.988	2779	2783	2785	rBV3	712	621	0.05%	0.005%
65	10.207	2839	2851	2870	rBV	402782	641532	46.95%	5.309%
66	10.374	2895	2903	2913	rVB4	4823	8233	0.60%	0.068%
67	10.435	2920	2922	2923	rBV	511	252	0.02%	0.002%
68	10.477	2932	2935	2939	rBV3	567	417	0.03%	0.003%
69	10.529	2947	2951	2952	rBV3	842	651	0.05%	0.005%
70	10.644	2983	2987	2989	rBV5	519	477	0.03%	0.004%
71	10.689	2995	3001	3003	rBV5	526	404	0.03%	0.003%
72	10.718	3007	3010	3013	rBV2	636	360	0.03%	0.003%
73	10.767	3019	3025	3027	rBV2	1213	1142	0.08%	0.009%
74	10.863	3053	3055	3059	rVB4	725	390	0.03%	0.003%
75	11.024	3104	3105	3107	rBV2	584	278	0.02%	0.002%
76	11.143	3137	3142	3144	rBV5	819	829	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028459.D
 Acq On : 09 Oct 2022 00:15
 Operator : SY/MD
 Sample : N4923-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10026

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.172	3144	3151	3162	rVV5	5121	8925	0.65%	0.074%
78	11.239	3162	3172	3195	rVV	659677	1020622	74.70%	8.445%
79	11.458	3236	3240	3242	rVB3	660	470	0.03%	0.004%
80	11.615	3277	3289	3313	rBV	626504	994425	72.78%	8.229%
81	11.741	3320	3328	3342	rVB2	13708	23495	1.72%	0.194%
82	11.995	3404	3407	3410	rBV3	785	642	0.05%	0.005%
83	12.107	3440	3442	3444	rBV2	523	293	0.02%	0.002%
84	12.242	3478	3484	3494	rVV7	1641	2834	0.21%	0.023%
85	12.345	3505	3516	3518	rBV6	4683	6016	0.44%	0.050%
86	12.580	3587	3589	3592	rBV	343	269	0.02%	0.002%
87	12.725	3631	3634	3638	rVB5	1052	796	0.06%	0.007%
88	12.873	3677	3680	3688	rVB8	2172	2376	0.17%	0.020%
89	12.943	3697	3702	3703	rBV4	1966	1678	0.12%	0.014%
90	13.046	3725	3734	3736	rBV5	2977	3507	0.26%	0.029%
91	13.365	3828	3833	3836	rBV2	948	1049	0.08%	0.009%
92	13.490	3862	3872	3892	rBV	258067	417242	30.54%	3.453%
93	14.200	4090	4093	4095	rBV3	1058	672	0.05%	0.006%
94	14.622	4214	4224	4241	rBV	113586	182969	13.39%	1.514%
95	14.805	4271	4281	4295	rBV	85116	138267	10.12%	1.144%
96	15.352	4443	4451	4467	rVB	43012	66943	4.90%	0.554%
97	15.654	4538	4545	4556	rVB	39737	61761	4.52%	0.511%
98	15.799	4582	4590	4597	rBV	61025	96519	7.06%	0.799%
99	16.258	4724	4733	4750	rVB2	163327	278320	20.37%	2.303%
100	16.471	4791	4799	4816	rVB	67998	105362	7.71%	0.872%




Sum of corrected areas: 12084937

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028459.D
Acq On : 09 Oct 2022 00:15
Operator : SY/MD
Sample : N4923-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10026

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

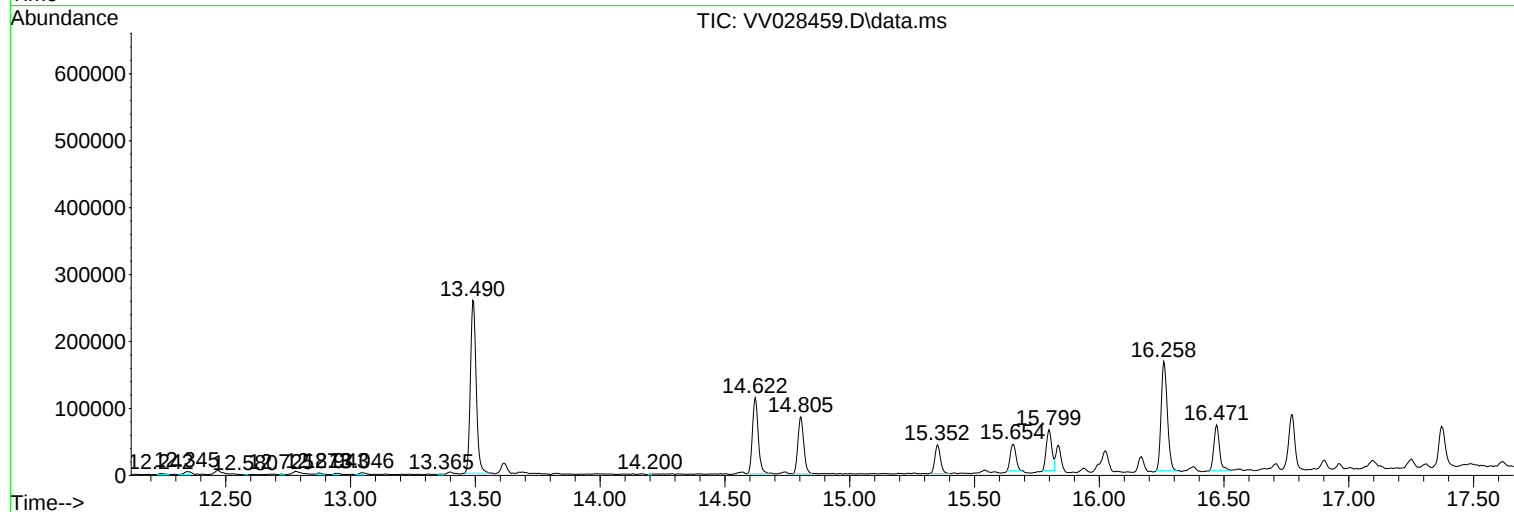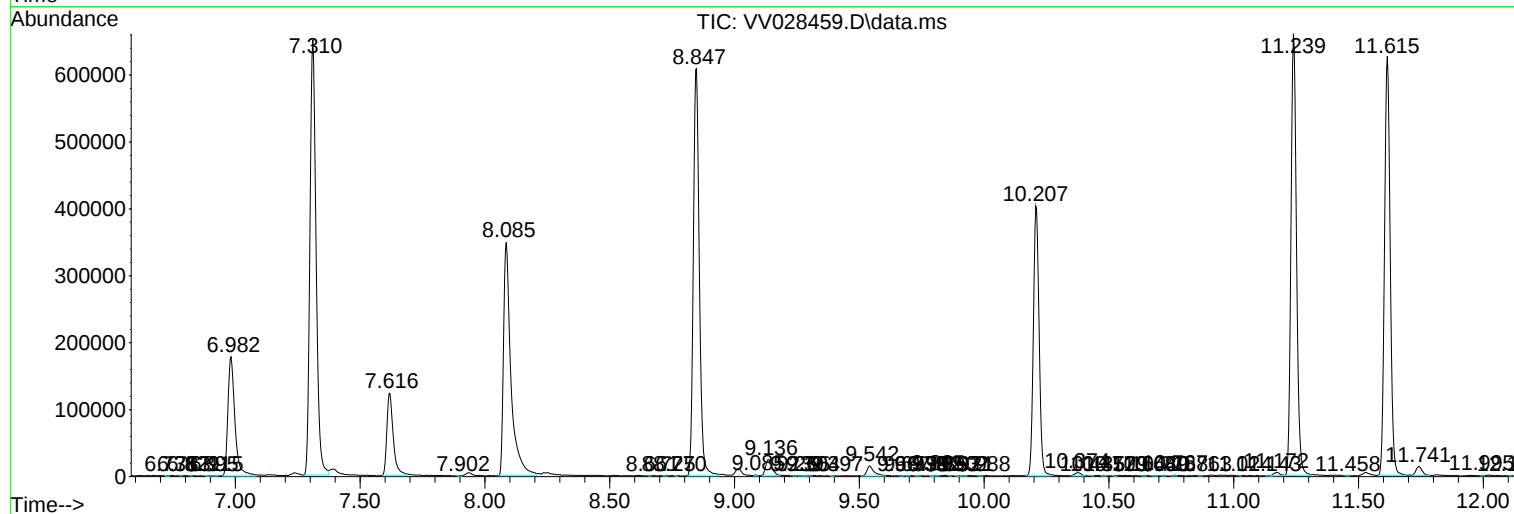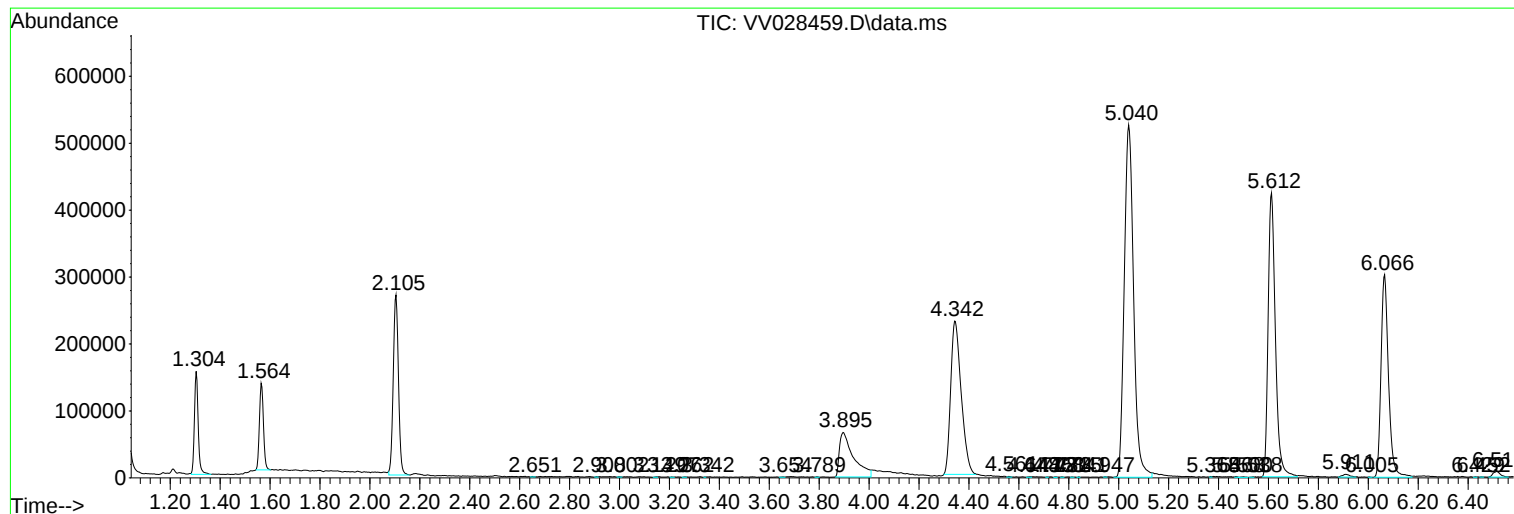

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028459.D
Acq On : 09 Oct 2022 00:15
Operator : SY/MD
Sample : N4923-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10026

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028459.D
Acq On : 09 Oct 2022 00:15
Operator : SY/MD
Sample : N4923-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10026

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc