

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028466.D
 Acq On : 09 Oct 2022 03:27
 Operator : SY/MD
 Sample : VV1008WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK273

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	246016	258193	15.47%	2.122%
2	1.568	157	164	174	rBV	187605	214148	12.83%	1.760%
3	2.105	322	331	349	rVB	376400	540874	32.41%	4.445%
4	2.941	587	591	593	rBV	827	607	0.04%	0.005%
5	2.995	606	608	611	rVB3	905	489	0.03%	0.004%
6	3.031	617	619	623	rVB4	954	553	0.03%	0.005%
7	3.079	632	634	639	rBV3	560	531	0.03%	0.004%
8	3.121	643	647	648	rBV3	735	375	0.02%	0.003%
9	3.169	658	662	663	rBV3	461	341	0.02%	0.003%
10	3.294	697	701	702	rBV2	556	427	0.03%	0.004%
11	3.481	756	759	762	rBV3	529	339	0.02%	0.003%
12	3.497	762	764	769	rVB4	727	488	0.03%	0.004%
13	3.529	769	774	781	rVB5	1149	1273	0.08%	0.010%
14	3.600	794	796	798	rBV2	523	302	0.02%	0.002%
15	3.658	810	814	818	rVB3	699	537	0.03%	0.004%
16	3.677	818	820	821	rBV2	687	317	0.02%	0.003%
17	3.703	826	828	832	rVB3	493	321	0.02%	0.003%
18	3.761	843	846	848	rBV3	523	354	0.02%	0.003%
19	3.899	875	889	928	rBV2	78754	340266	20.39%	2.797%
20	4.343	1014	1027	1059	rVB	253677	627819	37.62%	5.160%
21	4.854	1183	1186	1189	rBV5	474	396	0.02%	0.003%
22	4.896	1194	1199	1201	rBV4	601	469	0.03%	0.004%
23	5.040	1227	1244	1272	rBV2	648445	1669055	100.00%	13.718%
24	5.397	1352	1355	1362	rBV5	701	924	0.06%	0.008%
25	5.613	1410	1422	1452	rBV	430303	879309	52.68%	7.227%
26	5.860	1497	1499	1502	rBV2	649	413	0.02%	0.003%
27	5.908	1507	1514	1527	rVB10	4445	9148	0.55%	0.075%
28	6.066	1546	1563	1589	rBV	362417	751954	45.05%	6.180%
29	6.359	1652	1654	1658	rBV5	1113	703	0.04%	0.006%
30	6.481	1687	1692	1694	rBV4	805	744	0.04%	0.006%
31	6.513	1698	1702	1704	rBV2	657	468	0.03%	0.004%
32	6.641	1738	1742	1743	rBV2	672	409	0.02%	0.003%
33	6.847	1803	1806	1808	rVB2	644	377	0.02%	0.003%
34	6.867	1808	1812	1816	rBV5	721	686	0.04%	0.006%
35	6.895	1819	1821	1823	rBV	661	382	0.02%	0.003%
36	6.982	1837	1848	1872	rVV	212631	401140	24.03%	3.297%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028466.D
 Acq On : 09 Oct 2022 03:27
 Operator : SY/MD
 Sample : VV1008WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK273

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.310	1938	1950	1986	rBV	770137	1358180	81.37%	11.163%
38	7.616	2036	2045	2068	rBV	144784	261661	15.68%	2.151%
39	7.870	2119	2124	2127	rBV6	792	736	0.04%	0.006%
40	7.989	2158	2161	2163	rBV2	799	650	0.04%	0.005%
41	8.047	2175	2179	2181	rBV3	655	484	0.03%	0.004%
42	8.085	2181	2191	2230	rBV	426074	864365	51.79%	7.104%
43	8.551	2332	2336	2340	rBV4	797	604	0.04%	0.005%
44	8.786	2406	2409	2411	rBV2	718	511	0.03%	0.004%
45	8.847	2416	2428	2456	rBV	614326	1022790	61.28%	8.406%
46	9.194	2535	2536	2539	rBV3	895	471	0.03%	0.004%
47	9.265	2555	2558	2562	rVV5	700	621	0.04%	0.005%
48	9.320	2570	2575	2578	rBV5	808	691	0.04%	0.006%
49	9.403	2597	2601	2607	rBV3	695	810	0.05%	0.007%
50	9.471	2617	2622	2625	rBV5	892	847	0.05%	0.007%
51	9.542	2639	2644	2645	rBV	830	610	0.04%	0.005%
52	9.593	2657	2660	2663	rVB3	612	450	0.03%	0.004%
53	9.747	2705	2708	2710	rBV3	617	482	0.03%	0.004%
54	9.780	2715	2718	2723	rBV3	913	815	0.05%	0.007%
55	9.886	2748	2751	2759	rBV5	693	625	0.04%	0.005%
56	9.924	2759	2763	2765	rBV4	655	451	0.03%	0.004%
57	9.969	2774	2777	2780	rBV4	627	417	0.02%	0.003%
58	9.992	2780	2784	2789	rVV4	738	680	0.04%	0.006%
59	10.024	2792	2794	2798	rVB4	677	482	0.03%	0.004%
60	10.072	2806	2809	2812	rBV2	618	384	0.02%	0.003%
61	10.114	2819	2822	2825	rVB4	678	405	0.02%	0.003%
62	10.133	2825	2828	2831	rBV3	1057	818	0.05%	0.007%
63	10.207	2840	2851	2876	rBV	462954	741091	44.40%	6.091%
64	10.345	2892	2894	2898	rBV2	711	385	0.02%	0.003%
65	10.387	2904	2907	2910	rBV4	740	463	0.03%	0.004%
66	10.436	2919	2922	2926	rVB4	544	421	0.03%	0.003%
67	10.609	2974	2976	2980	rVB2	493	334	0.02%	0.003%
68	10.956	3082	3084	3086	rBV2	491	293	0.02%	0.002%
69	10.989	3091	3094	3098	rVB4	599	351	0.02%	0.003%
70	11.046	3110	3112	3113	rBV	792	360	0.02%	0.003%
71	11.085	3123	3124	3129	rVB2	465	301	0.02%	0.002%
72	11.153	3142	3145	3148	rBV2	719	602	0.04%	0.005%
73	11.178	3148	3153	3155	rBV5	1484	1501	0.09%	0.012%
74	11.239	3160	3172	3193	rBV	655832	1011851	60.62%	8.316%
75	11.525	3255	3261	3265	rBV5	1626	1564	0.09%	0.013%
76	11.616	3276	3289	3312	rBV	719379	1135338	68.02%	9.331%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028466.D
 Acq On : 09 Oct 2022 03:27
 Operator : SY/MD
 Sample : VV1008WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK273

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.815	3349	3351	3355	rBV4	521	468	0.03%	0.004%
78	11.857	3363	3364	3367	rVB2	701	379	0.02%	0.003%
79	11.876	3367	3370	3372	rBV	469	340	0.02%	0.003%
80	12.034	3412	3419	3422	rBV5	627	803	0.05%	0.007%
81	12.069	3427	3430	3432	rBV2	621	355	0.02%	0.003%
82	12.098	3436	3439	3442	rBV3	711	500	0.03%	0.004%
83	12.294	3497	3500	3504	rBV2	832	408	0.02%	0.003%
84	12.384	3525	3528	3531	rBV2	466	318	0.02%	0.003%
85	12.426	3538	3541	3545	rBV3	562	481	0.03%	0.004%
86	12.529	3570	3573	3576	rBV3	734	527	0.03%	0.004%
87	12.606	3595	3597	3600	rVB2	601	371	0.02%	0.003%
88	12.641	3604	3608	3613	rVB3	1112	948	0.06%	0.008%
89	12.747	3638	3641	3646	rBV3	529	401	0.02%	0.003%
90	12.837	3667	3669	3674	rVV5	620	549	0.03%	0.005%
91	12.998	3715	3719	3722	rBV2	596	508	0.03%	0.004%
92	13.053	3733	3736	3738	rBV4	647	316	0.02%	0.003%
93	13.259	3797	3800	3806	rVB7	1592	1471	0.09%	0.012%
94	13.349	3826	3828	3833	rBV3	604	356	0.02%	0.003%
95	13.461	3860	3863	3866	rBV	625	604	0.04%	0.005%
96	13.500	3866	3875	3889	rVV	18376	32399	1.94%	0.266%
97	13.734	3943	3948	3957	rBV7	2357	2986	0.18%	0.025%
98	14.149	4073	4077	4079	rBV2	707	508	0.03%	0.004%
99	14.487	4180	4182	4183	rBV	686	356	0.02%	0.003%
100	14.744	4258	4262	4264	rBV3	935	626	0.04%	0.005%




Sum of corrected areas: 12167004

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028466.D
Acq On : 09 Oct 2022 03:27
Operator : SY/MD
Sample : VV1008WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

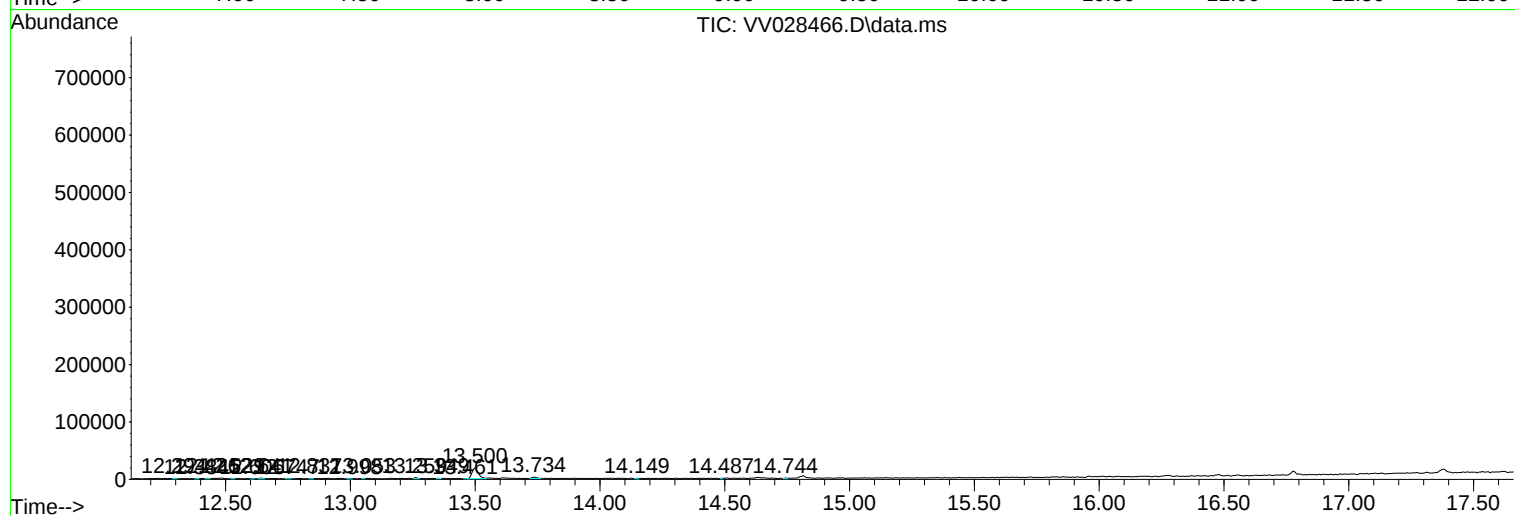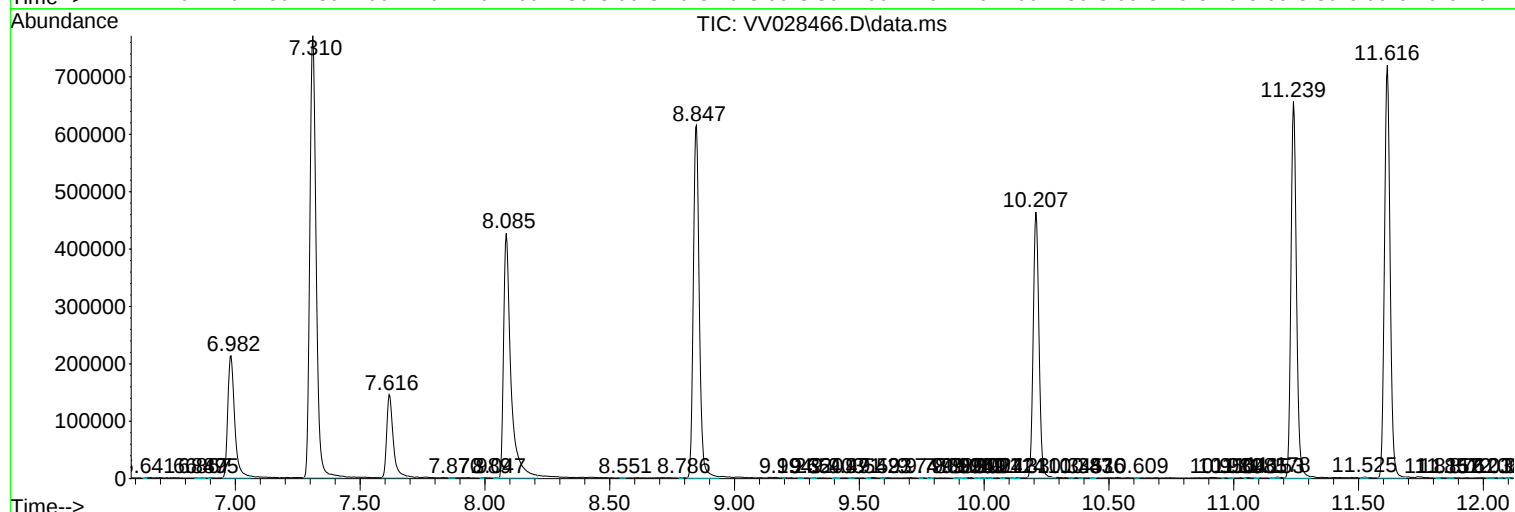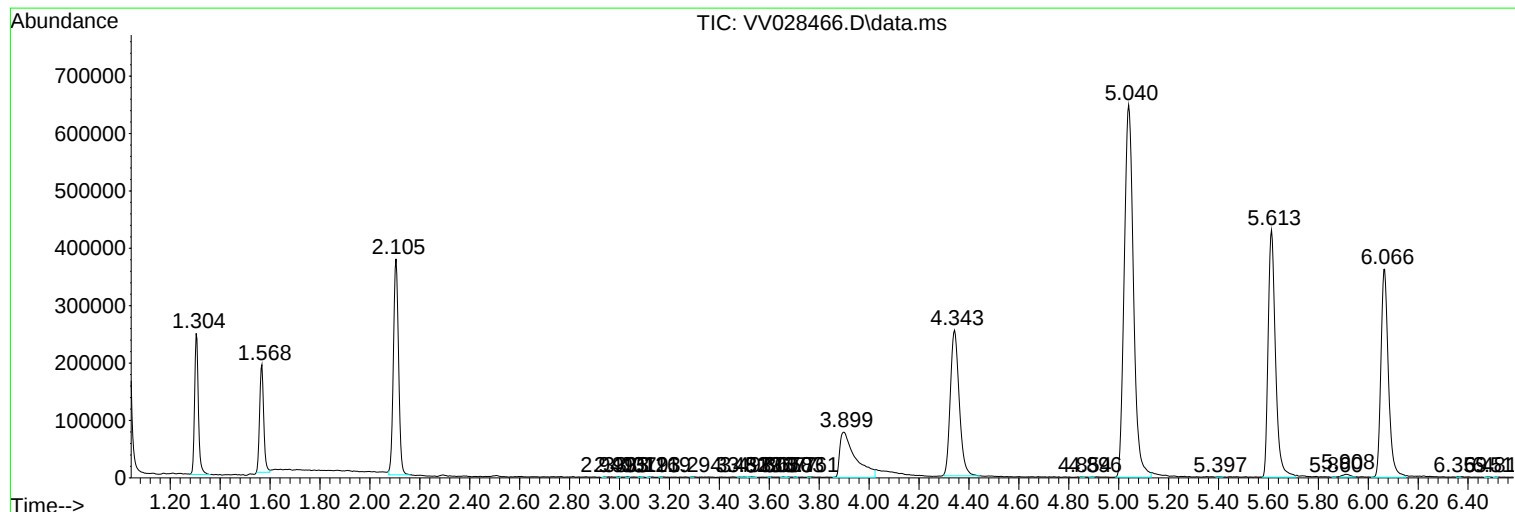

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028466.D
Acq On : 09 Oct 2022 03:27
Operator : SY/MD
Sample : VV1008WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028466.D
Acq On : 09 Oct 2022 03:27
Operator : SY/MD
Sample : VV1008WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc