

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028467.D
 Acq On : 09 Oct 2022 03:51
 Operator : SY/MD
 Sample : N4923-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	158783	165128	11.42%	1.521%
2	1.568	158	164	174	rBV	131491	148769	10.29%	1.371%
3	2.105	323	331	350	rVB	279833	407438	28.18%	3.754%
4	2.902	577	579	582	rVB2	993	503	0.03%	0.005%
5	2.934	586	589	594	rVB5	786	700	0.05%	0.006%
6	2.963	594	598	602	rBV4	1079	1219	0.08%	0.011%
7	3.021	611	616	617	rBV3	1011	893	0.06%	0.008%
8	3.088	634	637	640	rVB2	798	376	0.03%	0.003%
9	3.108	640	643	646	rBV3	629	546	0.04%	0.005%
10	3.268	691	693	697	rBV2	504	229	0.02%	0.002%
11	3.346	714	717	719	rBV	607	357	0.02%	0.003%
12	3.426	737	742	748	rBV5	871	1220	0.08%	0.011%
13	3.590	791	793	796	rVB2	564	288	0.02%	0.003%
14	3.654	809	813	814	rBV2	530	282	0.02%	0.003%
15	3.667	815	817	822	rVB2	838	509	0.04%	0.005%
16	3.690	822	824	826	rBV	783	292	0.02%	0.003%
17	3.712	830	831	833	rBV	563	252	0.02%	0.002%
18	3.735	836	838	841	rBV2	638	359	0.02%	0.003%
19	3.767	846	848	854	rVB3	658	441	0.03%	0.004%
20	3.802	854	859	862	rBV6	565	602	0.04%	0.006%
21	3.825	864	866	868	rBV2	707	423	0.03%	0.004%
22	3.899	879	889	917	rBV	66671	257772	17.83%	2.375%
23	4.342	1013	1027	1051	rBV	222051	546387	37.80%	5.034%
24	4.625	1112	1115	1119	rBV2	534	433	0.03%	0.004%
25	4.773	1157	1161	1164	rBV2	401	289	0.02%	0.003%
26	4.818	1173	1175	1178	rVB4	472	210	0.01%	0.002%
27	4.850	1181	1185	1187	rVV3	438	291	0.02%	0.003%
28	5.040	1228	1244	1280	rBV2	558407	1445606	100.00%	13.319%
29	5.310	1326	1328	1331	rBV4	842	513	0.04%	0.005%
30	5.484	1378	1382	1383	rBV2	693	400	0.03%	0.004%
31	5.612	1406	1422	1454	rBV	442561	901537	62.36%	8.306%
32	5.982	1535	1537	1540	rBV3	575	345	0.02%	0.003%
33	5.995	1540	1541	1544	rVV3	445	229	0.02%	0.002%
34	6.066	1549	1563	1594	rBV	310457	656498	45.41%	6.049%
35	6.378	1658	1660	1663	rVB3	663	296	0.02%	0.003%
36	6.423	1670	1674	1677	rBV5	814	633	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028467.D
 Acq On : 09 Oct 2022 03:51
 Operator : SY/MD
 Sample : N4923-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.461	1683	1686	1688	rVB2	906	522	0.04%	0.005%
38	6.509	1697	1701	1706	rBV4	989	1063	0.07%	0.010%
39	6.564	1713	1718	1723	rBV5	794	957	0.07%	0.009%
40	6.709	1760	1763	1765	rVB3	544	272	0.02%	0.003%
41	6.760	1775	1779	1783	rVB4	1059	801	0.06%	0.007%
42	6.783	1783	1786	1787	rBV3	656	358	0.02%	0.003%
43	6.870	1811	1813	1817	rBV4	475	208	0.01%	0.002%
44	6.921	1827	1829	1830	rBV	471	204	0.01%	0.002%
45	6.931	1830	1832	1837	rVB4	724	516	0.04%	0.005%
46	6.982	1837	1848	1880	rBV	187870	352746	24.40%	3.250%
47	7.310	1938	1950	1974	rBV	665630	1168966	80.86%	10.770%
48	7.616	2036	2045	2074	rBV	125859	232281	16.07%	2.140%
49	7.937	2136	2145	2152	rBV4	3344	5477	0.38%	0.050%
50	8.085	2182	2191	2226	rBV	367129	770263	53.28%	7.097%
51	8.805	2412	2415	2416	rBV	655	331	0.02%	0.003%
52	8.847	2416	2428	2449	rBV	631607	1040880	72.00%	9.590%
53	9.185	2530	2533	2535	rVB3	630	327	0.02%	0.003%
54	9.204	2537	2539	2541	rVV2	714	406	0.03%	0.004%
55	9.220	2543	2544	2548	rVB2	627	308	0.02%	0.003%
56	9.271	2557	2560	2561	rBV	623	273	0.02%	0.003%
57	9.361	2585	2588	2590	rBV2	513	328	0.02%	0.003%
58	9.387	2594	2596	2598	rBV2	459	204	0.01%	0.002%
59	9.471	2619	2622	2628	rVB5	727	681	0.05%	0.006%
60	9.519	2632	2637	2638	rBV3	867	599	0.04%	0.006%
61	9.587	2654	2658	2661	rBV5	1007	920	0.06%	0.008%
62	9.644	2672	2676	2678	rBV	451	335	0.02%	0.003%
63	9.709	2694	2696	2698	rBV2	442	239	0.02%	0.002%
64	9.776	2714	2717	2718	rVV3	804	468	0.03%	0.004%
65	9.799	2722	2724	2726	rBV	355	214	0.01%	0.002%
66	9.818	2728	2730	2732	rVB2	718	323	0.02%	0.003%
67	9.844	2736	2738	2740	rBV	358	226	0.02%	0.002%
68	9.934	2765	2766	2769	rVB2	717	251	0.02%	0.002%
69	9.953	2769	2772	2774	rBV2	454	305	0.02%	0.003%
70	10.107	2819	2820	2827	rVB5	751	512	0.04%	0.005%
71	10.136	2827	2829	2832	rBV3	419	213	0.01%	0.002%
72	10.207	2839	2851	2872	rBV	423372	677500	46.87%	6.242%
73	10.377	2898	2904	2911	rVB4	3542	4735	0.33%	0.044%
74	10.558	2957	2960	2961	rBV	624	355	0.02%	0.003%
75	10.615	2974	2978	2979	rVV3	691	448	0.03%	0.004%
76	10.715	3005	3009	3010	rBV2	316	228	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028467.D
 Acq On : 09 Oct 2022 03:51
 Operator : SY/MD
 Sample : N4923-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.818	3038	3041	3042	rBV2	697	379	0.03%	0.003%
78	10.950	3080	3082	3087	rBV4	392	361	0.02%	0.003%
79	11.037	3106	3109	3112	rBV4	464	376	0.03%	0.003%
80	11.088	3124	3125	3131	rBV3	570	405	0.03%	0.004%
81	11.123	3134	3136	3137	rBV3	733	316	0.02%	0.003%
82	11.181	3151	3154	3157	rVB3	887	579	0.04%	0.005%
83	11.239	3161	3172	3197	rBV	649291	1020078	70.56%	9.398%
84	11.467	3238	3243	3245	rBV4	1168	1072	0.07%	0.010%
85	11.615	3277	3289	3310	rBV	629299	992971	68.69%	9.149%
86	11.824	3352	3354	3357	rVB3	741	401	0.03%	0.004%
87	11.860	3363	3365	3369	rBV3	619	367	0.03%	0.003%
88	12.046	3422	3423	3426	rBV2	457	256	0.02%	0.002%
89	12.117	3443	3445	3446	rBV2	615	291	0.02%	0.003%
90	12.191	3465	3468	3471	rBV3	745	679	0.05%	0.006%
91	12.352	3514	3518	3519	rBV3	455	309	0.02%	0.003%
92	12.586	3589	3591	3592	rBV2	463	211	0.01%	0.002%
93	12.924	3693	3696	3698	rBV2	584	410	0.03%	0.004%
94	13.027	3724	3728	3731	rBV5	791	696	0.05%	0.006%
95	13.117	3752	3756	3759	rBV5	515	451	0.03%	0.004%
96	13.390	3839	3841	3843	rBV2	486	263	0.02%	0.002%
97	13.500	3867	3875	3889	rBV2	12814	22826	1.58%	0.210%
98	13.696	3933	3936	3940	rBV5	732	618	0.04%	0.006%
99	14.011	4032	4034	4036	rBV3	619	295	0.02%	0.003%
100	14.123	4067	4069	4073	rBV3	950	550	0.04%	0.005%


Sum of corrected areas: 10853668

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028467.D
Acq On : 09 Oct 2022 03:51
Operator : SY/MD
Sample : N4923-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

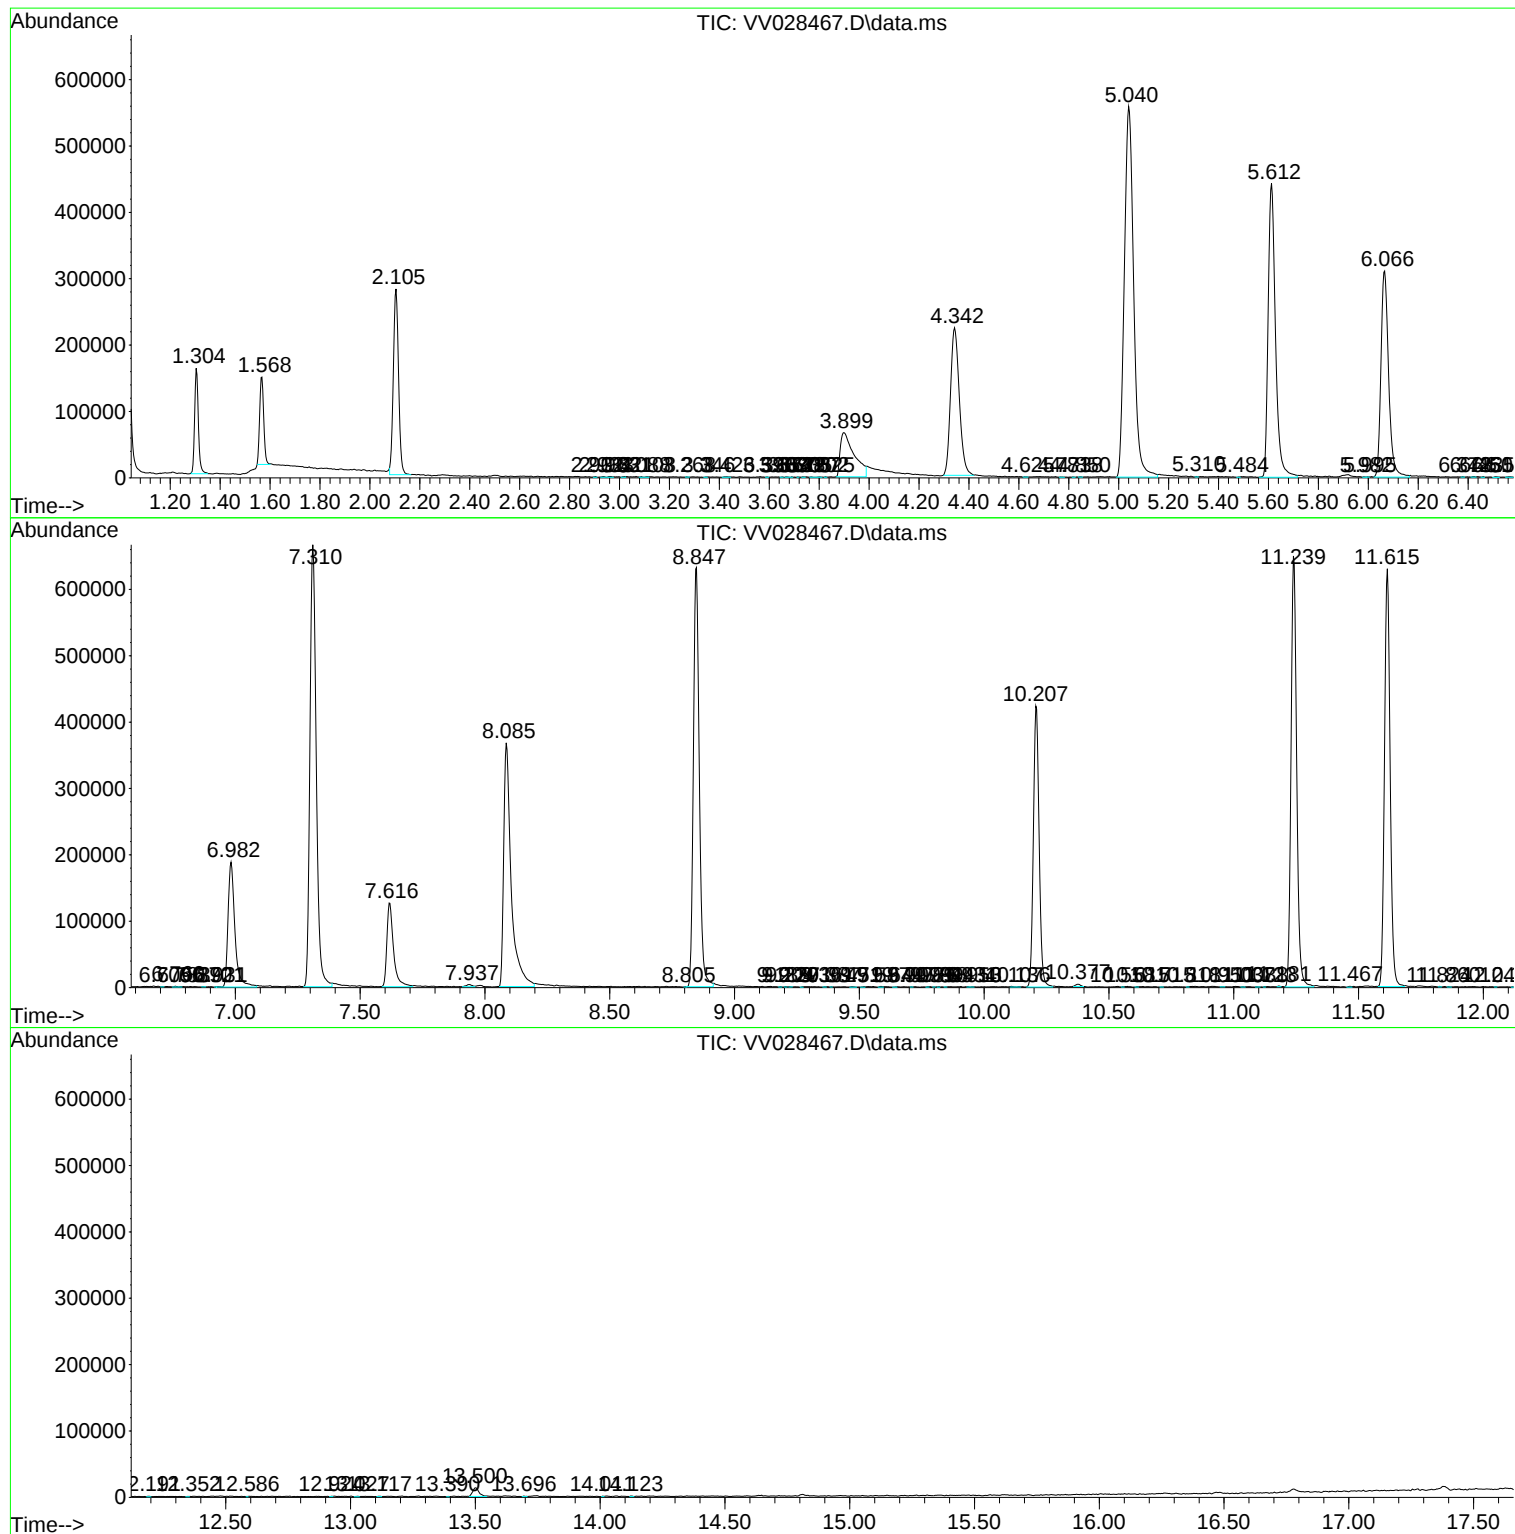

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028467.D
Acq On : 09 Oct 2022 03:51
Operator : SY/MD
Sample : N4923-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028467.D
Acq On : 09 Oct 2022 03:51
Operator : SY/MD
Sample : N4923-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------