

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028468.D
 Acq On : 09 Oct 2022 04:15
 Operator : SY/MD
 Sample : N4923-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	157914	165975	11.47%	1.509%
2	1.568	158	164	178	rVB	136058	151570	10.48%	1.378%
3	2.105	322	331	344	rVB	273955	391626	27.07%	3.560%
4	2.879	568	572	574	rBV3	709	521	0.04%	0.005%
5	3.002	608	610	614	rBV2	683	359	0.02%	0.003%
6	3.114	643	645	649	rBV3	545	390	0.03%	0.004%
7	3.310	703	706	709	rBV3	860	714	0.05%	0.006%
8	3.378	723	727	728	rBV	744	447	0.03%	0.004%
9	3.477	753	758	760	rBV5	545	532	0.04%	0.005%
10	3.500	763	765	768	rVB2	537	297	0.02%	0.003%
11	3.535	773	776	778	rBV3	479	407	0.03%	0.004%
12	3.577	785	789	792	rBV3	608	617	0.04%	0.006%
13	3.596	792	795	798	rVV3	548	442	0.03%	0.004%
14	3.706	827	829	832	rVB2	762	332	0.02%	0.003%
15	3.850	873	874	878	rBV2	502	292	0.02%	0.003%
16	3.902	878	890	916	rBV2	66150	264009	18.25%	2.400%
17	4.346	1014	1028	1059	rVB2	239690	716604	49.53%	6.515%
18	4.809	1169	1172	1173	rBV	1019	491	0.03%	0.004%
19	4.844	1181	1183	1185	rVB3	824	373	0.03%	0.003%
20	4.921	1203	1207	1210	rBV5	568	492	0.03%	0.004%
21	4.973	1220	1223	1224	rBV2	667	333	0.02%	0.003%
22	4.985	1224	1227	1228	rVV2	801	383	0.03%	0.003%
23	5.040	1228	1244	1282	rVV2	556258	1446775	100.00%	13.153%
24	5.519	1391	1393	1396	rBV2	625	300	0.02%	0.003%
25	5.558	1401	1405	1406	rBV2	775	533	0.04%	0.005%
26	5.612	1410	1422	1446	rBV	430603	875181	60.49%	7.957%
27	5.876	1500	1504	1505	rBV2	750	634	0.04%	0.006%
28	6.066	1549	1563	1593	rBV	310873	660131	45.63%	6.002%
29	6.346	1646	1650	1652	rBV3	914	666	0.05%	0.006%
30	6.429	1674	1676	1678	rBV2	642	321	0.02%	0.003%
31	6.513	1692	1702	1717	rBV2	8629	17812	1.23%	0.162%
32	6.580	1720	1723	1725	rBV3	761	425	0.03%	0.004%
33	6.596	1725	1728	1730	rVB3	755	354	0.02%	0.003%
34	6.667	1748	1750	1753	rBV4	834	475	0.03%	0.004%
35	6.760	1776	1779	1783	rBV3	512	453	0.03%	0.004%
36	6.825	1796	1799	1803	rVB5	750	471	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028468.D
 Acq On : 09 Oct 2022 04:15
 Operator : SY/MD
 Sample : N4923-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.886	1816	1818	1822	rVB4	591	357	0.02%	0.003%
38	6.982	1837	1848	1872	rBV	183788	346737	23.97%	3.152%
39	7.310	1939	1950	1974	rBV	664537	1158248	80.06%	10.530%
40	7.564	2027	2029	2032	rBV2	432	263	0.02%	0.002%
41	7.616	2036	2045	2072	rBV	126056	233705	16.15%	2.125%
42	7.966	2152	2154	2157	rBV3	849	643	0.04%	0.006%
43	8.014	2167	2169	2170	rBV2	649	278	0.02%	0.003%
44	8.085	2180	2191	2234	rBV	376933	805496	55.68%	7.323%
45	8.493	2314	2318	2319	rBV2	588	332	0.02%	0.003%
46	8.667	2369	2372	2374	rBV3	471	321	0.02%	0.003%
47	8.696	2378	2381	2386	rBV4	629	672	0.05%	0.006%
48	8.754	2397	2399	2403	rBV3	548	347	0.02%	0.003%
49	8.847	2416	2428	2450	rVV	616360	1024568	70.82%	9.315%
50	9.111	2506	2510	2512	rBV3	531	463	0.03%	0.004%
51	9.143	2512	2520	2522	rBV7	2896	3634	0.25%	0.033%
52	9.223	2539	2545	2553	rVB7	733	936	0.06%	0.009%
53	9.262	2554	2557	2559	rVV3	551	300	0.02%	0.003%
54	9.291	2564	2566	2571	rVB4	461	296	0.02%	0.003%
55	9.487	2623	2627	2633	rVB5	649	670	0.05%	0.006%
56	9.519	2633	2637	2638	rBV3	616	437	0.03%	0.004%
57	9.542	2638	2644	2650	rBV6	2832	4261	0.29%	0.039%
58	9.670	2680	2684	2687	rBV4	341	262	0.02%	0.002%
59	9.689	2687	2690	2693	rVV3	584	352	0.02%	0.003%
60	9.734	2699	2704	2712	rBV6	846	1148	0.08%	0.010%
61	9.805	2724	2726	2729	rBV	522	323	0.02%	0.003%
62	9.850	2737	2740	2741	rBV3	596	322	0.02%	0.003%
63	9.863	2741	2744	2748	rVV2	610	552	0.04%	0.005%
64	9.934	2760	2766	2772	rVB8	2060	2667	0.18%	0.024%
65	10.001	2782	2787	2789	rBV3	586	521	0.04%	0.005%
66	10.033	2794	2797	2799	rBV3	670	455	0.03%	0.004%
67	10.207	2840	2851	2869	rBV	427140	678651	46.91%	6.170%
68	10.490	2937	2939	2943	rBV2	566	256	0.02%	0.002%
69	10.535	2943	2953	2959	rBV4	2114	3169	0.22%	0.029%
70	10.660	2988	2992	2995	rBV	507	343	0.02%	0.003%
71	10.760	3019	3023	3024	rBV2	652	393	0.03%	0.004%
72	10.847	3046	3050	3053	rVB4	878	854	0.06%	0.008%
73	10.876	3055	3059	3064	rBV4	604	445	0.03%	0.004%
74	10.918	3066	3072	3076	rBV5	1883	2150	0.15%	0.020%
75	11.130	3136	3138	3140	rBV3	636	295	0.02%	0.003%
76	11.178	3148	3153	3157	rBV5	1641	2088	0.14%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028468.D
 Acq On : 09 Oct 2022 04:15
 Operator : SY/MD
 Sample : N4923-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.239	3162	3172	3199	rVV	634185	993037	68.64%	9.028%
78	11.509	3252	3256	3257	rBV2	527	448	0.03%	0.004%
79	11.615	3277	3289	3311	rBV	621900	997217	68.93%	9.066%
80	11.860	3363	3365	3368	rBV2	538	304	0.02%	0.003%
81	11.879	3369	3371	3373	rVV3	479	271	0.02%	0.002%
82	11.914	3377	3382	3385	rVB3	471	403	0.03%	0.004%
83	11.937	3385	3389	3390	rBV2	711	427	0.03%	0.004%
84	12.297	3497	3501	3504	rVB3	548	419	0.03%	0.004%
85	12.397	3530	3532	3535	rBV3	602	392	0.03%	0.004%
86	12.461	3547	3552	3553	rBV3	793	582	0.04%	0.005%
87	12.516	3567	3569	3571	rBV	567	333	0.02%	0.003%
88	12.567	3579	3585	3586	rBV3	573	438	0.03%	0.004%
89	12.609	3595	3598	3602	rBV3	427	429	0.03%	0.004%
90	12.754	3639	3643	3648	rVB6	772	803	0.06%	0.007%
91	12.860	3674	3676	3678	rBV3	589	258	0.02%	0.002%
92	12.950	3700	3704	3707	rBV3	755	633	0.04%	0.006%
93	13.001	3716	3720	3721	rBV2	463	284	0.02%	0.003%
94	13.146	3762	3765	3767	rBV	695	379	0.03%	0.003%
95	13.233	3791	3792	3795	rBV2	450	319	0.02%	0.003%
96	13.500	3865	3875	3887	rBV	10575	19932	1.38%	0.181%
97	14.146	4073	4076	4077	rBV3	591	347	0.02%	0.003%
98	14.181	4084	4087	4092	rBV3	727	574	0.04%	0.005%
99	14.213	4094	4097	4102	rBV4	544	577	0.04%	0.005%
100	14.506	4186	4188	4192	rVB2	972	510	0.04%	0.005%




Sum of corrected areas: 10999263

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028468.D
Acq On : 09 Oct 2022 04:15
Operator : SY/MD
Sample : N4923-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

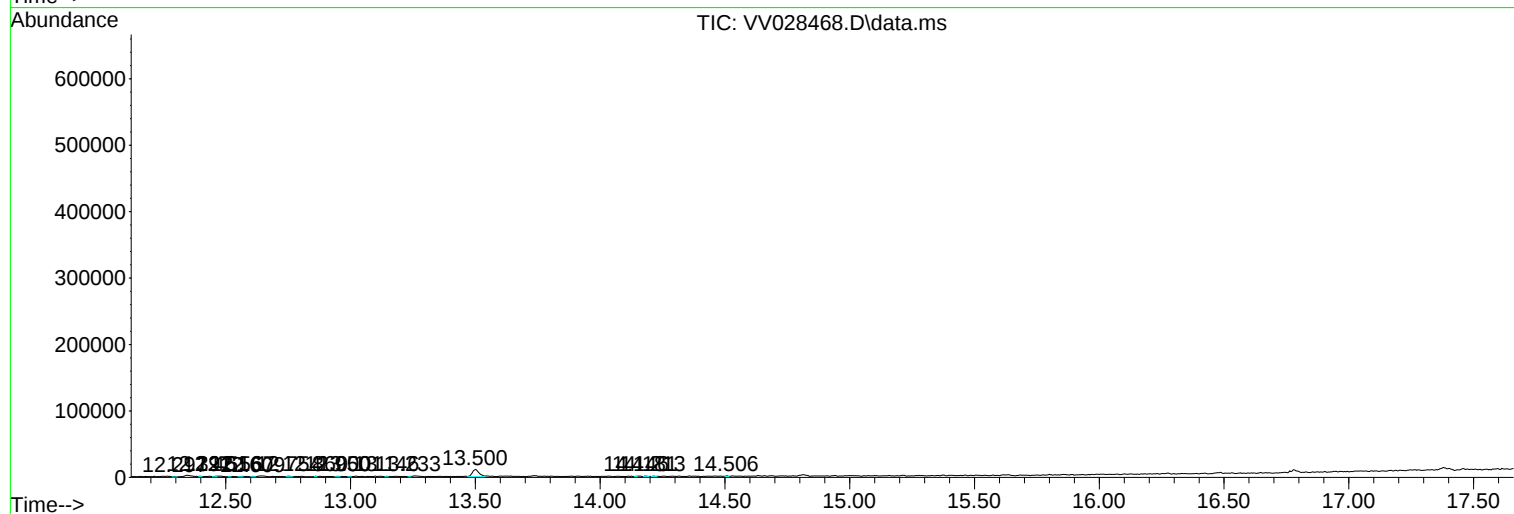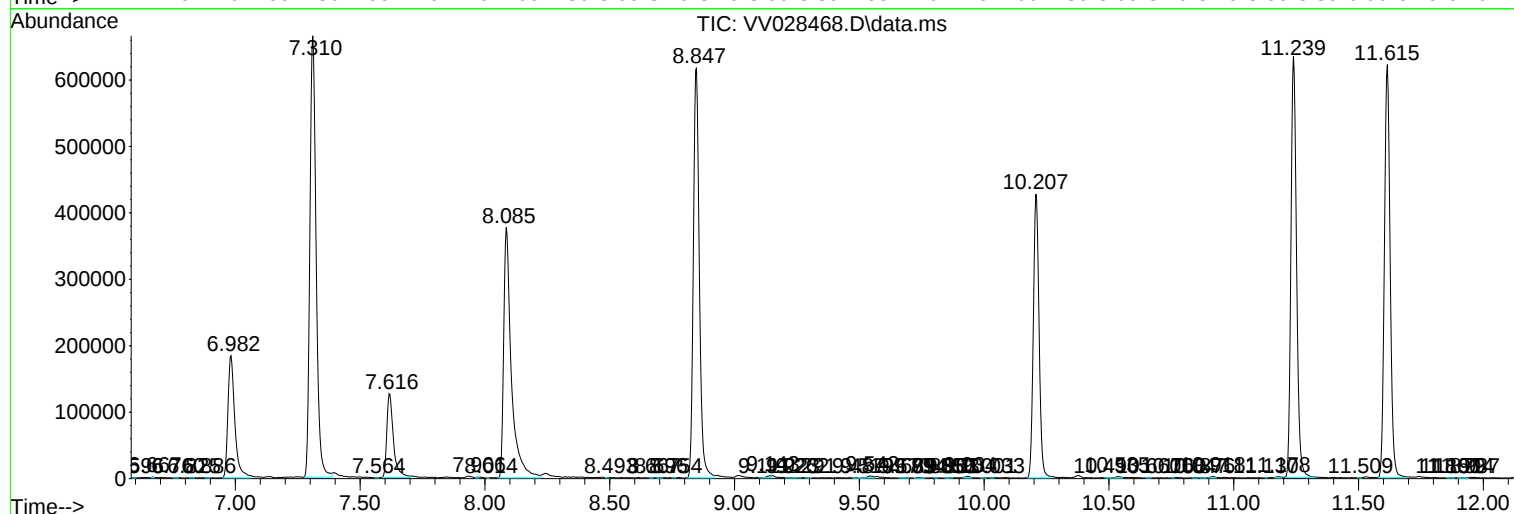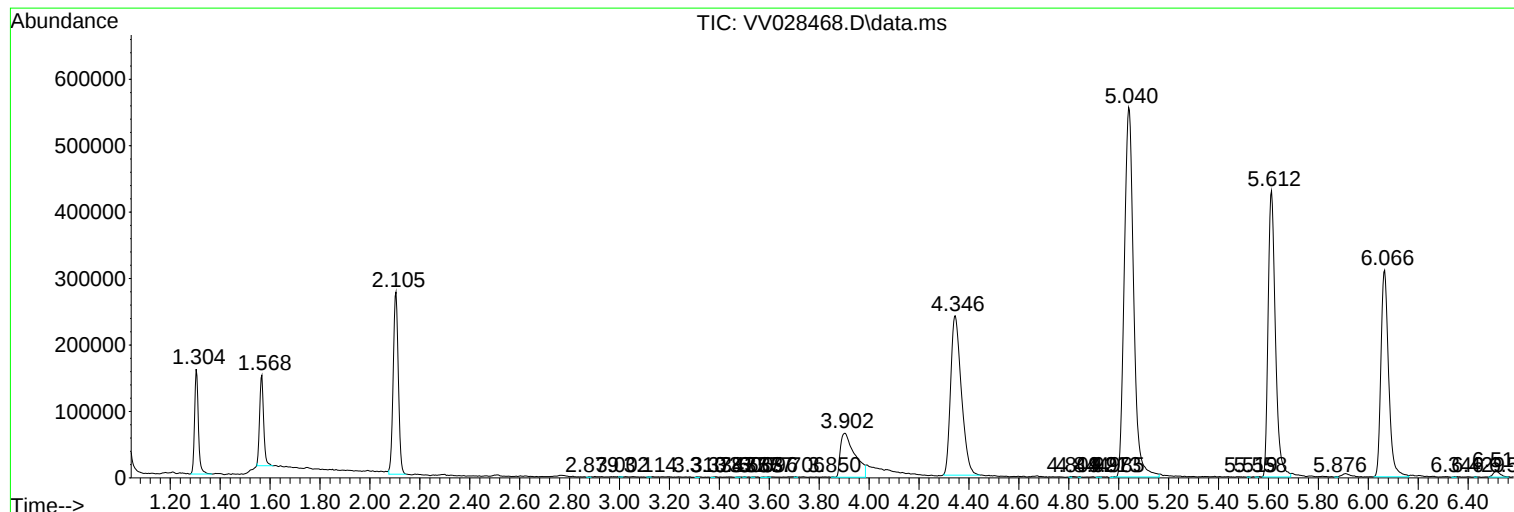

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028468.D
Acq On : 09 Oct 2022 04:15
Operator : SY/MD
Sample : N4923-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028468.D
Acq On : 09 Oct 2022 04:15
Operator : SY/MD
Sample : N4923-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
