

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028469.D
 Acq On : 09 Oct 2022 04:40
 Operator : SY/MD
 Sample : N4923-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10029

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rBV	149517	154062	10.79%	1.427%
2	1.568	158	164	181	rVB	137871	156274	10.94%	1.447%
3	2.104	322	331	349	rVB	267518	388592	27.21%	3.599%
4	3.140	650	653	659	rVB3	566	494	0.03%	0.005%
5	3.166	659	661	666	rBV4	569	404	0.03%	0.004%
6	3.188	666	668	670	rBV2	537	311	0.02%	0.003%
7	3.230	675	681	682	rBV5	737	751	0.05%	0.007%
8	3.320	703	709	710	rBV3	842	732	0.05%	0.007%
9	3.375	723	726	728	rBV3	565	349	0.02%	0.003%
10	3.420	737	740	743	rBV2	374	306	0.02%	0.003%
11	3.619	796	802	804	rBV5	704	716	0.05%	0.007%
12	3.648	808	811	814	rVV4	625	369	0.03%	0.003%
13	3.812	860	862	865	rBV2	360	286	0.02%	0.003%
14	3.860	874	877	881	rBV5	828	878	0.06%	0.008%
15	3.908	881	892	894	rBV	56250	85515	5.99%	0.792%
16	4.346	1014	1028	1059	rVB2	239306	702056	49.16%	6.501%
17	4.702	1138	1139	1144	rBV5	543	289	0.02%	0.003%
18	4.731	1144	1148	1150	rBV3	674	567	0.04%	0.005%
19	4.764	1155	1158	1160	rBV3	761	516	0.04%	0.005%
20	4.796	1164	1168	1171	rBV3	440	305	0.02%	0.003%
21	4.873	1190	1192	1194	rBV3	586	279	0.02%	0.003%
22	4.899	1197	1200	1204	rVV2	755	625	0.04%	0.006%
23	5.040	1226	1244	1277	rBV2	548680	1428024	100.00%	13.224%
24	5.474	1377	1379	1383	rVB3	741	397	0.03%	0.004%
25	5.529	1394	1396	1401	rBV4	618	372	0.03%	0.003%
26	5.612	1410	1422	1454	rBV	435538	890895	62.39%	8.250%
27	5.783	1473	1475	1479	rVB4	967	597	0.04%	0.006%
28	5.911	1503	1515	1524	rBV8	4198	9455	0.66%	0.088%
29	5.972	1532	1534	1538	rBV3	563	335	0.02%	0.003%
30	5.995	1538	1541	1544	rVB4	943	567	0.04%	0.005%
31	6.066	1544	1563	1593	rBV	309635	653333	45.75%	6.050%
32	6.509	1692	1701	1718	rBV3	7982	17753	1.24%	0.164%
33	6.571	1718	1720	1724	rBV3	693	379	0.03%	0.004%
34	6.606	1729	1731	1733	rBV2	560	389	0.03%	0.004%
35	6.664	1747	1749	1751	rBV2	850	455	0.03%	0.004%
36	6.776	1781	1784	1787	rBV3	659	449	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028469.D
 Acq On : 09 Oct 2022 04:40
 Operator : SY/MD
 Sample : N4923-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10029

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.825	1798	1799	1803	rVB	733	335	0.02%	0.003%
38	6.863	1806	1811	1812	rBV2	509	322	0.02%	0.003%
39	6.879	1813	1816	1821	rVB3	657	419	0.03%	0.004%
40	6.982	1835	1848	1872	rBV	182329	345957	24.23%	3.204%
41	7.310	1939	1950	1987	rBV	652679	1137919	79.68%	10.538%
42	7.619	2036	2046	2068	rBV	123614	226186	15.84%	2.095%
43	7.857	2117	2120	2122	rBV2	625	355	0.02%	0.003%
44	8.005	2164	2166	2169	rVB3	600	298	0.02%	0.003%
45	8.088	2181	2192	2224	rBV	370062	765960	53.64%	7.093%
46	8.509	2321	2323	2327	rBV3	527	390	0.03%	0.004%
47	8.590	2346	2348	2350	rBV3	503	317	0.02%	0.003%
48	8.657	2366	2369	2373	rBV4	790	490	0.03%	0.005%
49	8.844	2416	2427	2456	rBV	626842	1034590	72.45%	9.581%
50	9.136	2509	2518	2534	rVB	19111	34542	2.42%	0.320%
51	9.313	2569	2573	2575	rBV3	423	342	0.02%	0.003%
52	9.342	2579	2582	2585	rBV2	920	592	0.04%	0.005%
53	9.509	2630	2634	2635	rBV3	525	390	0.03%	0.004%
54	9.541	2637	2644	2658	rVV2	12546	21113	1.48%	0.196%
55	9.644	2673	2676	2678	rBV	549	366	0.03%	0.003%
56	9.718	2697	2699	2702	rVB4	573	306	0.02%	0.003%
57	9.738	2702	2705	2708	rBV3	594	342	0.02%	0.003%
58	9.779	2713	2718	2721	rVB4	770	488	0.03%	0.005%
59	9.799	2721	2724	2726	rBV2	469	306	0.02%	0.003%
60	9.886	2746	2751	2754	rBV4	696	659	0.05%	0.006%
61	9.966	2774	2776	2779	rBV2	726	483	0.03%	0.004%
62	10.062	2804	2806	2811	rVB3	502	399	0.03%	0.004%
63	10.101	2816	2818	2822	rVB3	588	326	0.02%	0.003%
64	10.123	2822	2825	2827	rBV3	509	300	0.02%	0.003%
65	10.207	2840	2851	2874	rBV	426149	671602	47.03%	6.219%
66	10.332	2887	2890	2892	rBV3	838	467	0.03%	0.004%
67	10.374	2894	2903	2917	rVB3	11903	20923	1.47%	0.194%
68	10.558	2958	2960	2962	rBV2	758	332	0.02%	0.003%
69	10.667	2990	2994	2998	rVB6	493	477	0.03%	0.004%
70	10.770	3021	3026	3027	rBV	693	533	0.04%	0.005%
71	10.812	3036	3039	3041	rBV2	586	373	0.03%	0.003%
72	10.930	3074	3076	3080	rVB4	680	375	0.03%	0.003%
73	11.156	3144	3146	3149	rBV4	744	493	0.03%	0.005%
74	11.239	3161	3172	3200	rVV	642722	1016298	71.17%	9.412%
75	11.538	3254	3265	3269	rBV9	1728	2820	0.20%	0.026%
76	11.615	3277	3289	3308	rBV	612440	985009	68.98%	9.122%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028469.D
 Acq On : 09 Oct 2022 04:40
 Operator : SY/MD
 Sample : N4923-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10029

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.860	3361	3365	3368	rBV4	551	476	0.03%	0.004%
78	11.940	3388	3390	3394	rBV3	551	436	0.03%	0.004%
79	12.014	3410	3413	3416	rVB2	770	395	0.03%	0.004%
80	12.184	3462	3466	3474	rVB7	594	873	0.06%	0.008%
81	12.239	3474	3483	3484	rBV4	2025	1998	0.14%	0.019%
82	12.451	3547	3549	3551	rVB3	693	280	0.02%	0.003%
83	12.471	3551	3555	3556	rVB3	610	316	0.02%	0.003%
84	12.487	3556	3560	3565	rBV4	549	657	0.05%	0.006%
85	12.625	3600	3603	3604	rBV2	637	297	0.02%	0.003%
86	12.657	3609	3613	3615	rBV3	519	411	0.03%	0.004%
87	12.715	3628	3631	3634	rBV3	482	299	0.02%	0.003%
88	12.731	3634	3636	3639	rBV3	630	363	0.03%	0.003%
89	12.840	3667	3670	3674	rBV4	433	336	0.02%	0.003%
90	12.869	3676	3679	3681	rBV2	452	285	0.02%	0.003%
91	12.956	3704	3706	3709	rBV2	580	388	0.03%	0.004%
92	12.972	3709	3711	3714	rBV2	744	482	0.03%	0.004%
93	13.136	3757	3762	3763	rBV3	572	422	0.03%	0.004%
94	13.432	3851	3854	3858	rBV4	805	798	0.06%	0.007%
95	13.503	3870	3876	3892	rVB2	7672	13943	0.98%	0.129%
96	13.741	3947	3950	3953	rBV4	811	668	0.05%	0.006%
97	13.779	3960	3962	3967	rVB5	759	621	0.04%	0.006%
98	13.850	3982	3984	3987	rBV3	508	337	0.02%	0.003%
99	13.972	4019	4022	4028	rBV3	597	647	0.05%	0.006%
100	14.184	4085	4088	4090	rBV2	496	417	0.03%	0.004%




Sum of corrected areas: 10798415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028469.D
Acq On : 09 Oct 2022 04:40
Operator : SY/MD
Sample : N4923-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10029

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

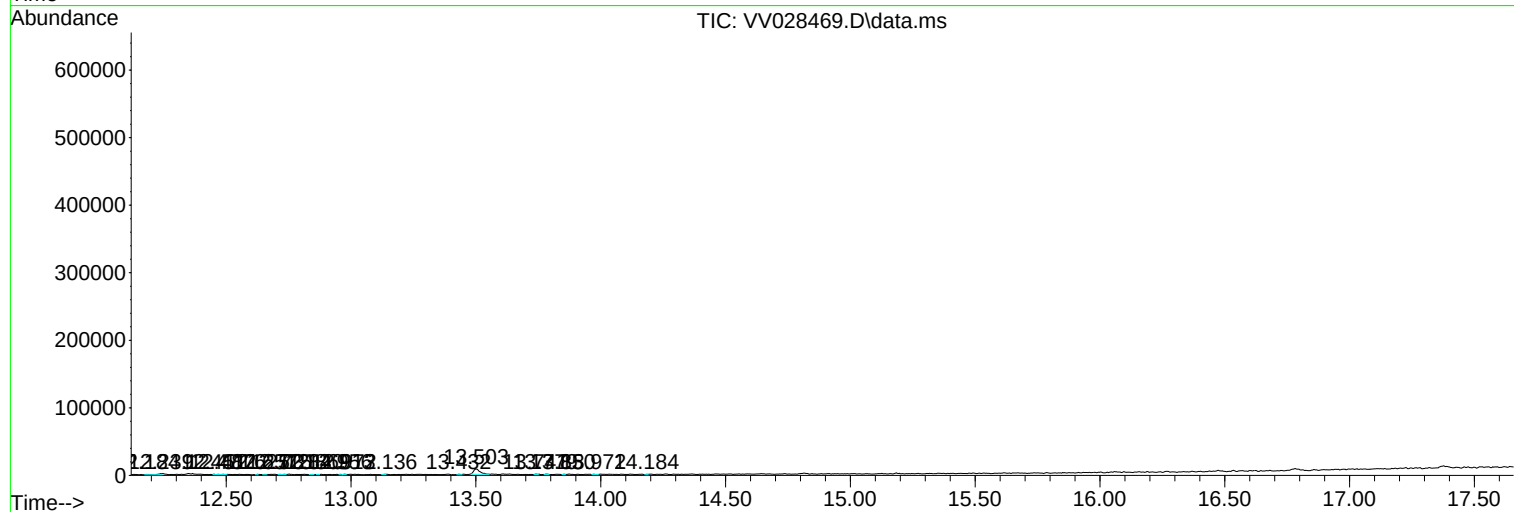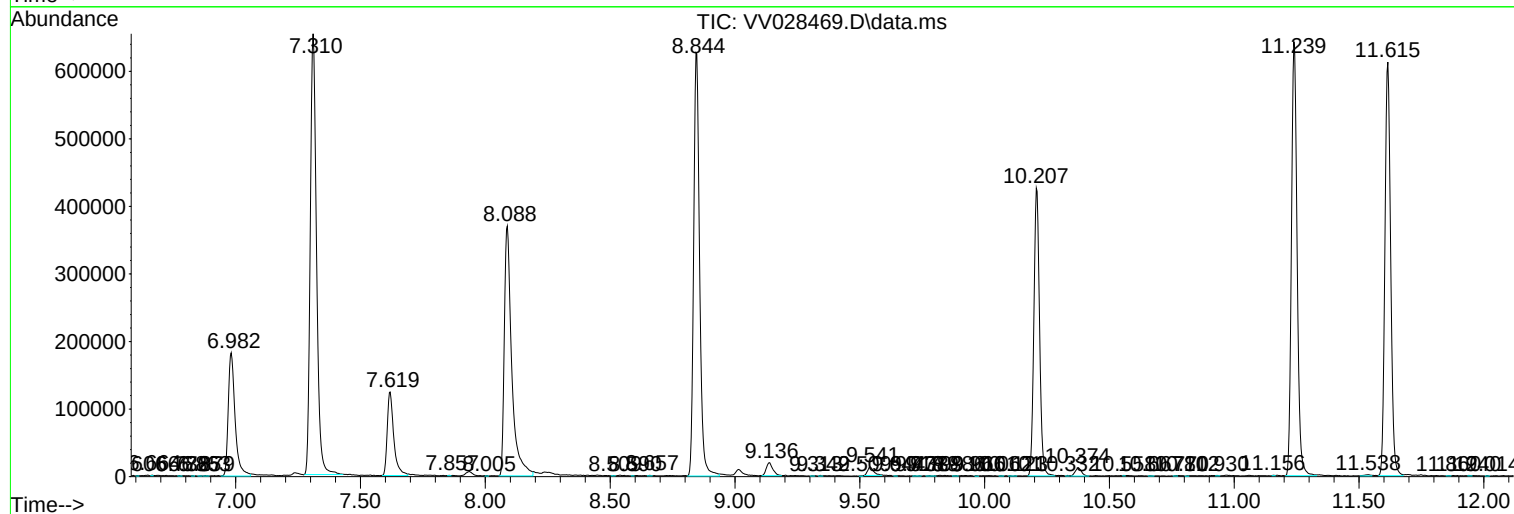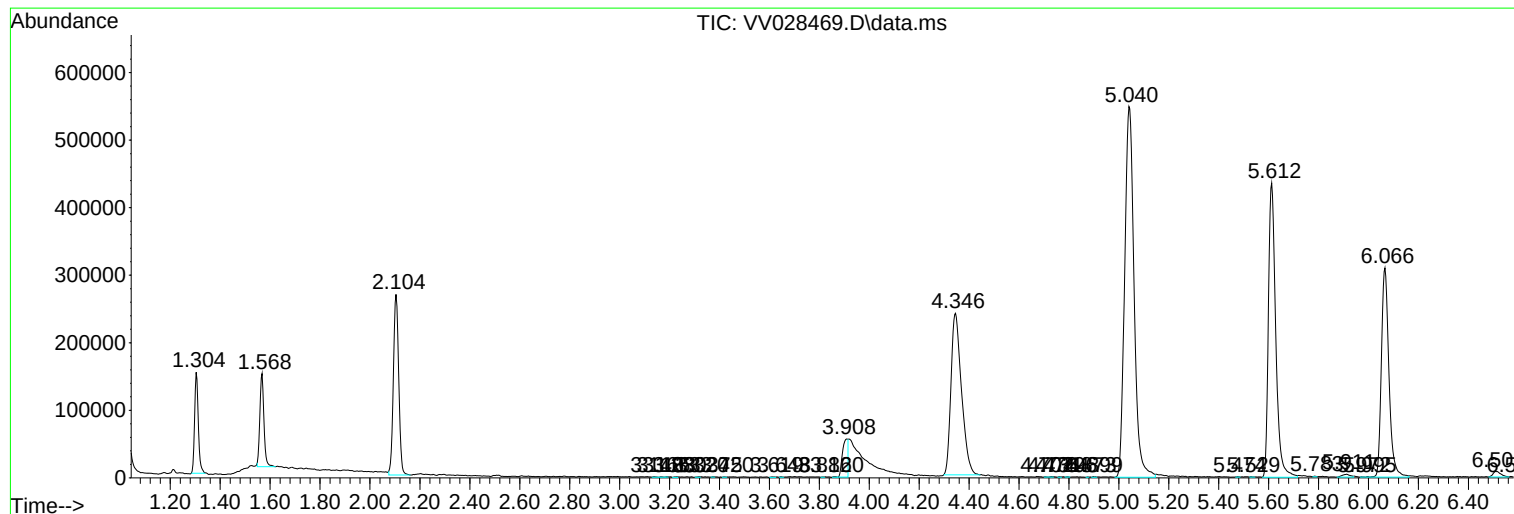

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028469.D
Acq On : 09 Oct 2022 04:40
Operator : SY/MD
Sample : N4923-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10029

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028469.D
Acq On : 09 Oct 2022 04:40
Operator : SY/MD
Sample : N4923-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10029

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc