

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028470.D
 Acq On : 09 Oct 2022 05:04
 Operator : SY/MD
 Sample : N4923-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	158065	164623	11.61%	1.558%
2	1.565	158	163	176	rVB	130077	146419	10.32%	1.386%
3	2.105	323	331	347	rVB	267818	389596	27.47%	3.687%
4	2.674	506	508	513	rVB5	957	587	0.04%	0.006%
5	2.799	544	547	549	rBV2	641	448	0.03%	0.004%
6	2.857	562	565	569	rVB2	816	426	0.03%	0.004%
7	2.876	569	571	574	rBV2	859	610	0.04%	0.006%
8	3.008	609	612	614	rBV3	664	383	0.03%	0.004%
9	3.192	667	669	671	rBV	642	399	0.03%	0.004%
10	3.230	679	681	683	rBV3	886	543	0.04%	0.005%
11	3.294	698	701	705	rVB4	555	421	0.03%	0.004%
12	3.317	705	708	710	rBV2	535	333	0.02%	0.003%
13	3.555	779	782	785	rBV3	758	458	0.03%	0.004%
14	3.590	791	793	796	rBV3	568	323	0.02%	0.003%
15	3.732	833	837	841	rBV4	708	654	0.05%	0.006%
16	3.770	846	849	853	rVB5	602	480	0.03%	0.005%
17	3.796	853	857	859	rBV2	793	528	0.04%	0.005%
18	3.902	879	890	929	rBV	60846	268441	18.93%	2.540%
19	4.343	1012	1027	1050	rBV	217515	546356	38.52%	5.170%
20	4.619	1109	1113	1115	rVB3	495	352	0.02%	0.003%
21	4.677	1129	1131	1135	rBV3	443	361	0.03%	0.003%
22	4.822	1170	1176	1178	rBV2	517	480	0.03%	0.005%
23	4.954	1211	1217	1219	rBV4	643	500	0.04%	0.005%
24	5.040	1224	1244	1286	rBV2	541527	1418381	100.00%	13.422%
25	5.375	1344	1348	1353	rBV5	845	1003	0.07%	0.009%
26	5.613	1410	1422	1455	rBV	424384	869054	61.27%	8.224%
27	6.066	1546	1563	1590	rBV	309447	652300	45.99%	6.173%
28	6.413	1669	1671	1675	rBV4	675	401	0.03%	0.004%
29	6.503	1693	1699	1701	rBV3	1377	1222	0.09%	0.012%
30	6.558	1713	1716	1719	rBV4	632	450	0.03%	0.004%
31	6.651	1742	1745	1747	rBV2	836	593	0.04%	0.006%
32	6.879	1813	1816	1819	rBV3	592	452	0.03%	0.004%
33	6.982	1837	1848	1875	rBV	182128	344692	24.30%	3.262%
34	7.169	1903	1906	1910	rBV5	804	742	0.05%	0.007%
35	7.310	1938	1950	1976	rBV	641032	1127266	79.48%	10.667%
36	7.558	2023	2027	2029	rBV3	670	455	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100822\
 Data File : VW028470.D
 Acq On : 09 Oct 2022 05:04
 Operator : SY/MD
 Sample : N4923-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.616	2035	2045	2077	rBV	121979	228773	16.13%	2.165%
38	7.934	2134	2144	2155	rVB3	7244	12471	0.88%	0.118%
39	8.085	2181	2191	2226	rBV	341533	700728	49.40%	6.631%
40	8.568	2338	2341	2344	rBV2	856	725	0.05%	0.007%
41	8.844	2414	2427	2453	rBV	608929	1018357	71.80%	9.637%
42	9.066	2493	2496	2498	rBV4	679	477	0.03%	0.005%
43	9.268	2557	2559	2565	rVB3	793	631	0.04%	0.006%
44	9.323	2573	2576	2580	rVB4	723	574	0.04%	0.005%
45	9.346	2580	2583	2586	rBV2	464	358	0.03%	0.003%
46	9.384	2591	2595	2597	rBV3	530	332	0.02%	0.003%
47	9.513	2628	2635	2637	rVB4	679	518	0.04%	0.005%
48	9.535	2637	2642	2645	rBV3	742	732	0.05%	0.007%
49	9.555	2645	2648	2651	rVV3	490	352	0.02%	0.003%
50	9.641	2670	2675	2676	rBV3	542	312	0.02%	0.003%
51	9.850	2735	2740	2741	rBV3	691	571	0.04%	0.005%
52	9.892	2750	2753	2756	rVB3	433	309	0.02%	0.003%
53	9.931	2761	2765	2766	rBV3	523	405	0.03%	0.004%
54	10.011	2788	2790	2794	rVV2	658	491	0.03%	0.005%
55	10.050	2798	2802	2804	rBV3	665	340	0.02%	0.003%
56	10.156	2828	2835	2839	rBV4	688	909	0.06%	0.009%
57	10.207	2839	2851	2871	rBV	406106	652841	46.03%	6.178%
58	10.378	2896	2904	2913	rVB2	10635	14832	1.05%	0.140%
59	10.442	2921	2924	2926	rVB2	545	332	0.02%	0.003%
60	10.468	2926	2932	2935	rBV2	574	676	0.05%	0.006%
61	10.526	2946	2950	2953	rBV2	573	444	0.03%	0.004%
62	10.551	2953	2958	2962	rBV5	890	714	0.05%	0.007%
63	10.574	2962	2965	2966	rBV4	508	319	0.02%	0.003%
64	10.622	2976	2980	2982	rBV2	583	427	0.03%	0.004%
65	10.725	3010	3012	3017	rVV4	492	318	0.02%	0.003%
66	10.773	3020	3027	3029	rBV6	790	694	0.05%	0.007%
67	10.863	3053	3055	3061	rVB3	724	490	0.03%	0.005%
68	10.911	3067	3070	3076	rBV4	771	608	0.04%	0.006%
69	10.979	3086	3091	3092	rBV3	448	353	0.02%	0.003%
70	11.018	3098	3103	3106	rBV2	651	473	0.03%	0.004%
71	11.072	3117	3120	3123	rBV4	623	328	0.02%	0.003%
72	11.114	3131	3133	3137	rBV2	430	322	0.02%	0.003%
73	11.159	3143	3147	3149	rBV2	470	402	0.03%	0.004%
74	11.239	3159	3172	3201	rBV	616667	979391	69.05%	9.268%
75	11.436	3231	3233	3242	rVB7	692	780	0.05%	0.007%
76	11.516	3256	3258	3260	rBV3	556	372	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028470.D
 Acq On : 09 Oct 2022 05:04
 Operator : SY/MD
 Sample : N4923-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.616	3277	3289	3311	rBV	625897	977491	68.92%	9.250%
78	11.834	3355	3357	3361	rVB3	574	338	0.02%	0.003%
79	12.059	3423	3427	3432	rBV4	612	496	0.03%	0.005%
80	12.130	3445	3449	3451	rBV3	562	375	0.03%	0.004%
81	12.243	3478	3484	3490	rBV6	1760	2346	0.17%	0.022%
82	12.307	3500	3504	3506	rBV4	588	413	0.03%	0.004%
83	12.362	3519	3521	3523	rBV2	649	382	0.03%	0.004%
84	12.432	3540	3543	3544	rBV2	650	398	0.03%	0.004%
85	12.577	3584	3588	3590	rVB4	564	418	0.03%	0.004%
86	12.661	3611	3614	3617	rVB2	791	473	0.03%	0.004%
87	12.683	3617	3621	3625	rVB5	768	581	0.04%	0.005%
88	12.870	3676	3679	3681	rBV2	619	390	0.03%	0.004%
89	12.889	3683	3685	3687	rBV2	671	357	0.03%	0.003%
90	12.921	3692	3695	3698	rBV3	651	367	0.03%	0.003%
91	13.024	3725	3727	3732	rVB4	763	521	0.04%	0.005%
92	13.053	3732	3736	3737	rBV	919	596	0.04%	0.006%
93	13.198	3777	3781	3784	rVB5	647	465	0.03%	0.004%
94	13.313	3813	3817	3819	rBV3	499	395	0.03%	0.004%
95	13.349	3824	3828	3832	rVB6	771	707	0.05%	0.007%
96	13.374	3832	3836	3839	rBV3	892	726	0.05%	0.007%
97	13.500	3865	3875	3886	rBV2	6981	12823	0.90%	0.121%
98	14.336	4133	4135	4138	rVB2	779	373	0.03%	0.004%
99	14.365	4138	4144	4147	rBV5	817	928	0.07%	0.009%
100	14.802	4278	4280	4283	rBV4	1147	828	0.06%	0.008%




Sum of corrected areas: 10567400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028470.D
Acq On : 09 Oct 2022 05:04
Operator : SY/MD
Sample : N4923-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

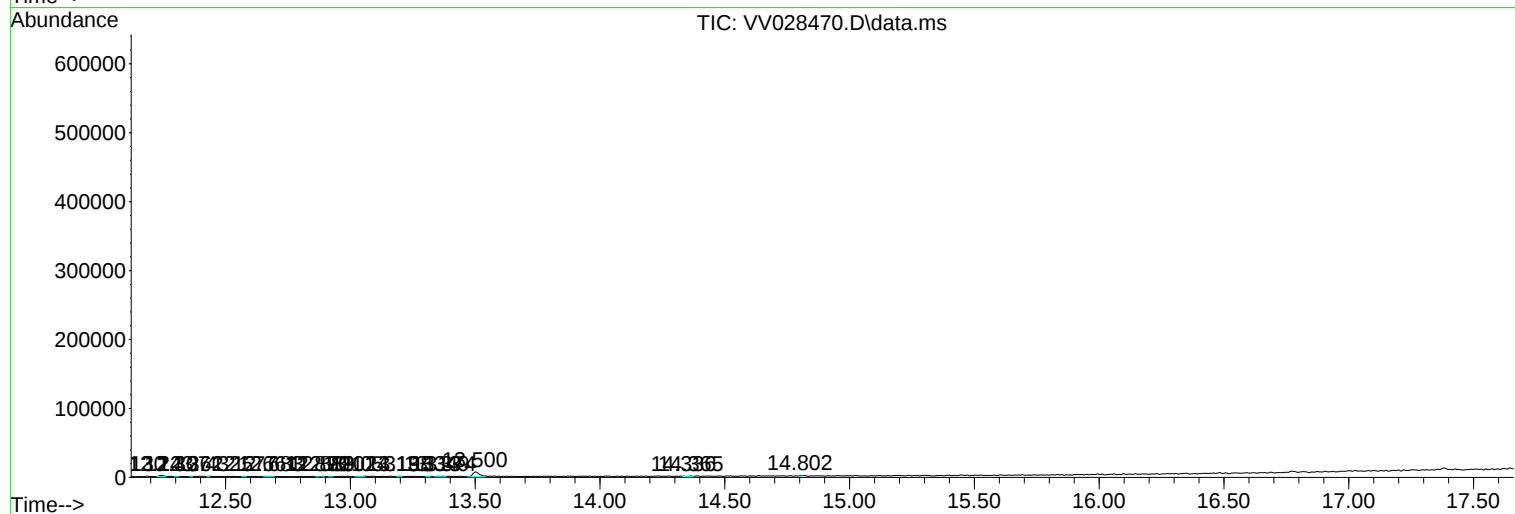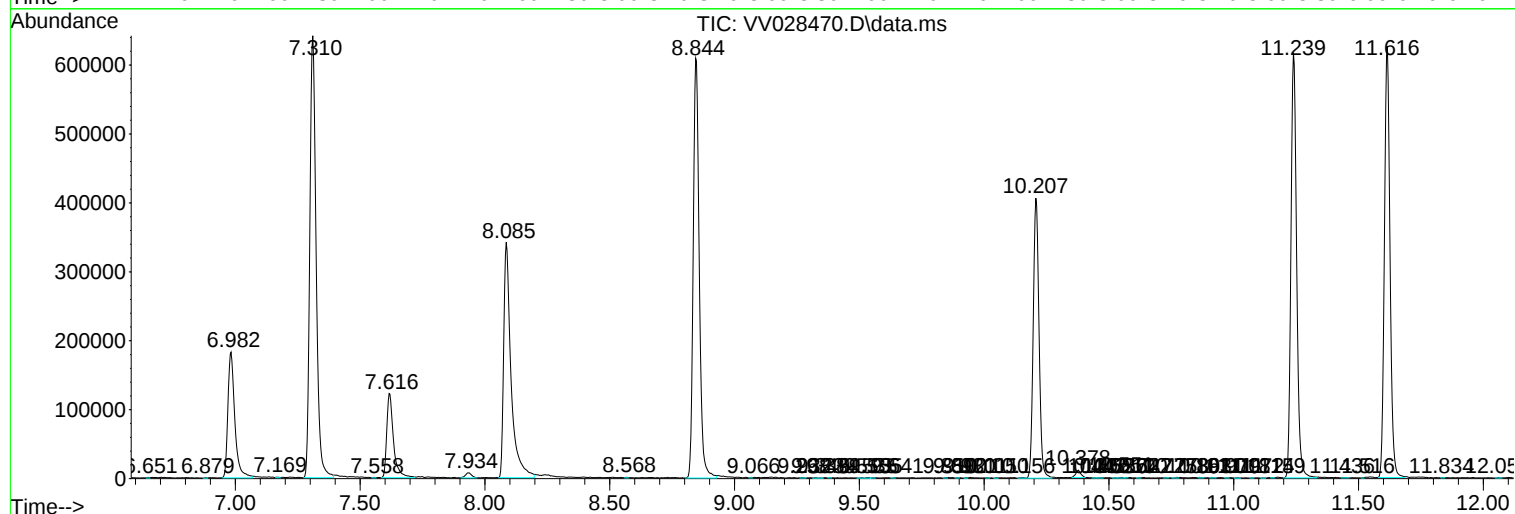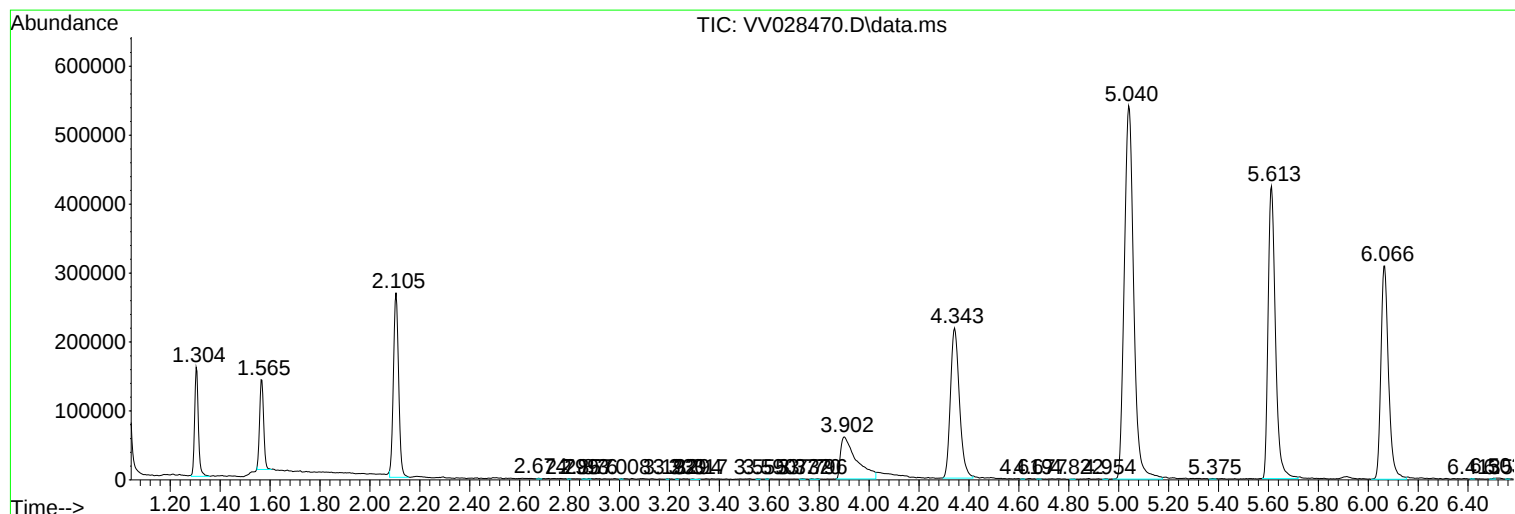

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028470.D
Acq On : 09 Oct 2022 05:04
Operator : SY/MD
Sample : N4923-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028470.D
Acq On : 09 Oct 2022 05:04
Operator : SY/MD
Sample : N4923-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc