

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028471.D
 Acq On : 09 Oct 2022 05:28
 Operator : SY/MD
 Sample : N4923-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	152710	162901	11.61%	1.526%
2	1.568	157	164	178	rBV	134289	155299	11.07%	1.455%
3	2.105	322	331	345	rVB	257850	367228	26.17%	3.440%
4	3.198	669	671	673	rBV3	465	233	0.02%	0.002%
5	3.259	688	690	693	rBV3	562	306	0.02%	0.003%
6	3.320	707	709	713	rBV2	400	260	0.02%	0.002%
7	3.535	773	776	778	rBV2	499	305	0.02%	0.003%
8	3.551	778	781	784	rVB3	675	371	0.03%	0.003%
9	3.748	840	842	845	rBV3	649	365	0.03%	0.003%
10	3.902	880	890	928	rBV	61998	287946	20.52%	2.697%
11	4.346	1013	1028	1059	rVB4	233830	683977	48.74%	6.406%
12	4.719	1140	1144	1146	rBV3	469	252	0.02%	0.002%
13	4.748	1149	1153	1158	rVB4	770	795	0.06%	0.007%
14	4.773	1158	1161	1162	rBV	442	206	0.01%	0.002%
15	4.822	1173	1176	1178	rBV2	614	421	0.03%	0.004%
16	4.915	1203	1205	1207	rBV2	603	254	0.02%	0.002%
17	5.040	1228	1244	1275	rBV2	538451	1403244	100.00%	13.143%
18	5.394	1352	1354	1356	rVB2	729	233	0.02%	0.002%
19	5.612	1410	1422	1451	rBV	417077	849707	60.55%	7.958%
20	6.066	1549	1563	1591	rBV	307558	640839	45.67%	6.002%
21	6.420	1671	1673	1677	rVB3	1040	514	0.04%	0.005%
22	6.442	1678	1680	1684	rBV3	670	474	0.03%	0.004%
23	6.513	1695	1702	1715	rVB3	7931	15810	1.13%	0.148%
24	6.629	1736	1738	1741	rBV2	555	381	0.03%	0.004%
25	6.773	1781	1783	1785	rBV2	563	335	0.02%	0.003%
26	6.818	1793	1797	1799	rBV4	580	363	0.03%	0.003%
27	6.982	1836	1848	1873	rBV2	181071	343951	24.51%	3.221%
28	7.310	1939	1950	1972	rBV	645245	1117432	79.63%	10.466%
29	7.616	2036	2045	2070	rBV	122603	221430	15.78%	2.074%
30	7.834	2111	2113	2116	rVB3	447	217	0.02%	0.002%
31	7.927	2137	2142	2144	rBV4	1931	1939	0.14%	0.018%
32	8.014	2167	2169	2172	rVB3	443	173	0.01%	0.002%
33	8.053	2177	2181	2182	rBV3	727	544	0.04%	0.005%
34	8.085	2182	2191	2226	rBV	367590	749134	53.39%	7.016%
35	8.403	2288	2290	2294	rBV4	874	693	0.05%	0.006%
36	8.561	2338	2339	2343	rVB4	713	269	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100822\
 Data File : VW028471.D
 Acq On : 09 Oct 2022 05:28
 Operator : SY/MD
 Sample : N4923-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	8.580	2343	2345	2346	rBV2	416	183	0.01%	0.002%
38	8.632	2359	2361	2367	rVB3	1101	766	0.05%	0.007%
39	8.706	2381	2384	2390	rVB4	877	758	0.05%	0.007%
40	8.844	2416	2427	2462	rBV	588420	988104	70.42%	9.255%
41	9.014	2471	2480	2487	rBV	9108	14715	1.05%	0.138%
42	9.136	2509	2518	2531	rBV	16871	30511	2.17%	0.286%
43	9.326	2574	2577	2581	rBV2	794	528	0.04%	0.005%
44	9.349	2581	2584	2588	rVB4	779	624	0.04%	0.006%
45	9.368	2588	2590	2591	rBV	366	202	0.01%	0.002%
46	9.407	2600	2602	2607	rBV2	303	237	0.02%	0.002%
47	9.445	2610	2614	2619	rBV4	445	373	0.03%	0.003%
48	9.477	2622	2624	2626	rBV	542	254	0.02%	0.002%
49	9.538	2636	2643	2657	rBV3	11236	19884	1.42%	0.186%
50	9.641	2670	2675	2682	rBV4	1116	1272	0.09%	0.012%
51	9.738	2703	2705	2707	rBV2	527	317	0.02%	0.003%
52	9.754	2709	2710	2714	rVV2	805	347	0.02%	0.003%
53	9.786	2717	2720	2722	rBV3	461	325	0.02%	0.003%
54	9.924	2760	2763	2765	rBV3	844	572	0.04%	0.005%
55	9.988	2780	2783	2785	rBV	721	483	0.03%	0.005%
56	10.040	2796	2799	2804	rBV3	580	509	0.04%	0.005%
57	10.075	2807	2810	2814	rBV4	815	789	0.06%	0.007%
58	10.149	2832	2833	2835	rVB	551	155	0.01%	0.001%
59	10.207	2839	2851	2870	rBV2	410887	656486	46.78%	6.149%
60	10.378	2896	2904	2911	rVV5	2914	5238	0.37%	0.049%
61	10.461	2928	2930	2934	rVB3	636	334	0.02%	0.003%
62	10.574	2961	2965	2968	rBV3	795	691	0.05%	0.006%
63	10.615	2974	2978	2980	rVB4	462	354	0.03%	0.003%
64	10.683	2997	2999	3000	rBV	613	253	0.02%	0.002%
65	10.709	3006	3007	3013	rVB3	605	407	0.03%	0.004%
66	10.734	3013	3015	3017	rBV	265	186	0.01%	0.002%
67	10.796	3032	3034	3036	rBV	451	243	0.02%	0.002%
68	11.053	3110	3114	3117	rBV4	830	748	0.05%	0.007%
69	11.239	3161	3172	3194	rBV	619975	957235	68.22%	8.966%
70	11.487	3247	3249	3251	rBV	293	179	0.01%	0.002%
71	11.513	3255	3257	3258	rBV	482	200	0.01%	0.002%
72	11.615	3277	3289	3311	rBV	609414	963428	68.66%	9.024%
73	11.792	3340	3344	3348	rBV4	329	367	0.03%	0.003%
74	11.940	3384	3390	3392	rBV4	873	874	0.06%	0.008%
75	11.985	3400	3404	3406	rBV3	491	432	0.03%	0.004%
76	12.021	3412	3415	3418	rVB3	657	341	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028471.D
 Acq On : 09 Oct 2022 05:28
 Operator : SY/MD
 Sample : N4923-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E10027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.098	3437	3439	3441	rBV2	395	175	0.01%	0.002%
78	12.111	3441	3443	3444	rBV	430	187	0.01%	0.002%
79	12.320	3506	3508	3509	rBV	654	327	0.02%	0.003%
80	12.516	3568	3569	3571	rBV2	526	242	0.02%	0.002%
81	12.561	3581	3583	3586	rBV2	448	182	0.01%	0.002%
82	12.574	3586	3587	3590	rBV2	371	227	0.02%	0.002%
83	12.667	3614	3616	3618	rVB2	759	363	0.03%	0.003%
84	12.689	3618	3623	3625	rBV2	517	527	0.04%	0.005%
85	12.715	3628	3631	3635	rBV3	615	433	0.03%	0.004%
86	12.760	3643	3645	3649	rVB3	954	668	0.05%	0.006%
87	12.786	3649	3653	3654	rBV3	660	477	0.03%	0.004%
88	12.873	3677	3680	3681	rBV	396	222	0.02%	0.002%
89	12.966	3706	3709	3712	rBV3	580	398	0.03%	0.004%
90	12.998	3716	3719	3723	rBV3	714	567	0.04%	0.005%
91	13.117	3754	3756	3760	rBV3	514	294	0.02%	0.003%
92	13.149	3764	3766	3769	rBV2	533	288	0.02%	0.003%
93	13.204	3780	3783	3786	rBV2	527	396	0.03%	0.004%
94	13.255	3797	3799	3800	rBV	546	230	0.02%	0.002%
95	13.500	3869	3875	3892	rVB3	5398	9979	0.71%	0.093%
96	13.606	3906	3908	3910	rBV2	606	287	0.02%	0.003%
97	13.738	3947	3949	3957	rBV6	653	661	0.05%	0.006%
98	13.802	3966	3969	3970	rBV2	644	396	0.03%	0.004%
99	14.143	4074	4075	4076	rBV	486	176	0.01%	0.002%
100	14.233	4101	4103	4105	rBV	834	376	0.03%	0.004%




Sum of corrected areas: 10676783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028471.D
Acq On : 09 Oct 2022 05:28
Operator : SY/MD
Sample : N4923-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

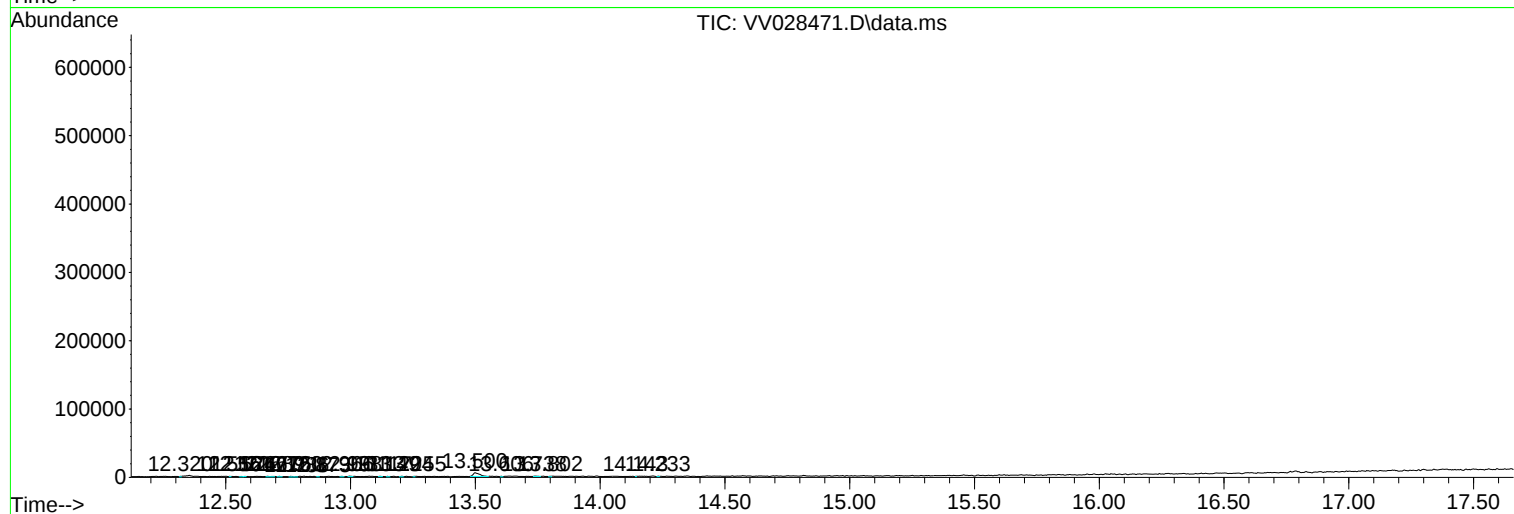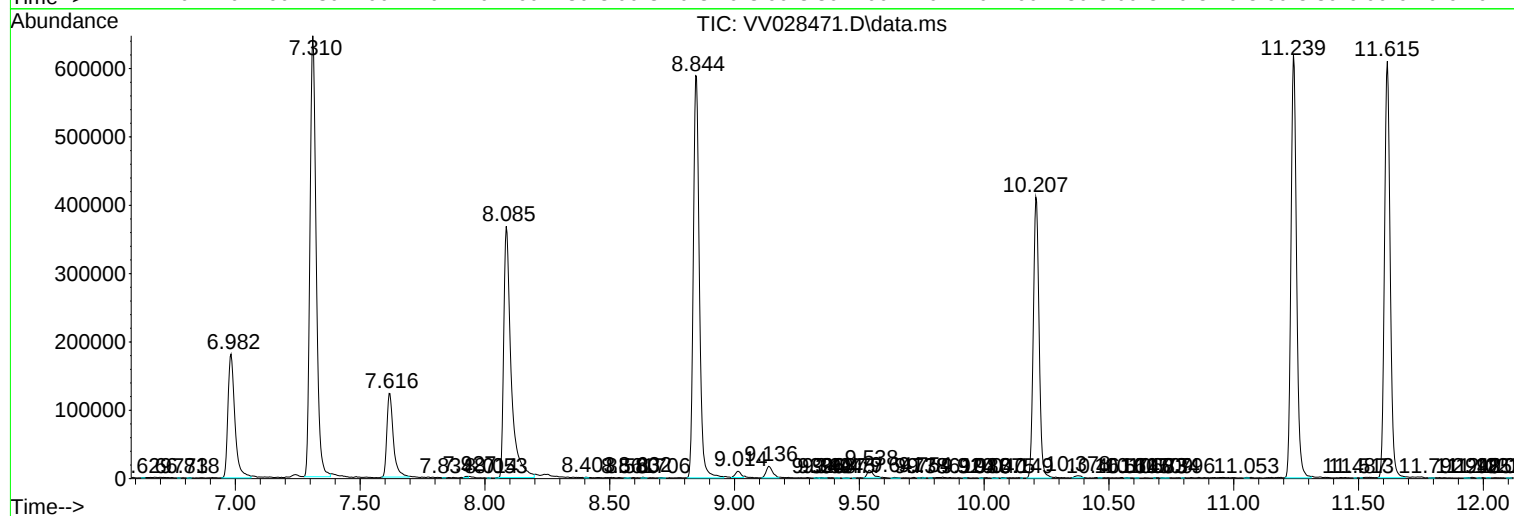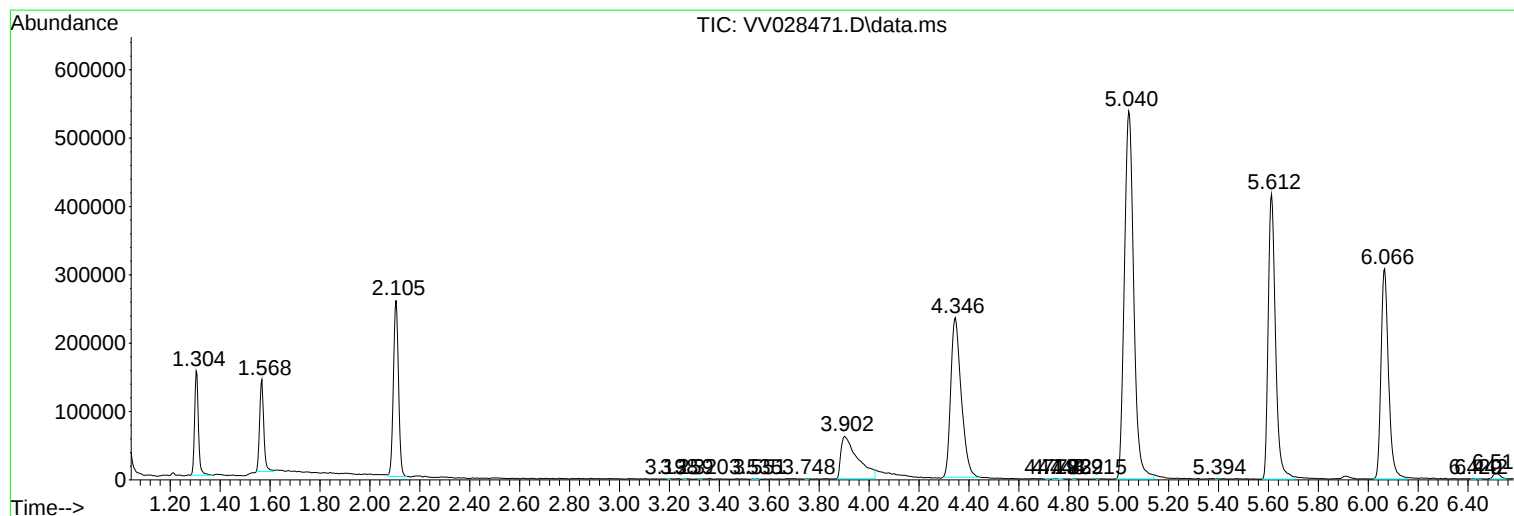

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028471.D
Acq On : 09 Oct 2022 05:28
Operator : SY/MD
Sample : N4923-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028471.D
Acq On : 09 Oct 2022 05:28
Operator : SY/MD
Sample : N4923-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E10027

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------