

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028478.D
 Acq On : 09 Oct 2022 11:48
 Operator : SY/MD
 Sample : VV1008WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	99	rVB	258201	267841	14.57%	2.020%
2	1.568	157	164	179	rVB	196785	232716	12.66%	1.755%
3	2.104	321	331	349	rVB	407413	597492	32.49%	4.506%
4	2.281	382	386	387	rBV4	1430	1065	0.06%	0.008%
5	2.291	387	389	396	rVB4	2275	1847	0.10%	0.014%
6	2.342	403	405	409	rBV4	1032	929	0.05%	0.007%
7	2.506	449	456	463	rVB7	1927	3085	0.17%	0.023%
8	2.551	467	470	471	rBV3	826	500	0.03%	0.004%
9	2.815	549	552	556	rVB4	775	659	0.04%	0.005%
10	2.934	587	589	592	rBV2	876	534	0.03%	0.004%
11	3.082	631	635	637	rBV3	608	443	0.02%	0.003%
12	3.149	652	656	661	rVB5	1351	1265	0.07%	0.010%
13	3.172	661	663	668	rVB3	963	561	0.03%	0.004%
14	3.416	734	739	743	rVV4	543	551	0.03%	0.004%
15	3.461	748	753	756	rVB5	979	726	0.04%	0.005%
16	3.744	839	841	845	rVB4	755	478	0.03%	0.004%
17	3.789	850	855	856	rBV2	564	477	0.03%	0.004%
18	3.895	877	888	933	rBV2	81182	382397	20.79%	2.884%
19	4.336	1009	1025	1054	rVV	277212	699857	38.06%	5.278%
20	4.622	1111	1114	1115	rBV3	845	484	0.03%	0.004%
21	4.699	1135	1138	1145	rVV6	845	768	0.04%	0.006%
22	4.789	1161	1166	1170	rBV4	692	749	0.04%	0.006%
23	4.921	1202	1207	1209	rBV5	761	642	0.03%	0.005%
24	4.953	1213	1217	1219	rBV3	692	549	0.03%	0.004%
25	5.037	1225	1243	1278	rBV2	704946	1838897	100.00%	13.868%
26	5.278	1315	1318	1323	rVB5	968	774	0.04%	0.006%
27	5.394	1350	1354	1356	rBV6	680	527	0.03%	0.004%
28	5.436	1363	1367	1370	rVB4	583	451	0.02%	0.003%
29	5.477	1376	1380	1381	rBV	854	503	0.03%	0.004%
30	5.606	1407	1420	1445	rBV	456208	924819	50.29%	6.975%
31	5.905	1502	1513	1514	rBV7	3442	4998	0.27%	0.038%
32	5.982	1532	1537	1538	rBV3	781	626	0.03%	0.005%
33	6.059	1547	1561	1586	rBV	395549	809242	44.01%	6.103%
34	6.323	1640	1643	1647	rVB4	1001	883	0.05%	0.007%
35	6.349	1647	1651	1652	rBV2	876	592	0.03%	0.004%
36	6.480	1689	1692	1696	rVB3	759	519	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028478.D
 Acq On : 09 Oct 2022 11:48
 Operator : SY/MD
 Sample : VV1008WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.609	1729	1732	1735	rVB4	745	447	0.02%	0.003%
38	6.699	1757	1760	1762	rBV2	778	508	0.03%	0.004%
39	6.808	1792	1794	1800	rBV5	872	840	0.05%	0.006%
40	6.976	1834	1846	1875	rBV	248122	461954	25.12%	3.484%
41	7.101	1883	1885	1889	rVB2	1219	669	0.04%	0.005%
42	7.201	1911	1916	1920	rVB5	756	801	0.04%	0.006%
43	7.307	1936	1949	1969	rBV	859955	1488503	80.95%	11.226%
44	7.542	2020	2022	2029	rVB6	919	831	0.05%	0.006%
45	7.612	2032	2044	2065	rBV	169149	304716	16.57%	2.298%
46	7.870	2122	2124	2128	rVB3	661	471	0.03%	0.004%
47	7.915	2131	2138	2141	rBV5	861	1197	0.07%	0.009%
48	7.934	2141	2144	2148	rBV4	1125	804	0.04%	0.006%
49	7.972	2152	2156	2161	rVB4	733	655	0.04%	0.005%
50	8.082	2176	2190	2223	rBV	445923	852242	46.35%	6.427%
51	8.580	2343	2345	2349	rBV2	684	476	0.03%	0.004%
52	8.632	2358	2361	2363	rBV	837	592	0.03%	0.004%
53	8.844	2414	2427	2449	rBV	639855	1062449	57.78%	8.013%
54	9.123	2511	2514	2517	rBV3	965	814	0.04%	0.006%
55	9.143	2517	2520	2524	rVV4	991	896	0.05%	0.007%
56	9.233	2546	2548	2553	rVV3	669	469	0.03%	0.004%
57	9.262	2553	2557	2562	rVV5	1027	949	0.05%	0.007%
58	9.487	2622	2627	2631	rBV4	525	525	0.03%	0.004%
59	9.532	2637	2641	2645	rBV4	1082	1017	0.06%	0.008%
60	9.551	2645	2647	2648	rVV	838	444	0.02%	0.003%
61	9.561	2648	2650	2659	rVB8	1356	1783	0.10%	0.013%
62	9.606	2659	2664	2665	rBV4	735	678	0.04%	0.005%
63	9.731	2701	2703	2709	rVB2	664	574	0.03%	0.004%
64	9.779	2715	2718	2722	rBV4	856	751	0.04%	0.006%
65	9.808	2724	2727	2733	rBV4	625	489	0.03%	0.004%
66	9.979	2776	2780	2784	rVB2	774	556	0.03%	0.004%
67	10.001	2784	2787	2789	rBV3	654	512	0.03%	0.004%
68	10.046	2795	2801	2805	rBV3	563	617	0.03%	0.005%
69	10.152	2831	2834	2837	rBV2	734	446	0.02%	0.003%
70	10.207	2837	2851	2879	rVV	500559	786310	42.76%	5.930%
71	10.377	2897	2904	2906	rBV4	1723	2018	0.11%	0.015%
72	10.535	2950	2953	2956	rBV3	674	500	0.03%	0.004%
73	10.638	2983	2985	2988	rBV2	696	489	0.03%	0.004%
74	10.914	3068	3071	3073	rBV4	937	559	0.03%	0.004%
75	10.982	3087	3092	3098	rBV6	708	903	0.05%	0.007%
76	11.017	3101	3103	3107	rBV4	736	526	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028478.D
 Acq On : 09 Oct 2022 11:48
 Operator : SY/MD
 Sample : VV1008WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.168	3143	3150	3155	rVV6	2264	3498	0.19%	0.026%
78	11.239	3160	3172	3190	rBV	705270	1095299	59.56%	8.260%
79	11.525	3258	3261	3263	rBV3	866	499	0.03%	0.004%
80	11.612	3276	3288	3313	rBV	803585	1267297	68.92%	9.558%
81	11.741	3325	3328	3334	rVB5	3995	3611	0.20%	0.027%
82	12.152	3452	3456	3459	rBV5	826	839	0.05%	0.006%
83	12.220	3474	3477	3481	rBV5	1218	1123	0.06%	0.008%
84	12.239	3481	3483	3489	rVB5	1651	1723	0.09%	0.013%
85	13.342	3824	3826	3832	rBV6	819	565	0.03%	0.004%
86	13.493	3862	3873	3890	rBV	49476	83179	4.52%	0.627%
87	13.615	3905	3911	3920	rBV5	4433	5642	0.31%	0.043%
88	13.802	3966	3969	3971	rVB4	873	489	0.03%	0.004%
89	13.821	3971	3975	3977	rBV4	1167	893	0.05%	0.007%
90	13.853	3982	3985	3989	rBV4	780	667	0.04%	0.005%
91	13.953	4014	4016	4023	rBV5	639	638	0.03%	0.005%
92	14.146	4071	4076	4078	rBV3	1299	1357	0.07%	0.010%
93	14.564	4203	4206	4214	rVB7	1079	1227	0.07%	0.009%
94	14.625	4217	4225	4237	rVB3	9603	14727	0.80%	0.111%
95	14.808	4276	4282	4294	rVB2	7032	10585	0.58%	0.080%
96	15.024	4345	4349	4351	rBV4	1139	929	0.05%	0.007%
97	15.081	4365	4367	4371	rBV4	896	588	0.03%	0.004%
98	15.162	4388	4392	4396	rBV6	1126	1215	0.07%	0.009%
99	15.361	4447	4454	4456	rBV6	1738	2035	0.11%	0.015%
100	15.493	4493	4495	4497	rBV	938	597	0.03%	0.005%




Sum of corrected areas: 13259648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028478.D
Acq On : 09 Oct 2022 11:48
Operator : SY/MD
Sample : VV1008WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

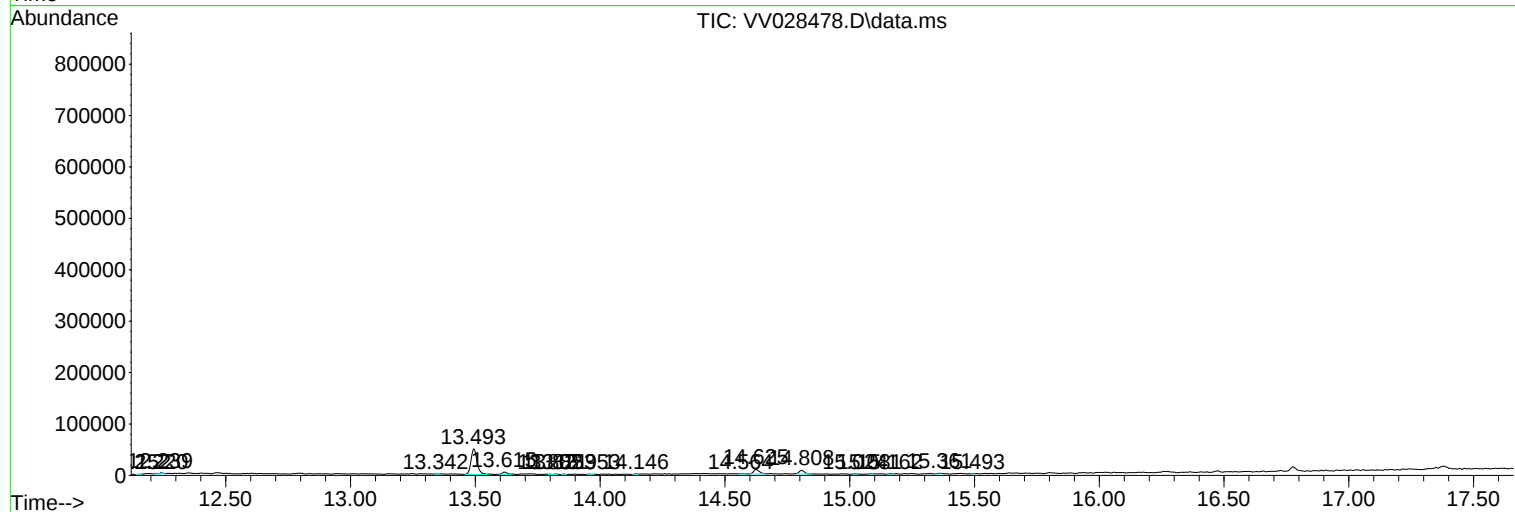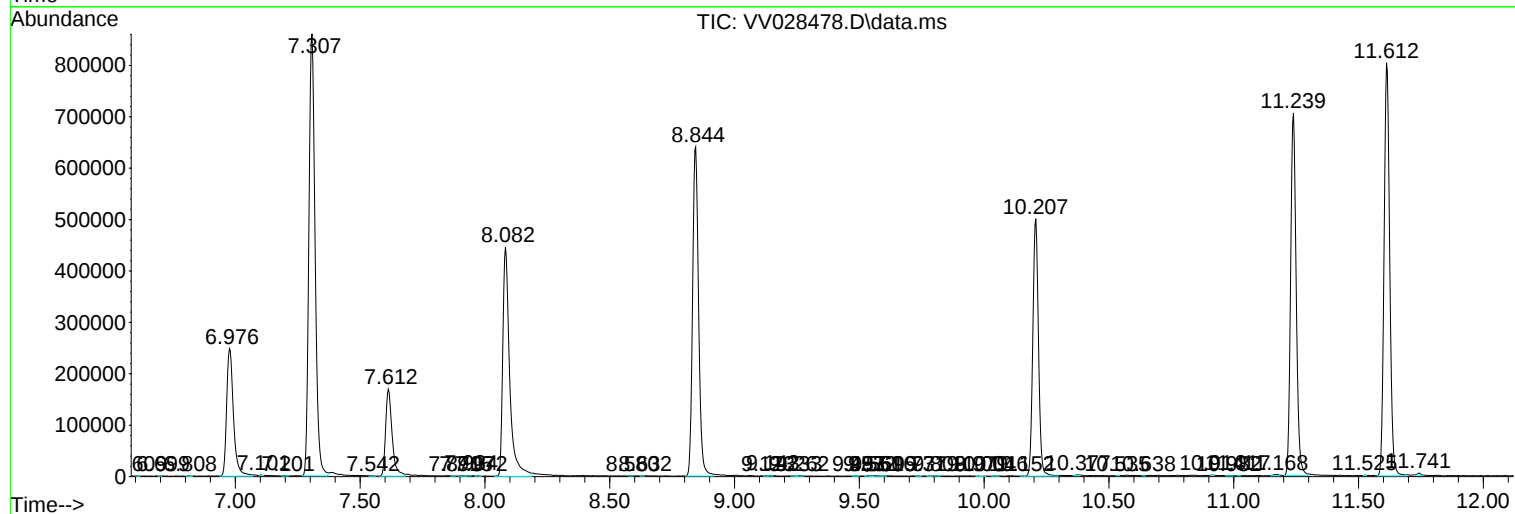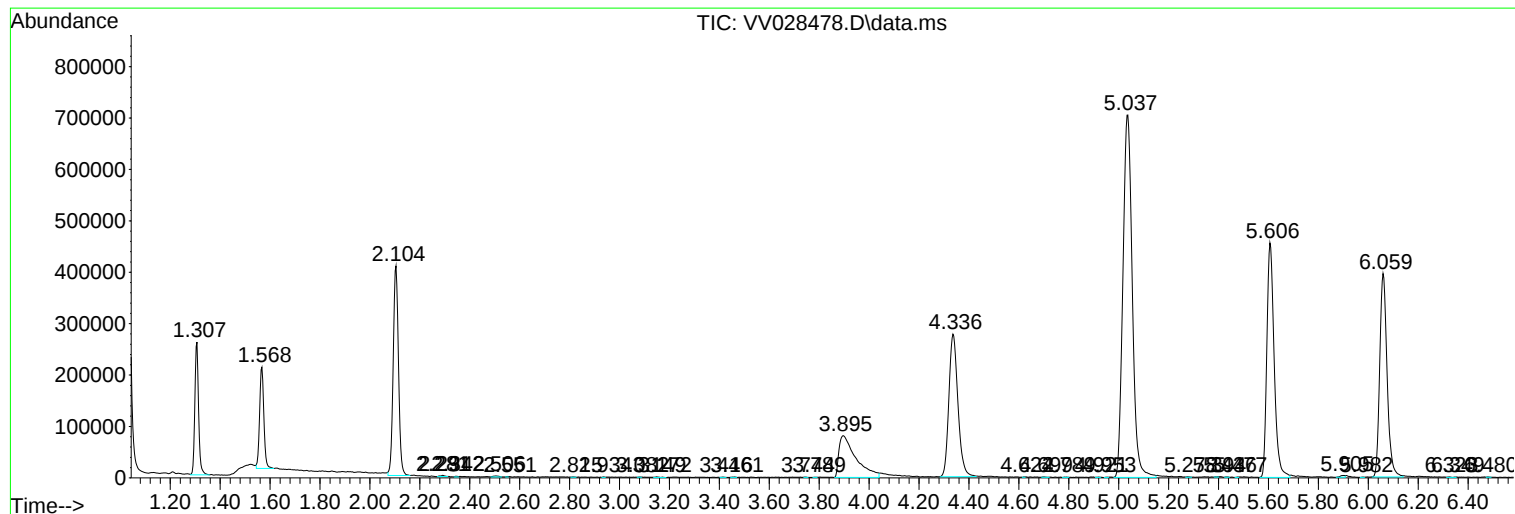

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028478.D
Acq On : 09 Oct 2022 11:48
Operator : SY/MD
Sample : VV1008WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028478.D
Acq On : 09 Oct 2022 11:48
Operator : SY/MD
Sample : VV1008WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------