

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028487.D
 Acq On : 09 Oct 2022 16:25
 Operator : SY/MD
 Sample : N4923-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rVB	213176	218565	13.56%	1.863%
2	1.565	158	163	174	rVB	169173	189595	11.76%	1.616%
3	2.101	322	330	350	rVB	349203	509583	31.61%	4.343%
4	2.854	560	564	565	rBV2	504	410	0.03%	0.003%
5	2.934	585	589	596	rBV4	1109	1301	0.08%	0.011%
6	3.085	634	636	641	rVB3	731	383	0.02%	0.003%
7	3.172	658	663	666	rBV3	715	678	0.04%	0.006%
8	3.375	724	726	729	rBV	480	309	0.02%	0.003%
9	3.468	748	755	757	rBV4	932	639	0.04%	0.005%
10	3.510	766	768	770	rBV	419	273	0.02%	0.002%
11	3.654	811	813	821	rVB4	731	604	0.04%	0.005%
12	3.780	849	852	854	rBV2	603	344	0.02%	0.003%
13	3.835	867	869	874	rVV3	374	342	0.02%	0.003%
14	3.899	879	889	943	rBV2	76853	391341	24.28%	3.335%
15	4.339	1011	1026	1052	rBV	242271	597846	37.09%	5.095%
16	4.773	1156	1161	1164	rBV4	607	632	0.04%	0.005%
17	4.799	1167	1169	1173	rVV4	681	507	0.03%	0.004%
18	4.831	1175	1179	1182	rVB3	957	659	0.04%	0.006%
19	4.863	1187	1189	1191	rBV2	647	440	0.03%	0.004%
20	5.037	1227	1243	1280	rVV2	624574	1611864	100.00%	13.737%
21	5.384	1348	1351	1353	rBV2	970	702	0.04%	0.006%
22	5.410	1357	1359	1360	rBV2	747	329	0.02%	0.003%
23	5.433	1365	1366	1370	rVB2	546	302	0.02%	0.003%
24	5.542	1396	1400	1403	rVB3	551	470	0.03%	0.004%
25	5.609	1409	1421	1459	rBV	391889	794595	49.30%	6.772%
26	5.870	1500	1502	1505	rBV3	507	304	0.02%	0.003%
27	5.905	1505	1513	1520	rBV6	2849	5172	0.32%	0.044%
28	6.063	1548	1562	1595	rBV	348460	724986	44.98%	6.179%
29	6.339	1645	1648	1651	rBV2	747	454	0.03%	0.004%
30	6.465	1685	1687	1693	rVB5	533	440	0.03%	0.004%
31	6.513	1697	1702	1704	rBV4	636	512	0.03%	0.004%
32	6.568	1717	1719	1724	rVB3	527	278	0.02%	0.002%
33	6.600	1726	1729	1732	rVB3	687	324	0.02%	0.003%
34	6.709	1760	1763	1766	rVB3	639	313	0.02%	0.003%
35	6.728	1766	1769	1772	rBV3	605	376	0.02%	0.003%
36	6.834	1798	1802	1803	rBV2	541	326	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028487.D
 Acq On : 09 Oct 2022 16:25
 Operator : SY/MD
 Sample : N4923-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.979	1836	1847	1873	rBV	208997	398119	24.70%	3.393%
38	7.307	1937	1949	1981	rBV	732822	1288758	79.95%	10.984%
39	7.616	2035	2045	2070	rBV	146201	262111	16.26%	2.234%
40	7.895	2130	2132	2137	rVB5	707	493	0.03%	0.004%
41	8.011	2166	2168	2173	rBV5	510	473	0.03%	0.004%
42	8.085	2180	2191	2227	rBV	443663	881280	54.67%	7.511%
43	8.481	2311	2314	2317	rBV3	926	679	0.04%	0.006%
44	8.519	2323	2326	2329	rVB3	568	268	0.02%	0.002%
45	8.584	2341	2346	2350	rBV4	1035	1040	0.06%	0.009%
46	8.622	2355	2358	2360	rBV2	829	423	0.03%	0.004%
47	8.635	2360	2362	2364	rVB2	716	316	0.02%	0.003%
48	8.844	2416	2427	2459	rBV	558111	922592	57.24%	7.863%
49	9.204	2536	2539	2541	rBV3	475	277	0.02%	0.002%
50	9.259	2550	2556	2559	rBV2	618	461	0.03%	0.004%
51	9.304	2566	2570	2573	rBV4	521	388	0.02%	0.003%
52	9.362	2584	2588	2592	rVB4	753	576	0.04%	0.005%
53	9.439	2609	2612	2614	rBV2	496	269	0.02%	0.002%
54	9.481	2623	2625	2630	rVB3	657	475	0.03%	0.004%
55	9.506	2630	2633	2636	rBV2	432	384	0.02%	0.003%
56	9.529	2636	2640	2642	rBV2	446	315	0.02%	0.003%
57	9.548	2642	2646	2650	rBV3	1339	1121	0.07%	0.010%
58	9.725	2698	2701	2704	rBV	447	328	0.02%	0.003%
59	9.870	2743	2746	2748	rBV2	497	305	0.02%	0.003%
60	9.934	2761	2766	2768	rVV2	843	725	0.04%	0.006%
61	10.014	2787	2791	2793	rBV4	599	409	0.03%	0.003%
62	10.088	2811	2814	2819	rVB4	500	351	0.02%	0.003%
63	10.207	2837	2851	2878	rBV	477887	751245	46.61%	6.403%
64	10.320	2884	2886	2892	rBV3	590	638	0.04%	0.005%
65	10.346	2892	2894	2898	rVB2	717	431	0.03%	0.004%
66	10.368	2898	2901	2903	rBV2	625	306	0.02%	0.003%
67	10.448	2924	2926	2931	rVV3	438	346	0.02%	0.003%
68	10.471	2931	2933	2939	rVB4	806	501	0.03%	0.004%
69	10.503	2939	2943	2947	rBV5	525	601	0.04%	0.005%
70	10.606	2972	2975	2977	rBV3	491	332	0.02%	0.003%
71	10.635	2980	2984	2986	rBV3	545	301	0.02%	0.003%
72	10.728	3010	3013	3015	rBV4	393	303	0.02%	0.003%
73	10.757	3019	3022	3026	rBV3	319	297	0.02%	0.003%
74	10.837	3044	3047	3049	rBV3	910	447	0.03%	0.004%
75	10.892	3058	3064	3066	rBV4	641	551	0.03%	0.005%
76	10.915	3066	3071	3077	rBV4	1467	1711	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
 Data File : VV028487.D
 Acq On : 09 Oct 2022 16:25
 Operator : SY/MD
 Sample : N4923-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.239	3161	3172	3198	rBV	587084	925917	57.44%	7.891%
78	11.464	3238	3242	3244	rBV3	543	289	0.02%	0.002%
79	11.616	3273	3289	3313	rBV	696339	1106526	68.65%	9.431%
80	11.886	3367	3373	3377	rVB5	594	741	0.05%	0.006%
81	12.162	3454	3459	3462	rBV4	580	460	0.03%	0.004%
82	12.310	3499	3505	3506	rBV5	358	326	0.02%	0.003%
83	12.358	3516	3520	3522	rBV3	1043	834	0.05%	0.007%
84	12.416	3534	3538	3541	rBV3	760	747	0.05%	0.006%
85	12.432	3541	3543	3547	rVB2	694	427	0.03%	0.004%
86	12.635	3599	3606	3607	rBV3	3007	2172	0.13%	0.019%
87	12.686	3618	3622	3624	rBV2	590	390	0.02%	0.003%
88	12.825	3662	3665	3669	rBV3	697	668	0.04%	0.006%
89	12.943	3698	3702	3704	rBV5	803	494	0.03%	0.004%
90	12.985	3712	3715	3718	rVB2	554	378	0.02%	0.003%
91	13.005	3718	3721	3723	rBV2	435	276	0.02%	0.002%
92	13.037	3726	3731	3732	rBV2	647	454	0.03%	0.004%
93	13.255	3793	3799	3809	rVB6	4542	6931	0.43%	0.059%
94	13.307	3814	3815	3818	rBV2	445	284	0.02%	0.002%
95	13.345	3824	3827	3831	rBV4	1006	975	0.06%	0.008%
96	13.497	3865	3874	3891	rVB	42147	71521	4.44%	0.610%
97	13.734	3940	3948	3959	rVB6	6776	10677	0.66%	0.091%
98	13.908	4000	4002	4006	rBV5	545	358	0.02%	0.003%
99	14.111	4062	4065	4068	rBV3	665	477	0.03%	0.004%
100	14.808	4275	4282	4293	rVB	15272	23918	1.48%	0.204%




Sum of corrected areas: 11733384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028487.D
Acq On : 09 Oct 2022 16:25
Operator : SY/MD
Sample : N4923-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

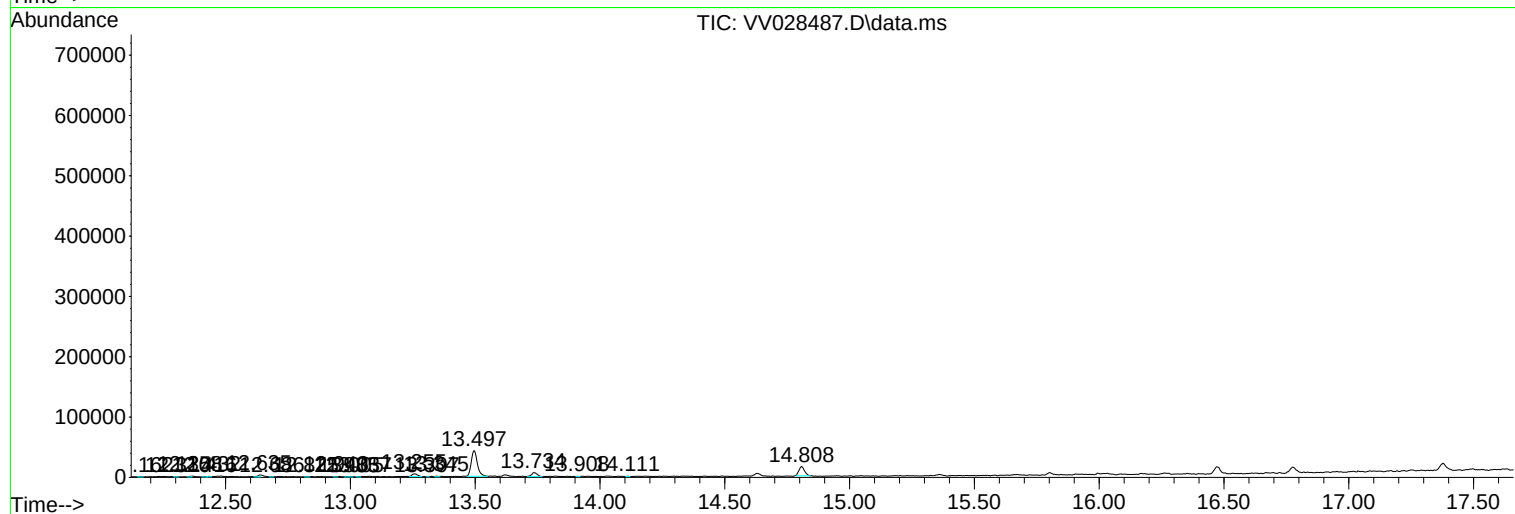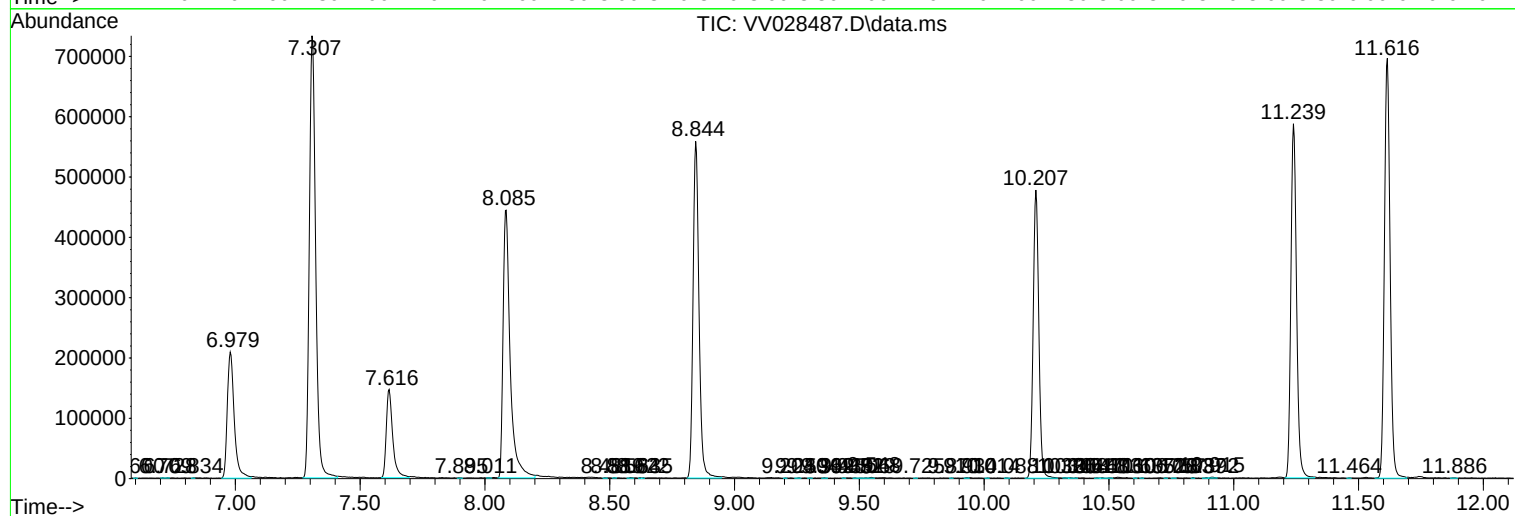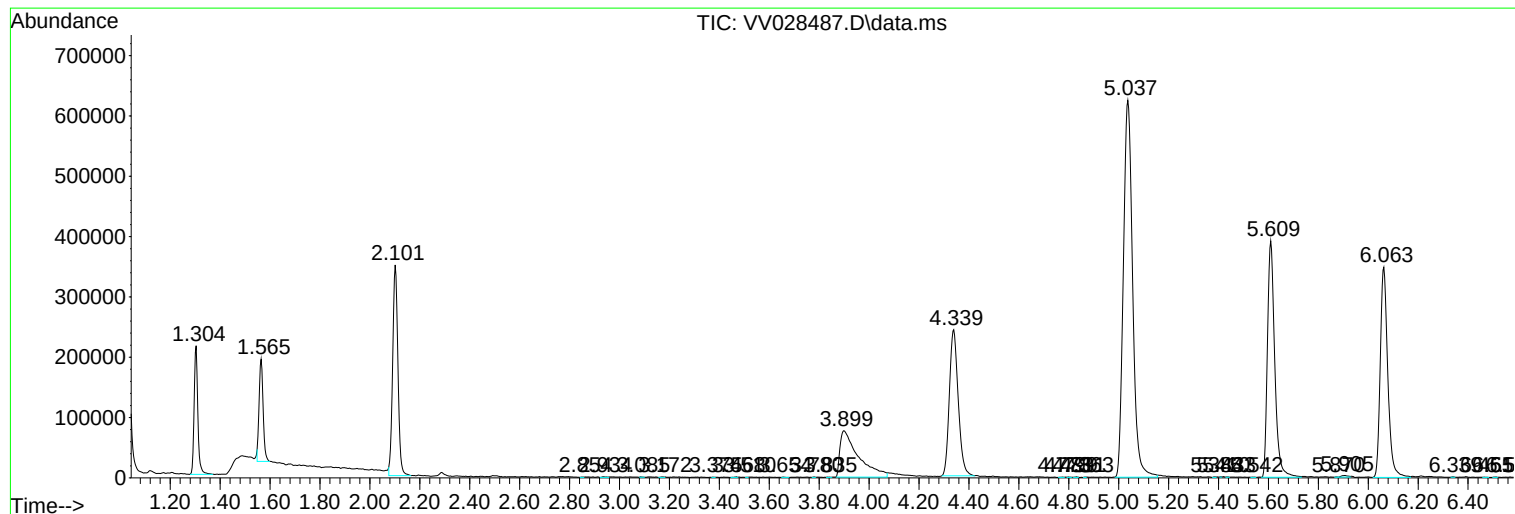

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028487.D
Acq On : 09 Oct 2022 16:25
Operator : SY/MD
Sample : N4923-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028487.D
Acq On : 09 Oct 2022 16:25
Operator : SY/MD
Sample : N4923-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------