
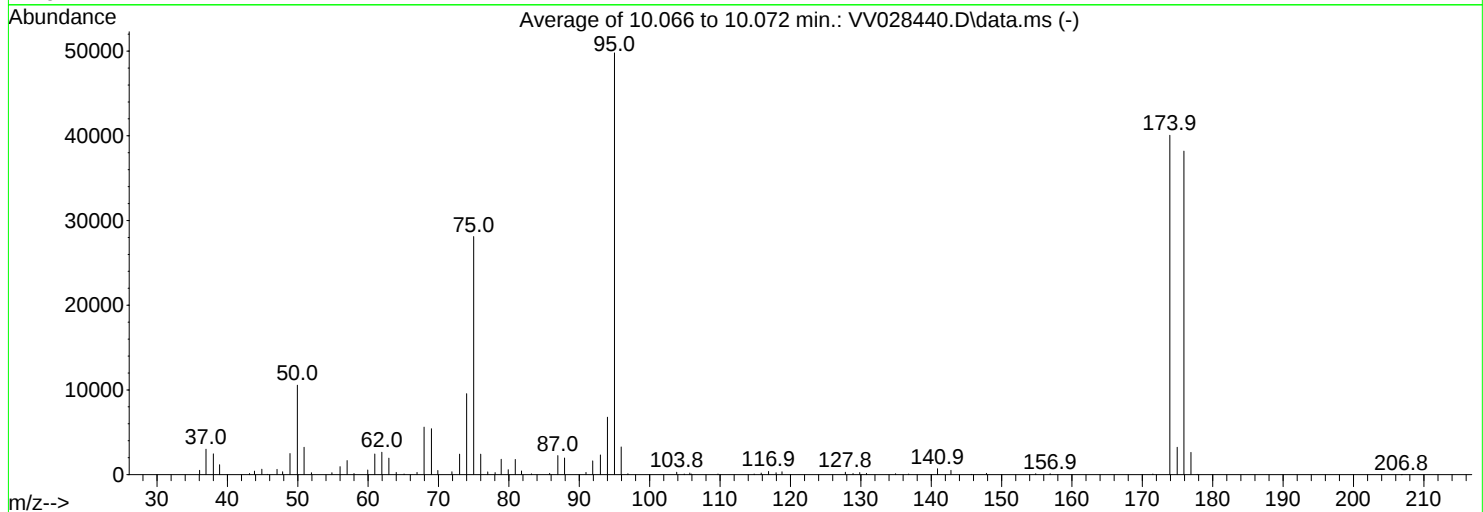


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100822\
Data File : VV028440.D
Acq On : 08 Oct 2022 16:09
Operator : SY/MD
Sample : BFB326
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB326

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Title : VOC Analysis
Last Update : Tue Oct 11 02:53:11 2022

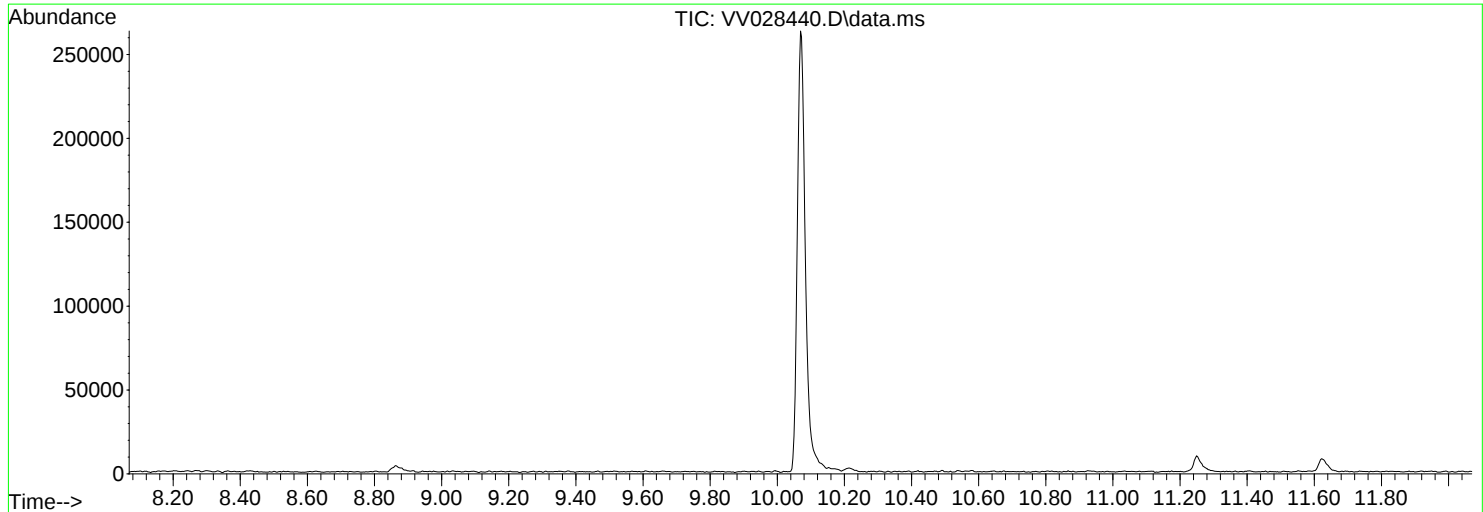

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2797

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	10558	PASS
75	95	30	80	56.4	28099	PASS
95	95	100	100	100.0	49795	PASS
96	95	5	9	6.6	3273	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.4	40059	PASS
175	174	5	9	8.1	3231	PASS
176	174	95	105	95.3	38189	PASS
177	176	5	10	6.9	2627	PASS

m/z	Abundance
38.80	103.0
39.80	362.0
40.80	103.0
42.90	116.0
43.80	526.0
206.80	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB326

m/z	Abundance
36.10	447.0
36.90	2952.0
38.00	2285.0
38.90	1187.0
39.80	298.0
43.20	121.0
43.90	858.0
44.90	547.0
45.70	102.0
47.00	658.0
47.80	367.0
48.90	2373.0
50.00	10269.0
50.90	3030.0
51.90	195.0
54.90	241.0
56.00	947.0
57.00	1543.0
58.00	128.0
59.90	619.0
61.00	2365.0
61.90	2588.0
62.90	1800.0
64.00	273.0
67.00	283.0
67.90	5665.0
69.00	5221.0
69.90	441.0
71.90	310.0
73.00	2276.0
74.00	9137.0
75.00	27064.0
76.00	2388.0
77.00	318.0
78.00	235.0
78.90	1645.0
79.90	520.0
80.90	1604.0
81.80	375.0
83.20	168.0
85.80	128.0
87.00	2280.0
87.90	1935.0
90.90	251.0
91.90	1626.0
93.00	2089.0
94.00	6557.0
95.00	47328.0
96.00	3188.0
96.90	124.0
103.80	284.0
105.70	306.0
109.70	118.0
114.80	129.0
115.90	209.0
116.90	346.0
118.00	201.0
118.80	314.0
127.80	261.0
128.90	144.0
129.90	215.0
130.80	142.0
134.90	105.0
136.80	128.0
140.90	709.0
142.80	509.0
145.70	114.0
147.80	135.0
154.80	111.0
157.00	115.0
171.50	105.0
173.90	36232.0
174.90	3103.0
175.90	34824.0
176.90	2369.0
206.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB326

m/z	Abundance
36.00	537.0
36.90	3129.0
38.00	2513.0
39.00	1320.0
39.80	304.0
43.20	146.0
44.00	1005.0
44.90	666.0
47.00	631.0
47.90	327.0
48.90	2591.0
50.00	10838.0
50.90	3355.0
51.90	229.0
54.90	236.0
56.00	983.0
57.00	1722.0
58.00	138.0
59.90	555.0
60.90	2525.0
61.90	2715.0
63.00	2006.0
64.00	267.0
65.10	117.0
67.00	281.0
67.90	5758.0
69.00	5614.0
69.90	521.0
71.90	343.0
73.00	2514.0
74.00	9960.0
75.00	29168.0
76.00	2486.0
77.00	335.0
78.10	265.0
78.90	1850.0
79.90	615.0
80.90	1815.0
81.80	439.0
83.20	106.0
85.80	160.0
86.90	2315.0
87.90	2034.0
90.90	268.0
91.90	1664.0
93.00	2408.0
94.00	7057.0
95.00	51496.0
95.90	3375.0
96.90	131.0
103.90	295.0
104.90	111.0
105.70	284.0
109.70	105.0
114.90	107.0
115.80	195.0
116.90	390.0
118.00	247.0
118.80	351.0
127.80	298.0
128.90	142.0
129.80	260.0
130.80	178.0
135.00	112.0
136.80	119.0
140.90	702.0
142.80	526.0
147.80	156.0
154.90	118.0
156.90	126.0
171.50	117.0
173.90	41576.0
174.90	3309.0
175.90	39448.0
176.90	2740.0
206.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB326

m/z	Abundance
36.00	539.0
37.00	2908.0
38.00	2557.0
38.90	1297.0
39.80	292.0
43.10	150.0
44.00	953.0
44.90	697.0
47.10	588.0
47.90	313.0
48.90	2532.0
49.90	10567.0
50.90	3296.0
52.00	265.0
54.80	198.0
56.00	914.0
57.00	1753.0
58.00	126.0
60.00	456.0
60.90	2435.0
62.00	2613.0
63.00	2007.0
64.00	245.0
65.10	139.0
66.90	226.0
68.00	5415.0
69.00	5457.0
69.90	531.0
71.90	354.0
73.00	2471.0
74.00	9574.0
75.00	28064.0
76.00	2382.0
77.00	340.0
78.00	256.0
78.90	1949.0
79.90	614.0
80.90	1966.0
81.80	474.0
85.80	148.0
86.90	2153.0
87.90	1954.0
91.00	254.0
91.90	1597.0
93.00	2502.0
94.00	6744.0
95.00	50560.0
95.90	3255.0
96.90	103.0
103.90	274.0
104.90	120.0
105.90	248.0
115.80	182.0
116.90	406.0
117.90	239.0
118.80	353.0
127.80	296.0
128.90	136.0
129.80	269.0
130.80	142.0
135.00	113.0
140.90	675.0
142.80	528.0
147.90	157.0
154.90	107.0
156.80	117.0
173.90	42368.0
175.00	3281.0
175.90	40296.0
176.90	2772.0
177.80	107.0
206.80	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB326