

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028538.D
 Acq On : 13 Oct 2022 15:41
 Operator : SY/MD
 Sample : N5070-08ME
 Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ6ME

Quant Time: Oct 14 04:50:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 14 04:49:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	356774	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	347198	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	186930	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	47060	17.095	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	34.180%#
7) Chloroethane-d5	1.565	69	42669	19.548	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	39.100%#
11) 1,1-Dichloroethene-d2	2.089	63	89795	19.166	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	38.340%#
21) 2-Butanone-d5	3.915	46	161459	66.999	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	67.000%
24) Chloroform-d	4.336	84	182956	36.237	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.480%
26) 1,2-Dichloroethane-d4	5.024	65	132439	40.673	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.340%
32) Benzene-d6	5.037	84	288949	25.972	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	51.940%#
36) 1,2-Dichloropropane-d6	6.063	67	105231	29.011	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	58.020%#
41) Toluene-d8	7.310	98	262835	26.387	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	52.780%#
43) trans-1,3-Dichloroprop...	7.619	79	63349	34.264	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.520%
47) 2-Hexanone-d5	8.108	63	149181	75.603	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.600%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	192913	38.865	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	77.720%
66) 1,2-Dichlorobenzene-d4	11.619	152	151416	39.092	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.180%#
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.979	75	4300	0.883	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028538.D
Acq On : 13 Oct 2022 15:41
Operator : SY/MD
Sample : N5070-08ME
Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ6ME

Quant Time: Oct 14 04:50:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 14 04:49:18 2022
Response via : Initial Calibration

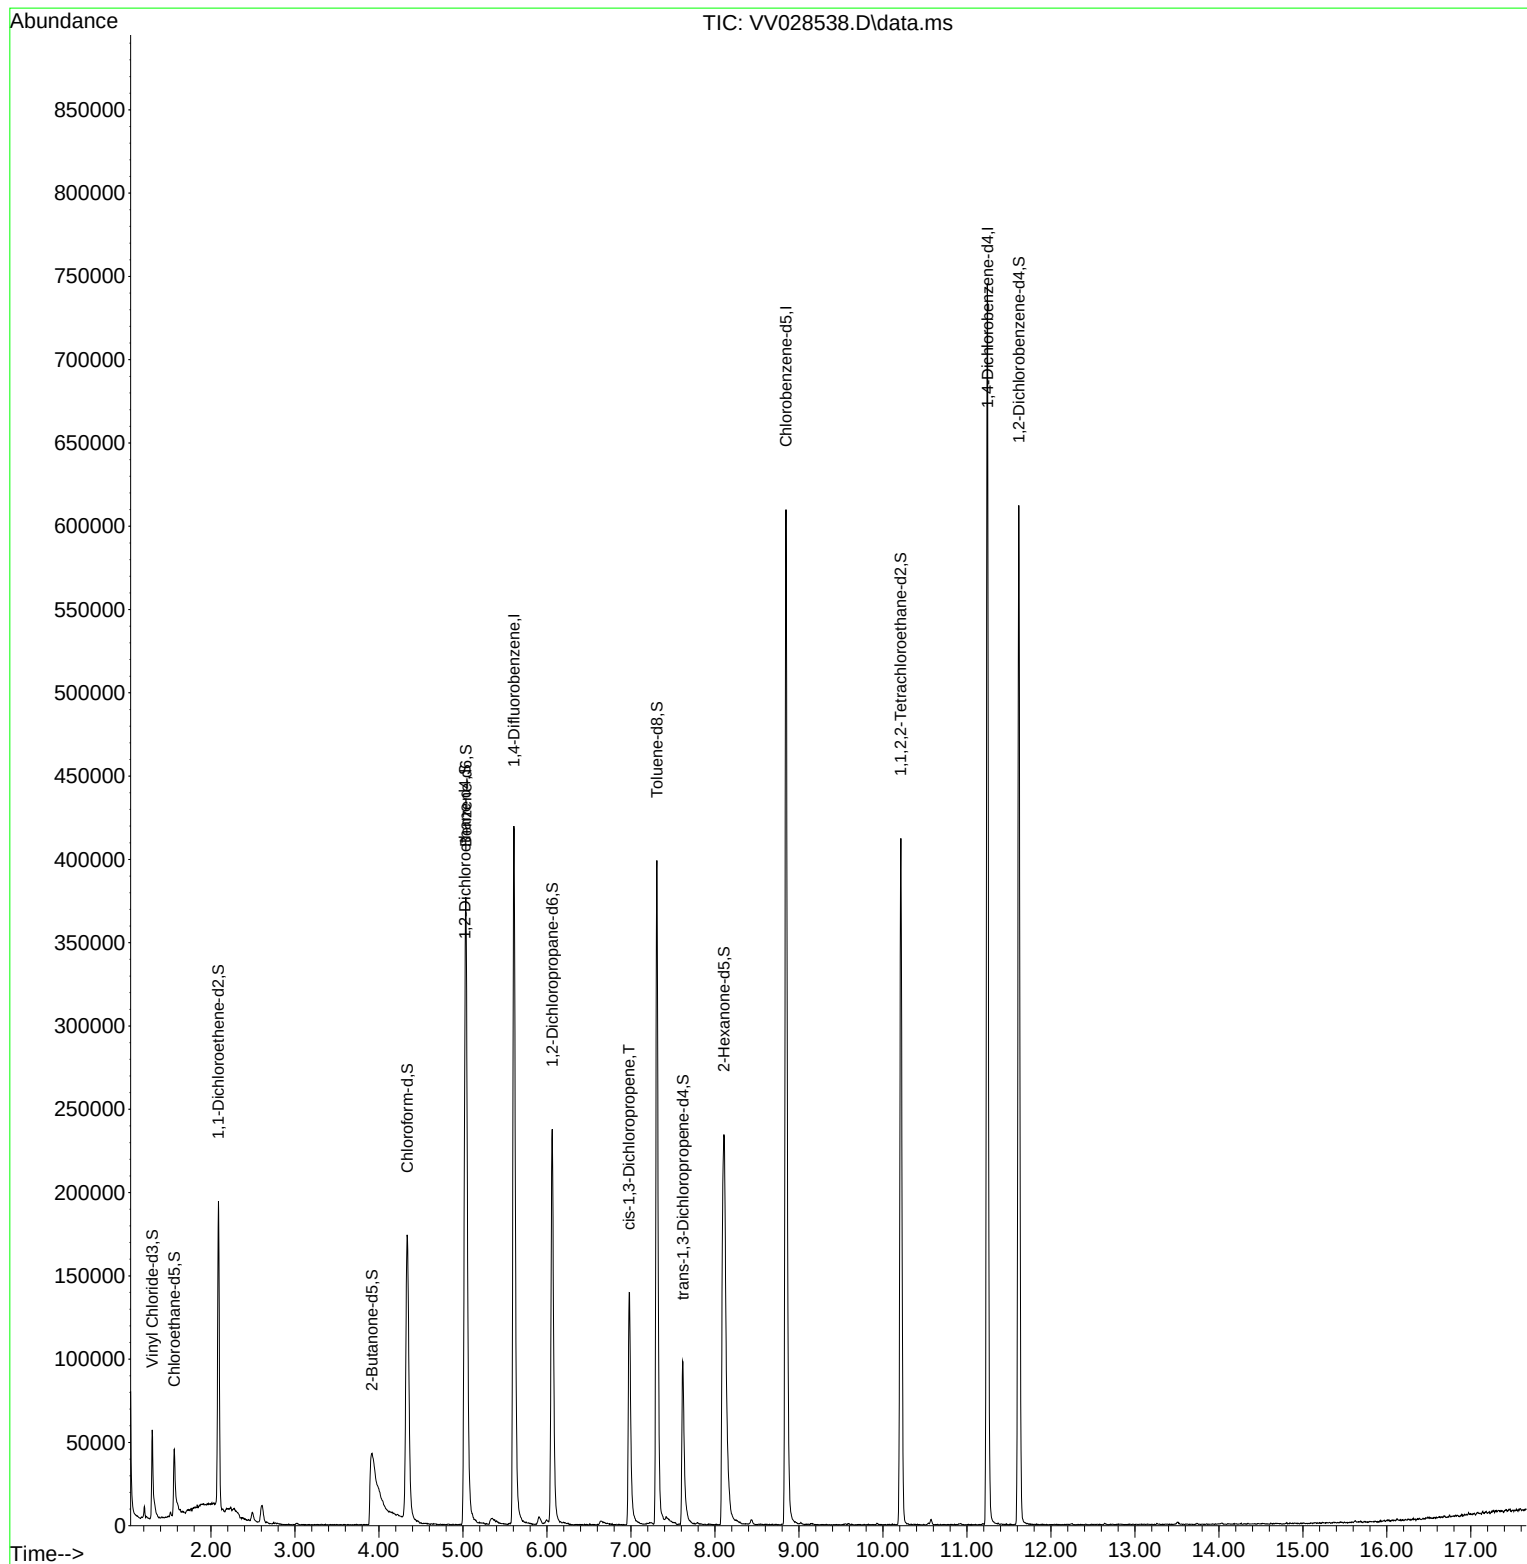

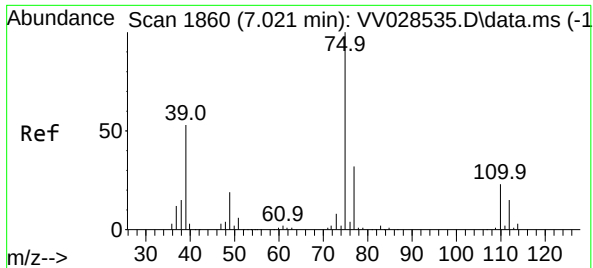

#39
 cis-1,3-Dichloropropene
 Concen: 0.883 ug/L
 RT: 6.979 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV028538.D
 Acq: 13 Oct 2022 15:41

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ6ME

Tgt Ion: 75 Resp: 4300
 Ion Ratio Lower Upper
 75 100
 77 49.3 23.2 43.0#

