

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101322\
 Data File : VW028539.D
 Acq On : 13 Oct 2022 16:05
 Operator : SY/MD
 Sample : N5070-13ME
 Misc : 4.56g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BR9ME

Quant Time: Oct 14 04:50:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 14 04:49:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	251306	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	245215	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	138225	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	37964	19.578	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	39.160%#
7) Chloroethane-d5	1.564	69	32388	21.065	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	42.120%#
11) 1,1-Dichloroethene-d2	2.088	63	75715	22.943	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	45.880%#
21) 2-Butanone-d5	3.921	46	80586	47.474	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	47.470%
24) Chloroform-d	4.339	84	149964	42.168	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.340%
26) 1,2-Dichloroethane-d4	5.024	65	112033	48.846	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.700%
32) Benzene-d6	5.040	84	236802	30.137	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	60.280%#
36) 1,2-Dichloropropane-d6	6.066	67	86331	33.698	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	67.400%#
41) Toluene-d8	7.310	98	217747	30.952	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	61.900%#
43) trans-1,3-Dichloroprop...	7.619	79	53876	41.259	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.520%
47) 2-Hexanone-d5	8.111	63	120594	86.533	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.530%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	156955	44.771	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.540%
66) 1,2-Dichlorobenzene-d4	11.619	152	131391	45.875	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.740%
Target Compounds						
					Qvalue	
6) Bromomethane	1.519	94	1038	1.065	ug/L	88
29) Cyclohexane	4.667	56	3455	0.980	ug/L	# 71
35) Methylcyclohexane	6.120	83	13856	3.984	ug/L	99
39) cis-1,3-Dichloropropene	6.982	75	3775	1.097	ug/L	85
53) m,p-Xylene	9.140	106	4301	1.252	ug/L	94
54) o-Xylene	9.541	106	4161	1.210	ug/L	94
63) 1,2,4-Trimethylbenzene	10.914	105	6933	0.810	ug/L	97
71) Naphthalene	13.500	128	13804	1.522	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028539.D
Acq On : 13 Oct 2022 16:05
Operator : SY/MD
Sample : N5070-13ME
Misc : 4.56g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR9ME

Quant Time: Oct 14 04:50:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 14 04:49:18 2022
Response via : Initial Calibration




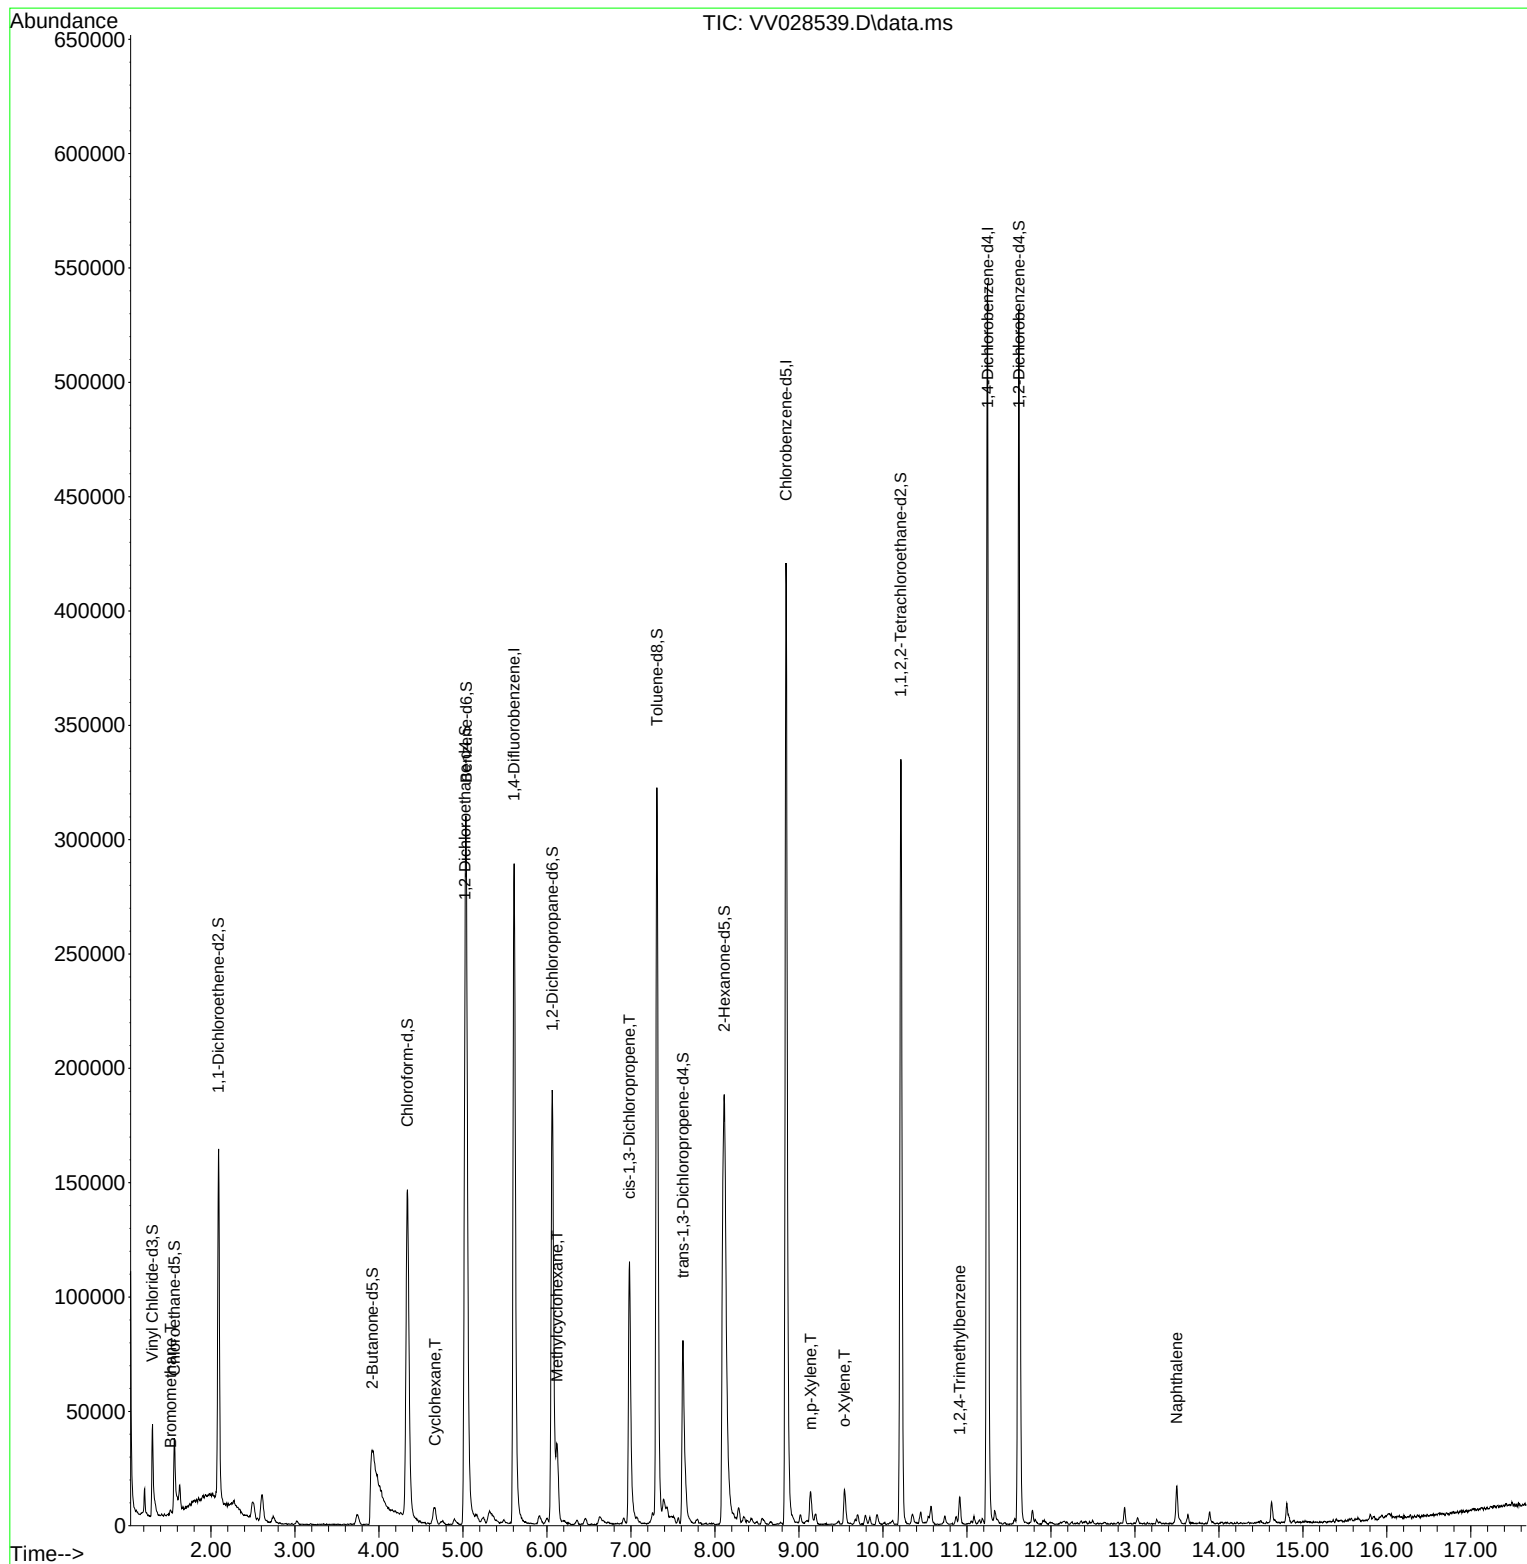


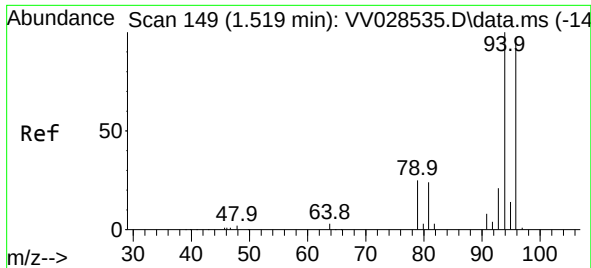

#6
Bromomethane
Concen: 1.065 ug/L
RT: 1.519 min Scan# 149
Delta R.T. -0.000 min
Lab File: VV028539.D
Acq: 13 Oct 2022 16:05




Instrument :
MSVOA_V
ClientSampleId :
C0BR9ME


Tgt Ion: 94 Resp: 1038
Ion Ratio Lower Upper
94 100
96 104.6 65.5 121.6

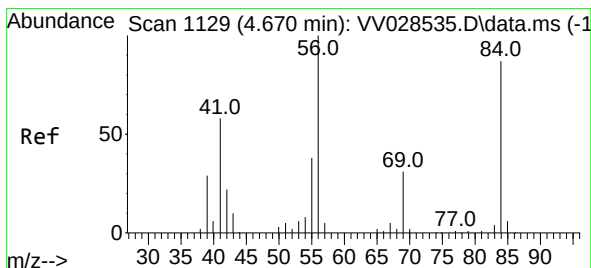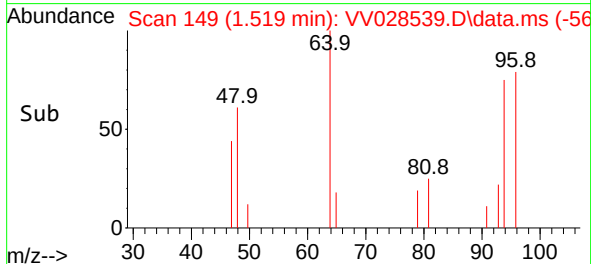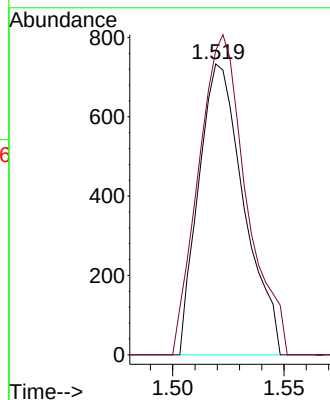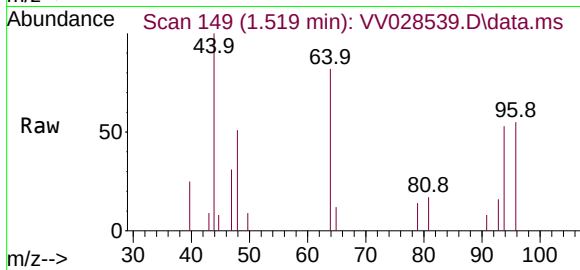

#29
Cyclohexane
Concen: 0.980 ug/L
RT: 4.667 min Scan# 1128
Delta R.T. -0.003 min
Lab File: VV028539.D
Acq: 13 Oct 2022 16:05

Tgt Ion: 56 Resp: 3455
Ion Ratio Lower Upper
56 100
69 32.0 23.0 34.6
84 49.4 65.8 98.8#


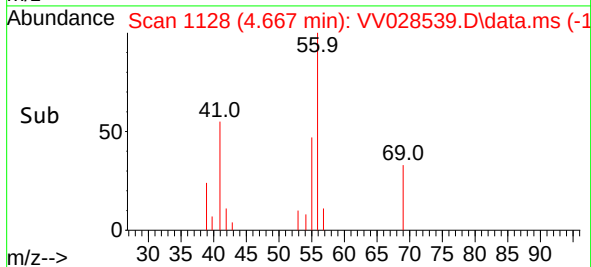
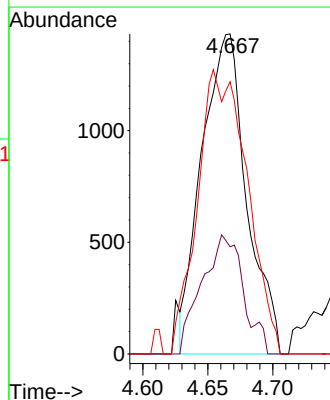
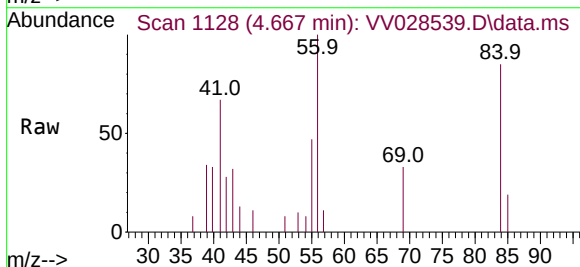


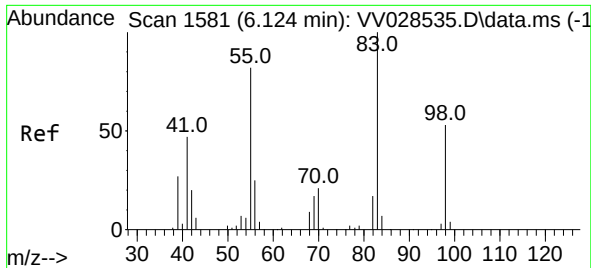

#35
Methylcyclohexane
Concen: 3.984 ug/L
RT: 6.120 min Scan# 11
Delta R.T. -0.003 min
Lab File: VV028539.D
Acq: 13 Oct 2022 16:05




Instrument :
MSVOA_V
ClientSampleId :
C0BR9ME


Tgt Ion: 83 Resp: 13856
Ion Ratio Lower Upper
83 100
55 78.3 63.7 95.5
98 47.8 38.2 57.2

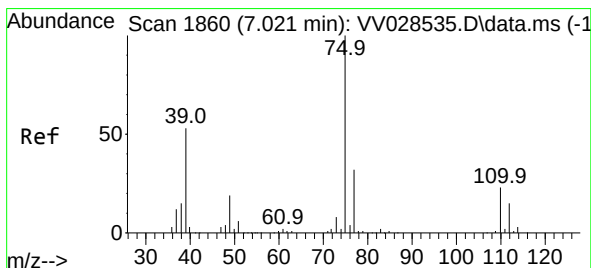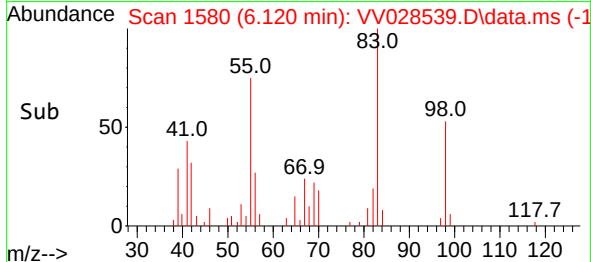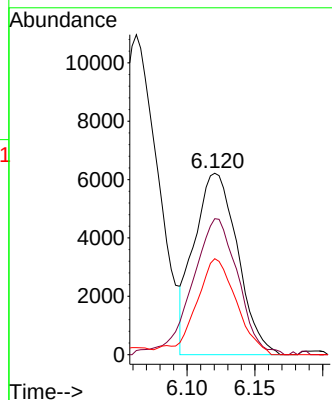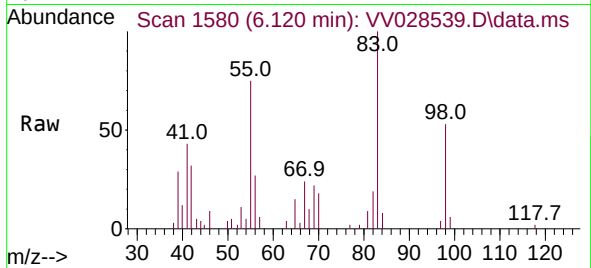

#39
cis-1,3-Dichloropropene
Concen: 1.097 ug/L
RT: 6.982 min Scan# 1848
Delta R.T. -0.039 min
Lab File: VV028539.D
Acq: 13 Oct 2022 16:05

Tgt Ion: 75 Resp: 3775
Ion Ratio Lower Upper
75 100
77 41.7 23.2 43.0


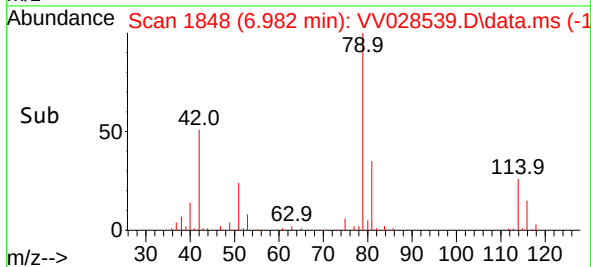
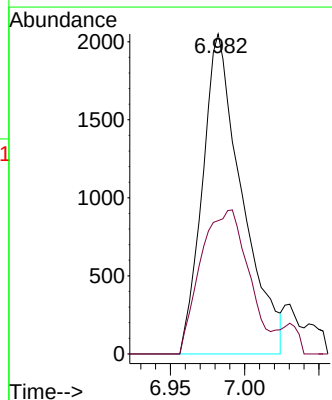
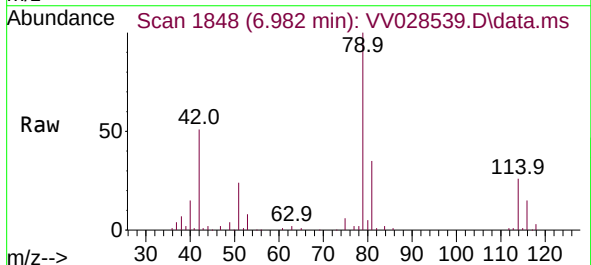


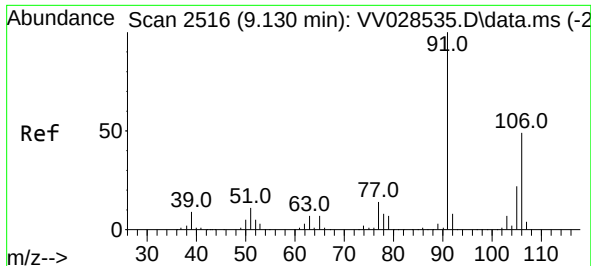

#53
m,p-Xylene
Concen: 1.252 ug/L
RT: 9.140 min Scan# 2516
Delta R.T. 0.010 min
Lab File: VV028539.D
Acq: 13 Oct 2022 16:05




Instrument :
MSVOA_V
ClientSampleId :
C0BR9ME


Tgt Ion:106 Resp: 4301
Ion Ratio Lower Upper
106 100
91 198.0 145.2 269.6

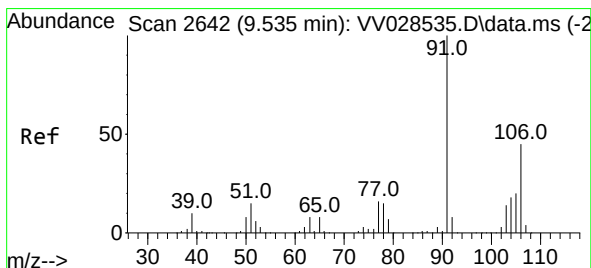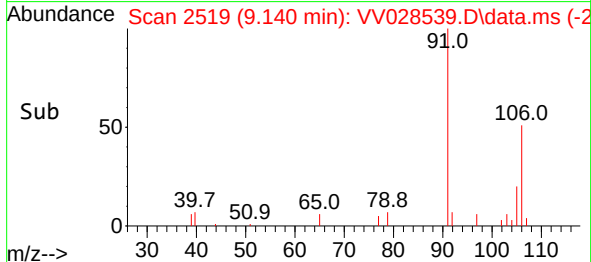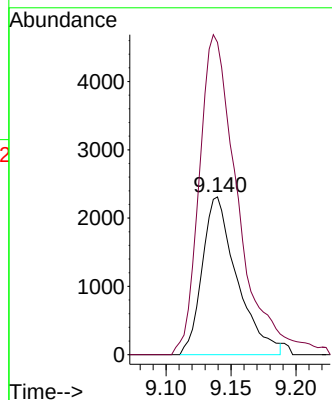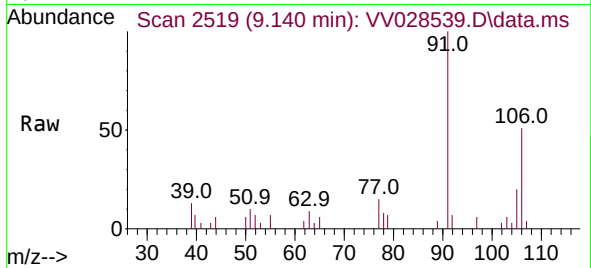

#54
o-Xylene
Concen: 1.210 ug/L
RT: 9.541 min Scan# 2644
Delta R.T. 0.006 min
Lab File: VV028539.D
Acq: 13 Oct 2022 16:05

Tgt Ion:106 Resp: 4161
Ion Ratio Lower Upper
106 100
91 227.9 152.5 283.3

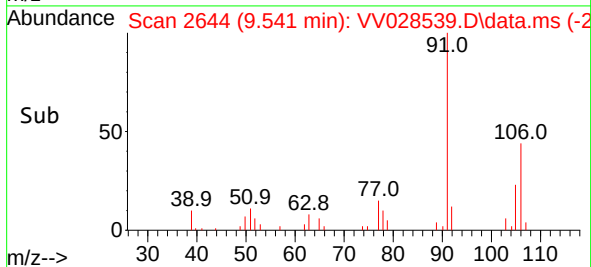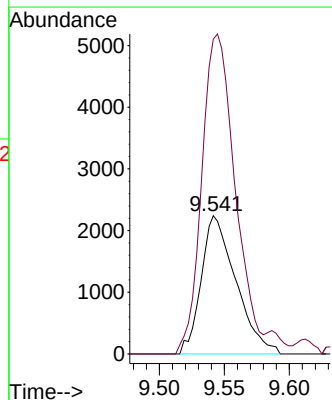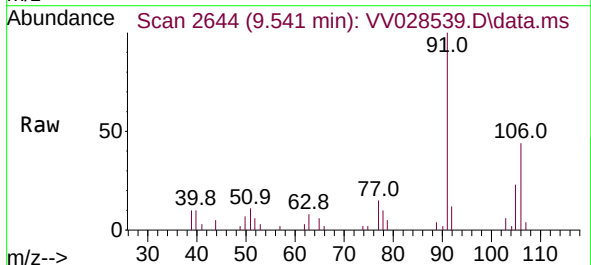

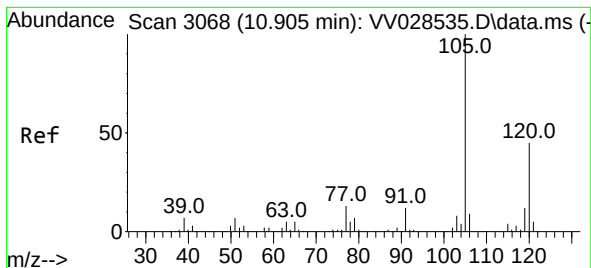

#63

1,2,4-Trimethylbenzene

Concen: 0.810 ug/L

RT: 10.914 min Scan# 3068

Delta R.T. 0.010 min

Lab File: VV028539.D

Acq: 13 Oct 2022 16:05

Instrument :

MSVOA_V

ClientSampleId :





C0BR9ME

Tgt Ion:105 Resp: 6933

Ion Ratio Lower Upper

105 100

120 42.9 35.9 53.9

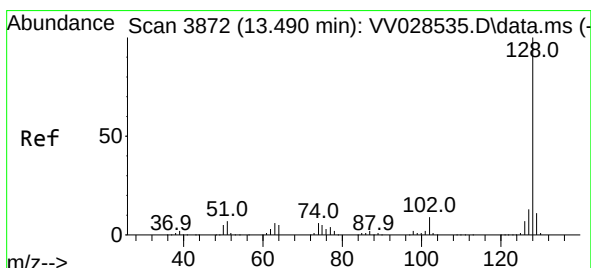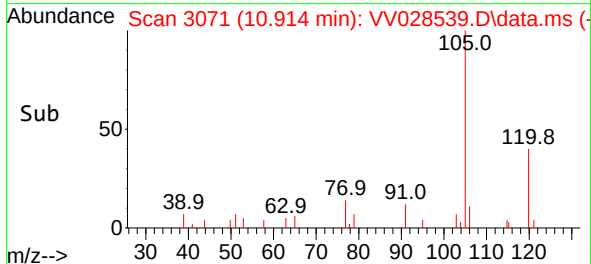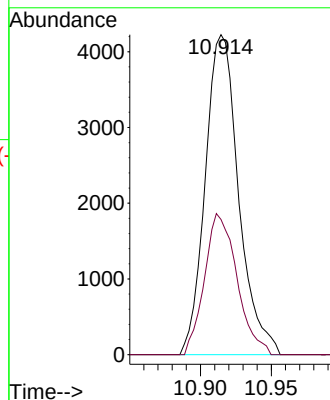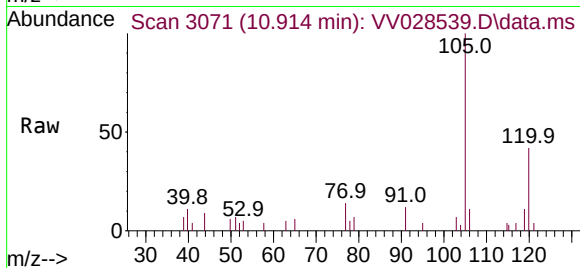

#71

Naphthalene

Concen: 1.522 ug/L

RT: 13.500 min Scan# 3875

Delta R.T. 0.010 min

Lab File: VV028539.D

Acq: 13 Oct 2022 16:05

Tgt Ion:128 Resp: 13804

Ion Ratio Lower Upper

128 100

127 14.2 10.6 15.8

129 11.2 8.9 13.3

