




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028543.D
 Acq On : 13 Oct 2022 17:39
 Operator : SY/MD
 Sample : N5070-09ME
 Misc : 6.73g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ7MERE

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:51:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 14 04:49:18 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

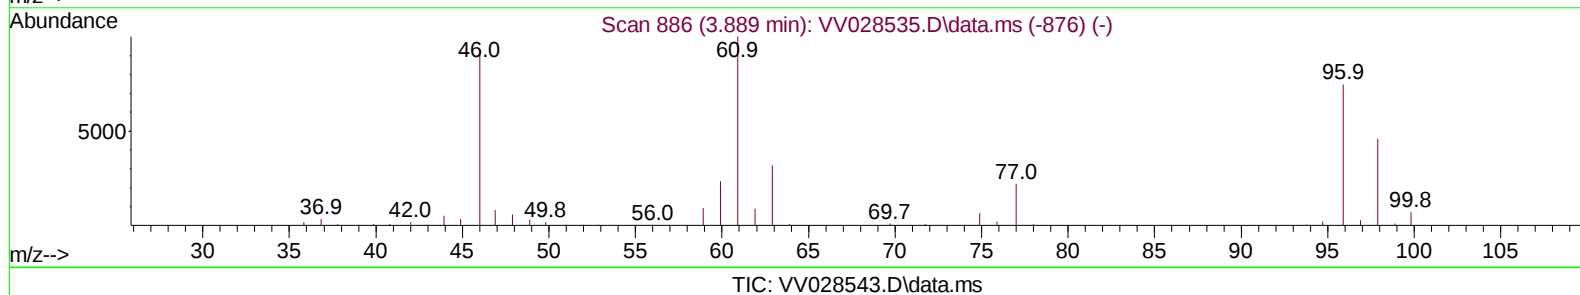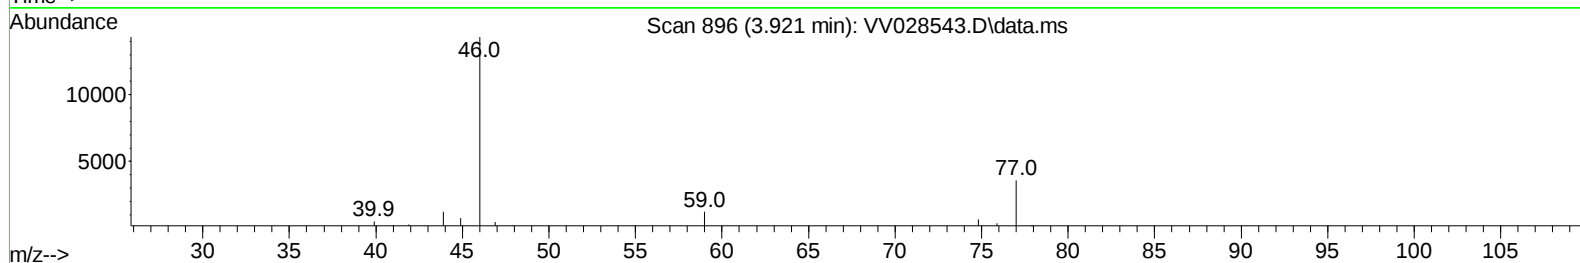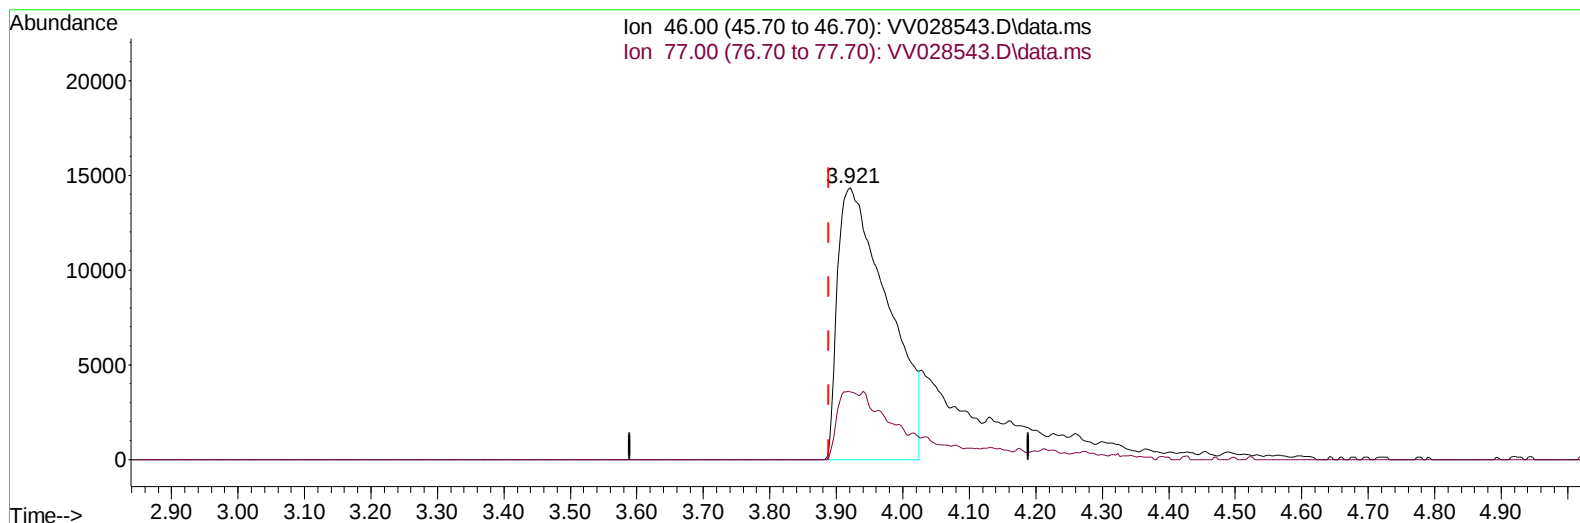

(21) 2-Butanone-d5 (S)

3.921min (+ 0.032) 46.33 ug/L

response 75135

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.10	10.57#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028543.D
 Acq On : 13 Oct 2022 17:39
 Operator : SY/MD
 Sample : N5070-09ME
 Misc : 6.73g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ7MERE

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:51:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 14 04:49:18 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

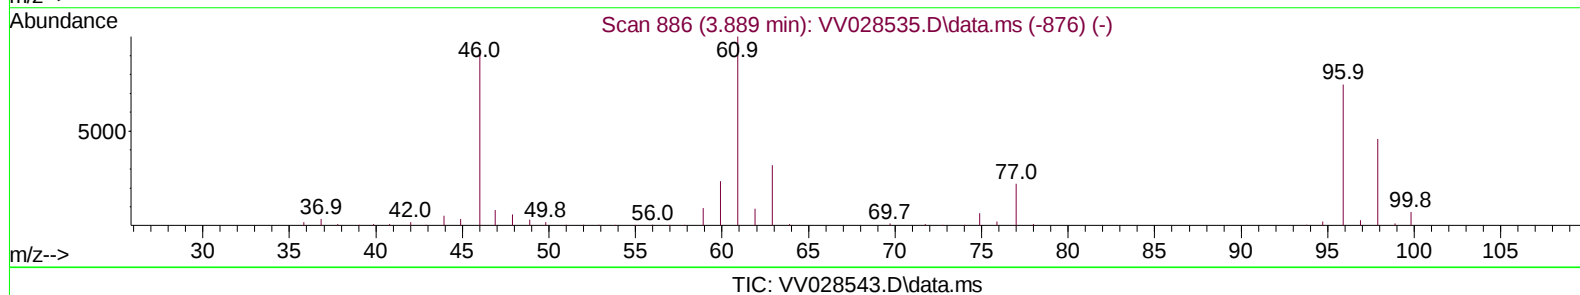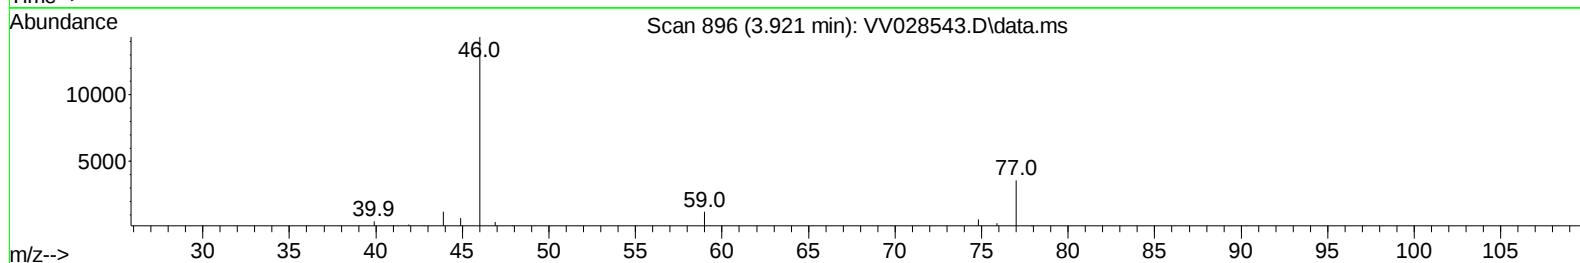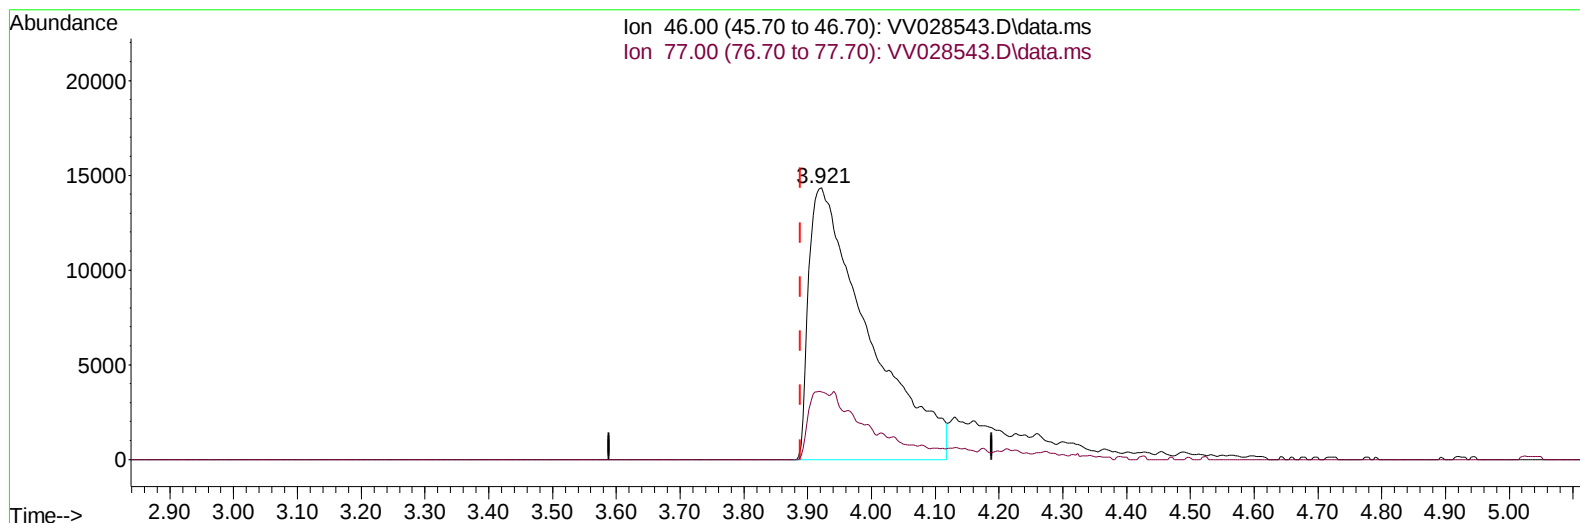

(21) 2-Butanone-d5 (S)

3.921min (+ 0.032) 57.03 ug/L m

response 92480

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.10	8.59#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028543.D
 Acq On : 13 Oct 2022 17:39
 Operator : SY/MD
 Sample : N5070-09ME
 Misc : 6.73g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ7MERE

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:51:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 14 04:49:18 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
 Supervised By :Mahesh Dadoda 10/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	240079	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	226358	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	126321	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	25540	13.787	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery =	27.580%#		
7) Chloroethane-d5	1.561	69	24352	16.579	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery =	33.160%#		
11) 1,1-Dichloroethene-d2	2.085	63	53763	17.053	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery =	34.100%#		
21) 2-Butanone-d5	3.921	46	92480m	57.028	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery =	57.030%		
24) Chloroform-d	4.336	84	104862	30.865	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	61.720%#		
26) 1,2-Dichloroethane-d4	5.024	65	76837	35.068	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	70.140%		
32) Benzene-d6	5.040	84	164286	22.650	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	45.300%#		
36) 1,2-Dichloropropane-d6	6.063	67	58861	24.890	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery =	49.780%#		
41) Toluene-d8	7.310	98	146370	22.539	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	45.080%#		
43) trans-1,3-Dichloroprop...	7.622	79	35544	29.488	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	58.980%#		
47) 2-Hexanone-d5	8.108	63	78815	61.266	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery =	61.270%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	107419	33.194	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery =	66.380%		
66) 1,2-Dichlorobenzene-d4	11.619	152	91498	34.957	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	69.920%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028543.D
Acq On : 13 Oct 2022 17:39
Operator : SY/MD
Sample : N5070-09ME
Misc : 6.73g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ7MERE

Manual IntegrationsAPPROVED

Quant Time: Oct 14 04:51:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 14 04:49:18 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/17/2022
Supervised By :Mahesh Dadoda 10/18/2022

