

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028538.D
 Acq On : 13 Oct 2022 15:41
 Operator : SY/MD
 Sample : N5070-08ME
 Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	104	rVB	52793	73275	6.36%	0.823%
2	1.565	157	163	181	rBV	37942	60511	5.25%	0.680%
3	2.089	319	326	339	rVB	185255	258450	22.42%	2.905%
4	2.844	559	561	566	rVB	322	245	0.02%	0.003%
5	2.921	583	585	586	rBV	291	131	0.01%	0.001%
6	3.018	611	615	617	rBV4	612	488	0.04%	0.005%
7	3.169	659	662	663	rBV	187	97	0.01%	0.001%
8	3.317	704	708	710	rBV	279	200	0.02%	0.002%
9	3.362	721	722	727	rBV2	320	164	0.01%	0.002%
10	3.452	748	750	753	rBV	209	96	0.01%	0.001%
11	3.468	753	755	758	rBV2	209	113	0.01%	0.001%
12	3.581	787	790	793	rBV2	245	215	0.02%	0.002%
13	3.632	803	806	811	rVB2	243	175	0.02%	0.002%
14	3.658	811	814	821	rVB	155	172	0.01%	0.002%
15	3.712	829	831	836	rBV	277	285	0.02%	0.003%
16	3.815	859	863	865	rBV2	323	183	0.02%	0.002%
17	3.831	865	868	871	rVV	158	130	0.01%	0.001%
18	3.918	882	895	952	rBV2	42847	298464	25.89%	3.354%
19	4.619	1110	1113	1119	rBV2	573	536	0.05%	0.006%
20	4.699	1134	1138	1142	rBV2	260	253	0.02%	0.003%
21	4.825	1172	1177	1183	rVB3	537	818	0.07%	0.009%
22	4.860	1183	1188	1191	rBV2	317	292	0.03%	0.003%
23	4.880	1191	1194	1199	rBV2	468	398	0.03%	0.004%
24	4.912	1201	1204	1206	rBV2	303	203	0.02%	0.002%
25	5.034	1226	1242	1273	rBV2	376636	959979	83.28%	10.789%
26	5.339	1328	1337	1338	rBV4	3488	4601	0.40%	0.052%
27	5.539	1395	1399	1400	rBV	579	346	0.03%	0.004%
28	5.606	1409	1420	1454	rBV	418558	853361	74.03%	9.590%
29	5.863	1498	1500	1502	rBV3	282	121	0.01%	0.001%
30	5.905	1504	1513	1528	rVV10	4498	10351	0.90%	0.116%
31	6.063	1550	1562	1590	rVB	235909	491577	42.64%	5.524%
32	6.342	1645	1649	1650	rBV	211	154	0.01%	0.002%
33	6.378	1657	1660	1663	rBV2	234	194	0.02%	0.002%
34	6.449	1679	1682	1684	rBV2	398	185	0.02%	0.002%
35	6.474	1686	1690	1692	rVV2	290	186	0.02%	0.002%
36	6.510	1698	1701	1706	rBV4	582	408	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101322\
 Data File : VW028538.D
 Acq On : 13 Oct 2022 15:41
 Operator : SY/MD
 Sample : N5070-08ME
 Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.564	1715	1718	1720	rVB2	211	103	0.01%	0.001%
38	6.606	1728	1731	1733	rVB2	281	145	0.01%	0.002%
39	6.642	1733	1742	1750	rBV7	2234	5113	0.44%	0.057%
40	6.812	1793	1795	1797	rVB2	244	102	0.01%	0.001%
41	6.857	1807	1809	1812	rBV	345	142	0.01%	0.002%
42	6.915	1823	1827	1830	rBV	326	241	0.02%	0.003%
43	6.979	1836	1847	1872	rBV	139414	275389	23.89%	3.095%
44	7.191	1911	1913	1916	rBV2	538	367	0.03%	0.004%
45	7.310	1938	1950	1977	rBV	398292	706724	61.31%	7.942%
46	7.568	2028	2030	2033	rBV	345	249	0.02%	0.003%
47	7.616	2036	2045	2075	rBV	98210	200165	17.36%	2.250%
48	7.915	2136	2138	2140	rBV	257	141	0.01%	0.002%
49	7.928	2140	2142	2145	rVB2	448	252	0.02%	0.003%
50	7.986	2158	2160	2162	rBV2	214	109	0.01%	0.001%
51	8.018	2168	2170	2172	rBV2	342	175	0.02%	0.002%
52	8.108	2184	2198	2239	rVV2	234073	760970	66.01%	8.552%
53	8.596	2346	2350	2354	rBV3	389	295	0.03%	0.003%
54	8.651	2366	2367	2369	rBV	332	125	0.01%	0.001%
55	8.680	2373	2376	2378	rVV	427	247	0.02%	0.003%
56	8.715	2382	2387	2390	rBV2	404	338	0.03%	0.004%
57	8.728	2390	2391	2397	rVB2	367	264	0.02%	0.003%
58	8.754	2397	2399	2400	rBV	220	104	0.01%	0.001%
59	8.796	2409	2412	2416	rBV2	445	435	0.04%	0.005%
60	8.847	2416	2428	2460	rVV	609191	1090304	94.58%	12.253%
61	9.069	2496	2497	2500	rBV2	293	163	0.01%	0.002%
62	9.088	2500	2503	2506	rVB2	331	202	0.02%	0.002%
63	9.146	2515	2521	2525	rBV2	703	897	0.08%	0.010%
64	9.201	2535	2538	2539	rBV2	268	144	0.01%	0.002%
65	9.223	2543	2545	2549	rVB2	295	161	0.01%	0.002%
66	9.532	2640	2641	2644	rBV	254	121	0.01%	0.001%
67	9.551	2644	2647	2649	rBV	368	301	0.03%	0.003%
68	9.587	2654	2658	2661	rBV3	657	523	0.05%	0.006%
69	9.931	2759	2765	2770	rBV4	832	984	0.09%	0.011%
70	9.985	2779	2782	2786	rBV	208	129	0.01%	0.001%
71	10.111	2819	2821	2823	rBV	557	274	0.02%	0.003%
72	10.214	2841	2853	2875	rBV	411824	698912	60.63%	7.855%
73	10.413	2913	2915	2917	rVB	384	139	0.01%	0.002%
74	10.439	2920	2923	2926	rBV	207	118	0.01%	0.001%
75	10.487	2933	2938	2944	rVB2	450	385	0.03%	0.004%
76	10.545	2944	2956	2958	rBV3	1185	1595	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028538.D
 Acq On : 13 Oct 2022 15:41
 Operator : SY/MD
 Sample : N5070-08ME
 Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.686	2998	3000	3004	rVB2	264	97	0.01%	0.001%
78	10.854	3049	3052	3054	rBV2	371	137	0.01%	0.002%
79	10.902	3065	3067	3070	rBV2	367	236	0.02%	0.003%
80	11.011	3098	3101	3102	rBV	198	97	0.01%	0.001%
81	11.185	3152	3155	3156	rBV2	573	297	0.03%	0.003%
82	11.243	3162	3173	3201	rBV	744966	1152749	100.00%	12.955%
83	11.471	3240	3244	3251	rVB	548	445	0.04%	0.005%
84	11.619	3277	3290	3314	rBV	611722	974636	84.55%	10.953%
85	11.831	3352	3356	3359	rBV3	443	317	0.03%	0.004%
86	11.915	3380	3382	3386	rVB2	256	131	0.01%	0.001%
87	12.133	3446	3450	3456	rBV2	235	295	0.03%	0.003%
88	12.252	3477	3487	3492	rBV2	609	906	0.08%	0.010%
89	12.304	3499	3503	3506	rBV2	187	140	0.01%	0.002%
90	12.323	3506	3509	3511	rBV	245	153	0.01%	0.002%
91	12.413	3534	3537	3539	rBV2	342	197	0.02%	0.002%
92	12.481	3555	3558	3561	rBV	297	194	0.02%	0.002%
93	12.638	3605	3607	3610	rBV2	507	295	0.03%	0.003%
94	12.886	3682	3684	3688	rBV2	202	156	0.01%	0.002%
95	12.918	3692	3694	3696	rBV	215	113	0.01%	0.001%
96	13.201	3780	3782	3787	rVB	321	195	0.02%	0.002%
97	13.262	3797	3801	3805	rBV3	831	741	0.06%	0.008%
98	13.333	3820	3823	3826	rBV2	296	190	0.02%	0.002%
99	13.442	3855	3857	3860	rVB	330	121	0.01%	0.001%
100	14.619	4220	4223	4226	rBV2	637	400	0.03%	0.004%




Sum of corrected areas: 8898142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028538.D
Acq On : 13 Oct 2022 15:41
Operator : SY/MD
Sample : N5070-08ME
Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

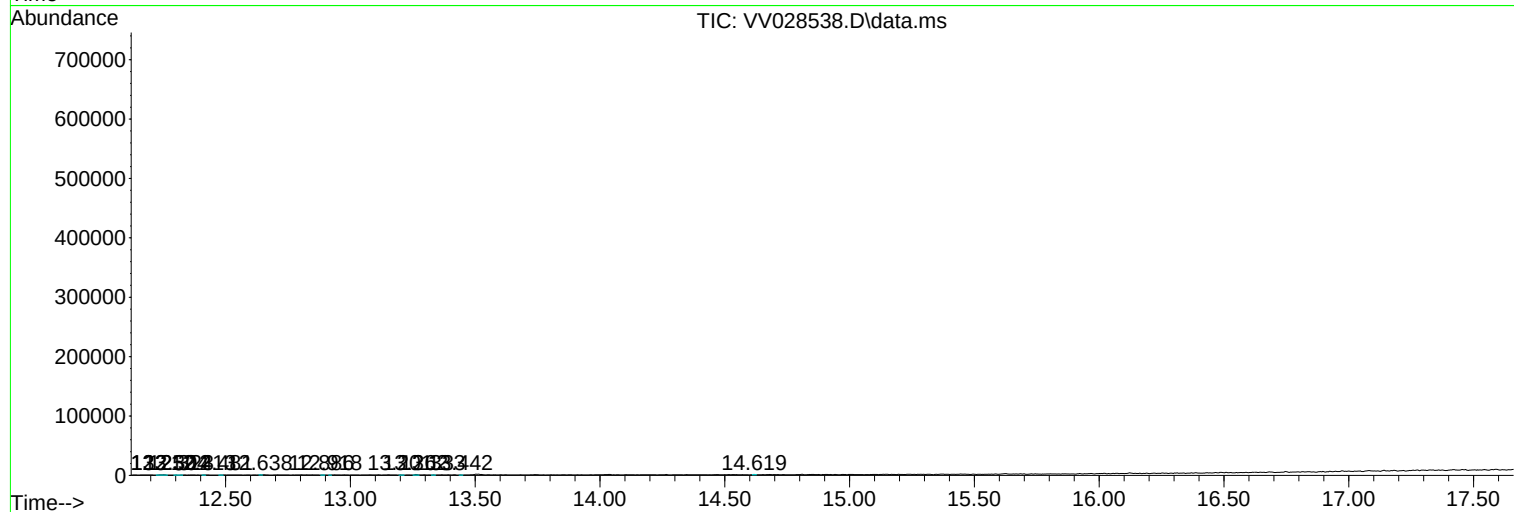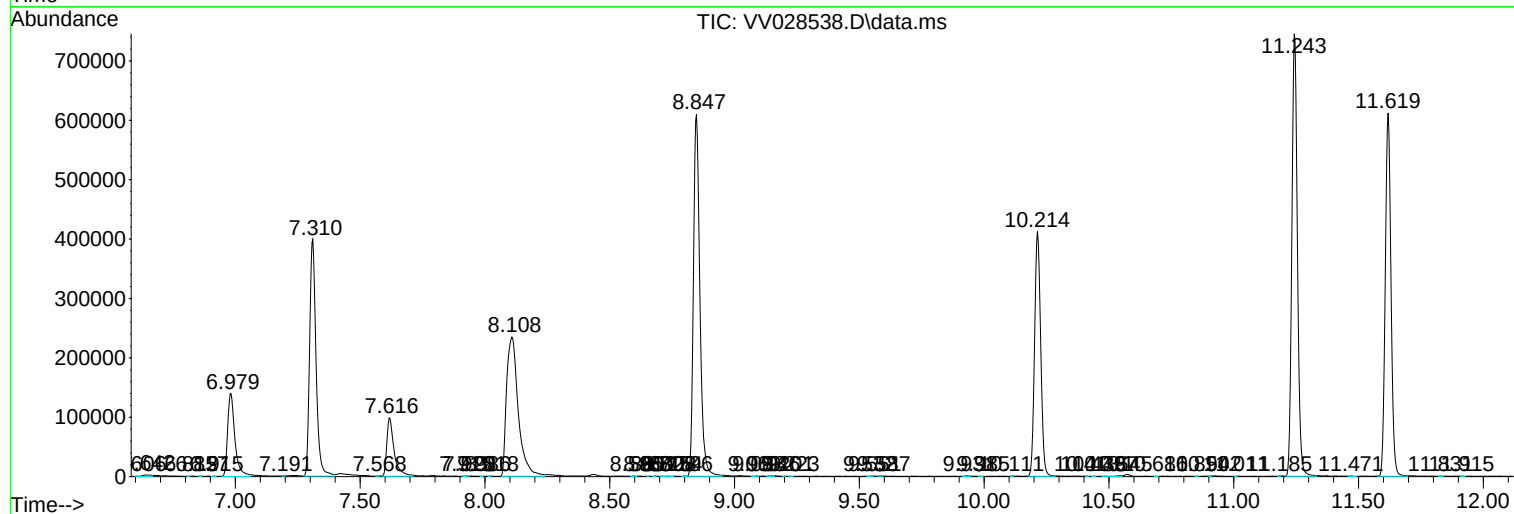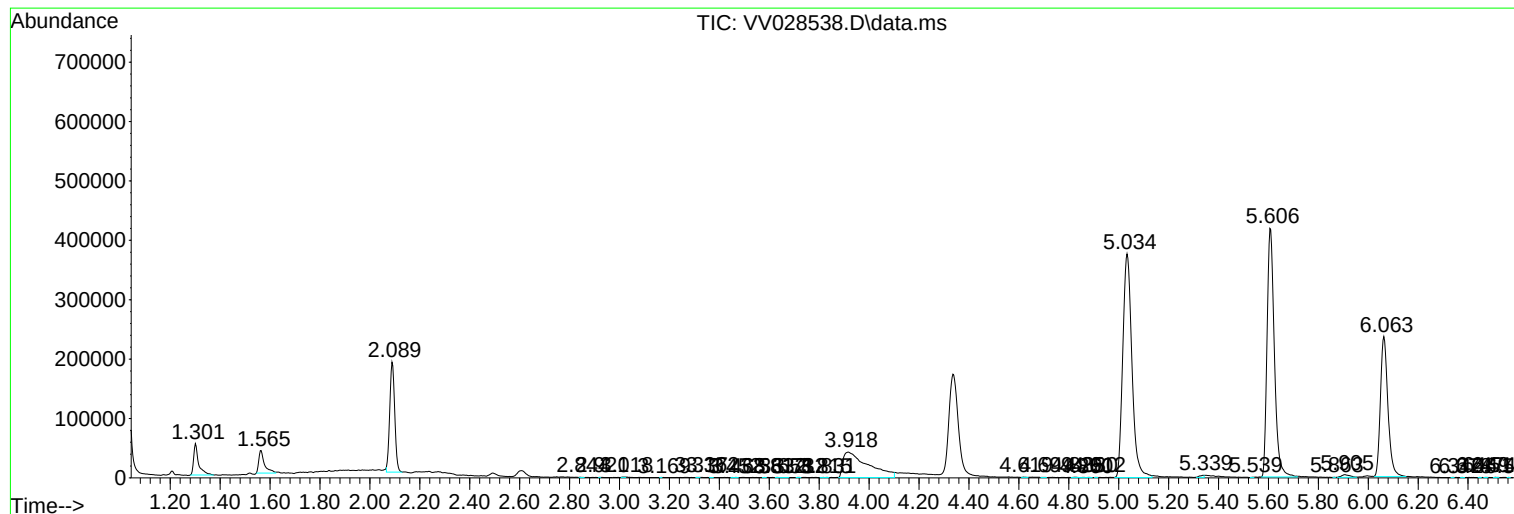

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028538.D
Acq On : 13 Oct 2022 15:41
Operator : SY/MD
Sample : N5070-08ME
Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028538.D
Acq On : 13 Oct 2022 15:41
Operator : SY/MD
Sample : N5070-08ME
Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc