

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028542.D
 Acq On : 13 Oct 2022 17:15
 Operator : SY/MD
 Sample : N5023-07ME
 Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBE0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	28900	37841	4.58%	0.689%
2	1.564	158	163	173	rBV	24112	28474	3.45%	0.519%
3	2.908	578	581	582	rBV	266	119	0.01%	0.002%
4	3.021	613	616	620	rBV4	480	431	0.05%	0.008%
5	3.063	625	629	634	rBV	220	221	0.03%	0.004%
6	3.162	655	660	661	rBV	203	142	0.02%	0.003%
7	3.175	661	664	668	rVV2	249	194	0.02%	0.004%
8	3.211	671	675	677	rBV2	193	131	0.02%	0.002%
9	3.259	687	690	693	rVB	282	174	0.02%	0.003%
10	3.362	719	722	725	rBV	220	164	0.02%	0.003%
11	3.420	737	740	743	rBV2	173	158	0.02%	0.003%
12	3.455	747	751	756	rVB2	296	258	0.03%	0.005%
13	3.686	819	823	829	rVB2	237	271	0.03%	0.005%
14	3.719	829	833	834	rBV	302	220	0.03%	0.004%
15	3.776	843	851	855	rBV	307	300	0.04%	0.005%
16	3.799	855	858	861	rVB	245	153	0.02%	0.003%
17	3.828	861	867	869	rBV2	178	156	0.02%	0.003%
18	3.844	869	872	878	rVB2	265	253	0.03%	0.005%
19	3.918	882	895	896	rBV	29107	42827	5.19%	0.780%
20	4.667	1123	1128	1133	rBV4	379	508	0.06%	0.009%
21	4.905	1197	1202	1204	rBV3	389	254	0.03%	0.005%
22	4.940	1210	1213	1215	rBV	204	135	0.02%	0.002%
23	5.037	1228	1243	1281	rBV2	230599	587366	71.12%	10.699%
24	5.272	1313	1316	1319	rBV3	501	457	0.06%	0.008%
25	5.339	1329	1337	1339	rBV6	3255	4253	0.51%	0.077%
26	5.506	1386	1389	1390	rBV2	201	104	0.01%	0.002%
27	5.542	1397	1400	1403	rBV2	423	347	0.04%	0.006%
28	5.609	1410	1421	1450	rBV	295384	603694	73.10%	10.996%
29	5.812	1482	1484	1489	rVB3	748	464	0.06%	0.008%
30	5.911	1506	1515	1530	rBV9	3286	7591	0.92%	0.138%
31	6.001	1535	1543	1549	rVV5	1959	3582	0.43%	0.065%
32	6.066	1551	1563	1592	rVB	142111	300802	36.42%	5.479%
33	6.288	1626	1632	1634	rBV2	273	261	0.03%	0.005%
34	6.407	1666	1669	1673	rVV2	181	109	0.01%	0.002%
35	6.432	1673	1677	1680	rVV2	334	169	0.02%	0.003%
36	6.448	1680	1682	1687	rVV	338	197	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101322\
 Data File : VW028542.D
 Acq On : 13 Oct 2022 17:15
 Operator : SY/MD
 Sample : N5023-07ME
 Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBE0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.506	1697	1700	1703	rBV	141	116	0.01%	0.002%
38	6.580	1722	1723	1727	rBV2	184	139	0.02%	0.003%
39	6.645	1736	1743	1747	rBV6	1783	2721	0.33%	0.050%
40	6.747	1772	1775	1778	rBV3	601	388	0.05%	0.007%
41	6.792	1785	1789	1790	rBV	253	186	0.02%	0.003%
42	6.924	1828	1830	1835	rVB3	396	291	0.04%	0.005%
43	6.985	1837	1849	1876	rBV	84167	166679	20.18%	3.036%
44	7.230	1913	1925	1926	rBV3	1346	1615	0.20%	0.029%
45	7.310	1940	1950	1971	rBV	228772	414412	50.18%	7.549%
46	7.622	2037	2047	2077	rBV	59687	120296	14.57%	2.191%
47	7.857	2117	2120	2122	rVB3	366	206	0.02%	0.004%
48	7.879	2124	2127	2133	rBV	312	257	0.03%	0.005%
49	7.927	2139	2142	2145	rBV2	321	315	0.04%	0.006%
50	7.953	2148	2150	2153	rBV2	338	166	0.02%	0.003%
51	8.008	2159	2167	2171	rBV2	358	552	0.07%	0.010%
52	8.111	2182	2199	2235	rBV	154075	485273	58.76%	8.839%
53	8.435	2291	2300	2309	rBV4	3192	5906	0.72%	0.108%
54	8.606	2351	2353	2355	rBV2	257	117	0.01%	0.002%
55	8.657	2365	2369	2373	rBV3	299	279	0.03%	0.005%
56	8.693	2376	2380	2383	rBV	237	192	0.02%	0.003%
57	8.718	2386	2388	2393	rVB2	490	374	0.05%	0.007%
58	8.760	2395	2401	2402	rBV	368	222	0.03%	0.004%
59	8.847	2417	2428	2455	rVV	422104	755915	91.53%	13.769%
60	9.021	2481	2482	2484	rBV2	528	150	0.02%	0.003%
61	9.095	2503	2505	2510	rVV2	272	219	0.03%	0.004%
62	9.178	2527	2531	2535	rBV2	306	248	0.03%	0.005%
63	9.201	2536	2538	2541	rVB	251	103	0.01%	0.002%
64	9.416	2601	2605	2612	rBV2	370	462	0.06%	0.008%
65	9.474	2620	2623	2628	rVB2	195	134	0.02%	0.002%
66	9.500	2628	2631	2634	rBV2	199	137	0.02%	0.002%
67	9.525	2636	2639	2643	rVB2	281	192	0.02%	0.003%
68	9.548	2644	2646	2647	rBV2	406	133	0.02%	0.002%
69	9.593	2656	2660	2662	rBV2	232	131	0.02%	0.002%
70	9.628	2668	2671	2672	rBV	175	107	0.01%	0.002%
71	9.808	2724	2727	2728	rBV	208	124	0.02%	0.002%
72	10.021	2791	2793	2797	rVB	279	147	0.02%	0.003%
73	10.053	2797	2803	2804	rBV2	188	164	0.02%	0.003%
74	10.123	2820	2825	2831	rBV2	336	324	0.04%	0.006%
75	10.213	2841	2853	2871	rBV	258968	442730	53.61%	8.064%
76	10.442	2921	2924	2926	rBV	248	141	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028542.D
 Acq On : 13 Oct 2022 17:15
 Operator : SY/MD
 Sample : N5023-07ME
 Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBE0ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.574	2959	2965	2974	rVB5	2801	3676	0.45%	0.067%
78	10.738	3010	3016	3017	rBV	328	255	0.03%	0.005%
79	10.767	3020	3025	3028	rBV2	265	262	0.03%	0.005%
80	10.921	3065	3073	3079	rBV4	496	841	0.10%	0.015%
81	10.950	3079	3082	3085	rBV	265	151	0.02%	0.003%
82	11.078	3117	3122	3126	rBV2	370	338	0.04%	0.006%
83	11.185	3151	3155	3158	rBV3	308	234	0.03%	0.004%
84	11.246	3162	3174	3196	rBV	516178	825836	100.00%	15.043%
85	11.422	3228	3229	3231	rBV	233	120	0.01%	0.002%
86	11.619	3279	3290	3313	rBV	390055	629759	76.26%	11.471%
87	12.030	3414	3418	3420	rBV2	290	229	0.03%	0.004%
88	12.085	3433	3435	3436	rBV2	359	121	0.01%	0.002%
89	12.098	3436	3439	3442	rBV2	208	119	0.01%	0.002%
90	12.191	3466	3468	3471	rVB2	382	172	0.02%	0.003%
91	12.422	3537	3540	3545	rVB	367	289	0.03%	0.005%
92	12.448	3545	3548	3552	rBV2	273	313	0.04%	0.006%
93	12.950	3701	3704	3708	rBV	383	261	0.03%	0.005%
94	13.120	3754	3757	3760	rBV	422	314	0.04%	0.006%
95	13.255	3796	3799	3800	rBV	261	141	0.02%	0.003%
96	13.381	3834	3838	3840	rBV	382	278	0.03%	0.005%
97	13.503	3874	3876	3877	rBV	599	229	0.03%	0.004%
98	13.602	3905	3907	3910	rBV	218	131	0.02%	0.002%
99	13.847	3981	3983	3990	rBV2	477	588	0.07%	0.011%
100	13.995	4027	4029	4031	rBV2	366	191	0.02%	0.003%




Sum of corrected areas: 5489891

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028542.D
Acq On : 13 Oct 2022 17:15
Operator : SY/MD
Sample : N5023-07ME
Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBE0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

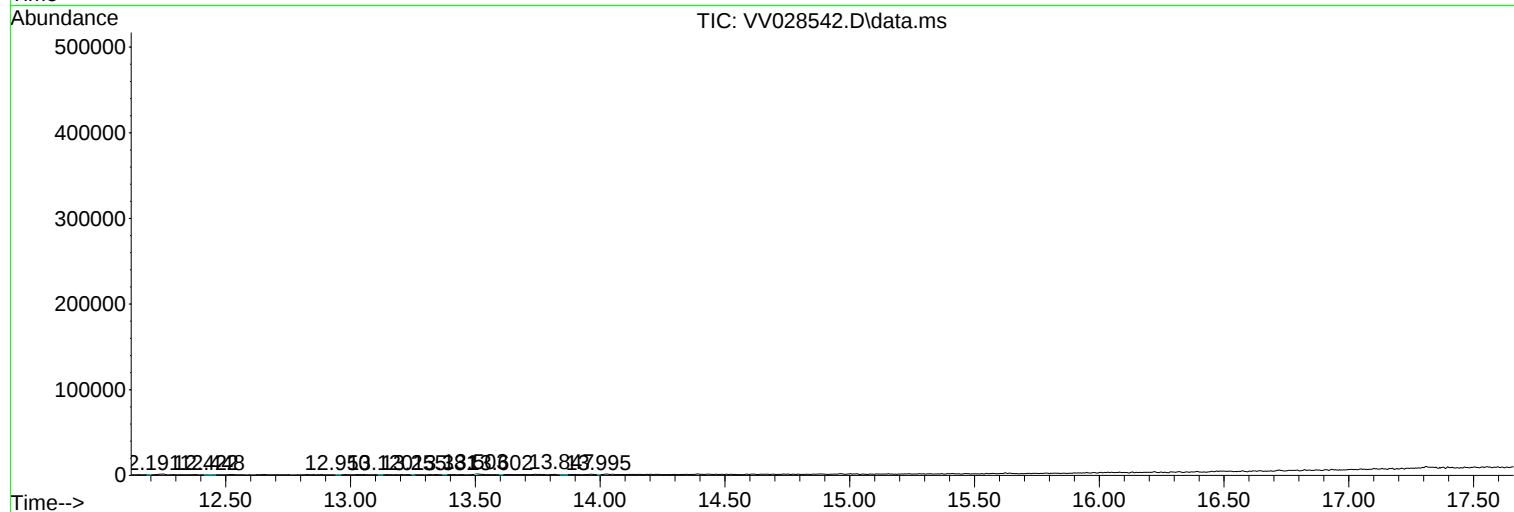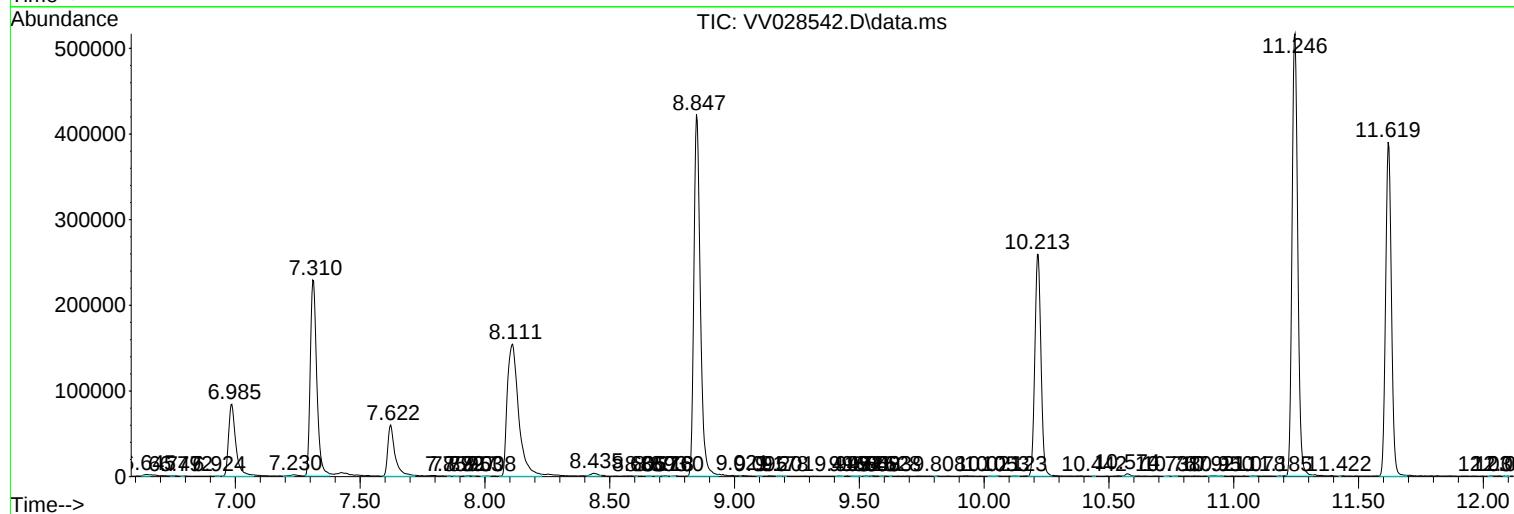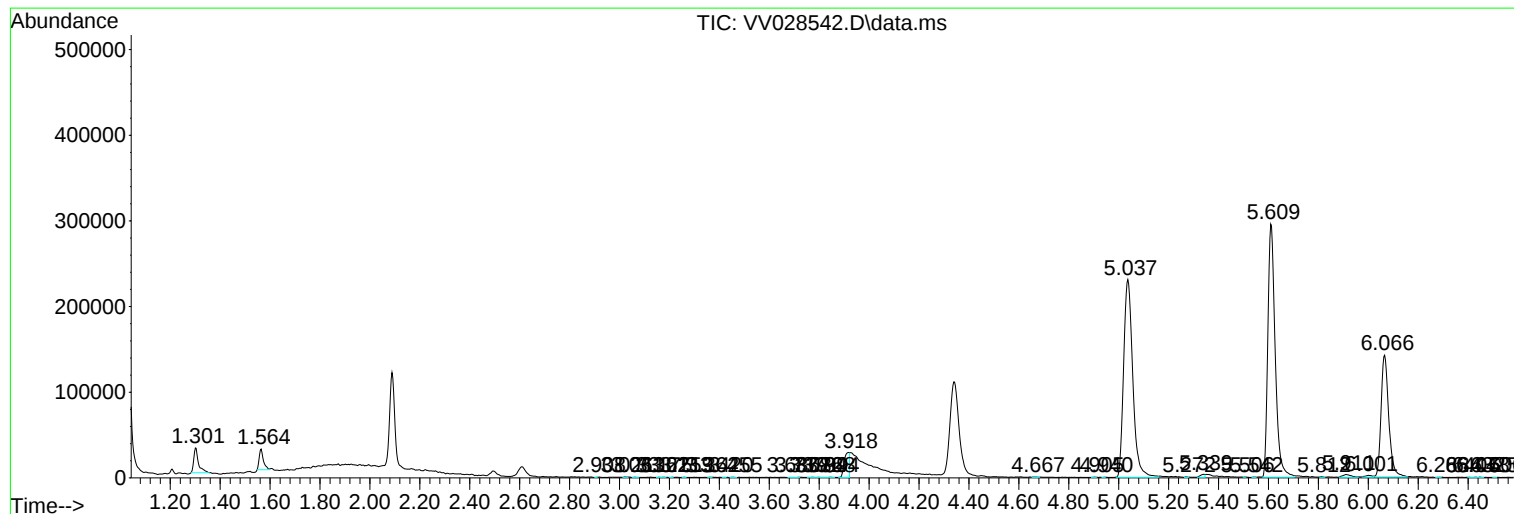

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028542.D
Acq On : 13 Oct 2022 17:15
Operator : SY/MD
Sample : N5023-07ME
Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
Data File : VV028542.D
Acq On : 13 Oct 2022 17:15
Operator : SY/MD
Sample : N5023-07ME
Misc : 6.14g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc