


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101322\
 Data File : VV028534.D
 Acq On : 13 Oct 2022 09:42
 Operator : SY/MD
 Sample : BFB330
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB330

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 14 04:49:18 2022

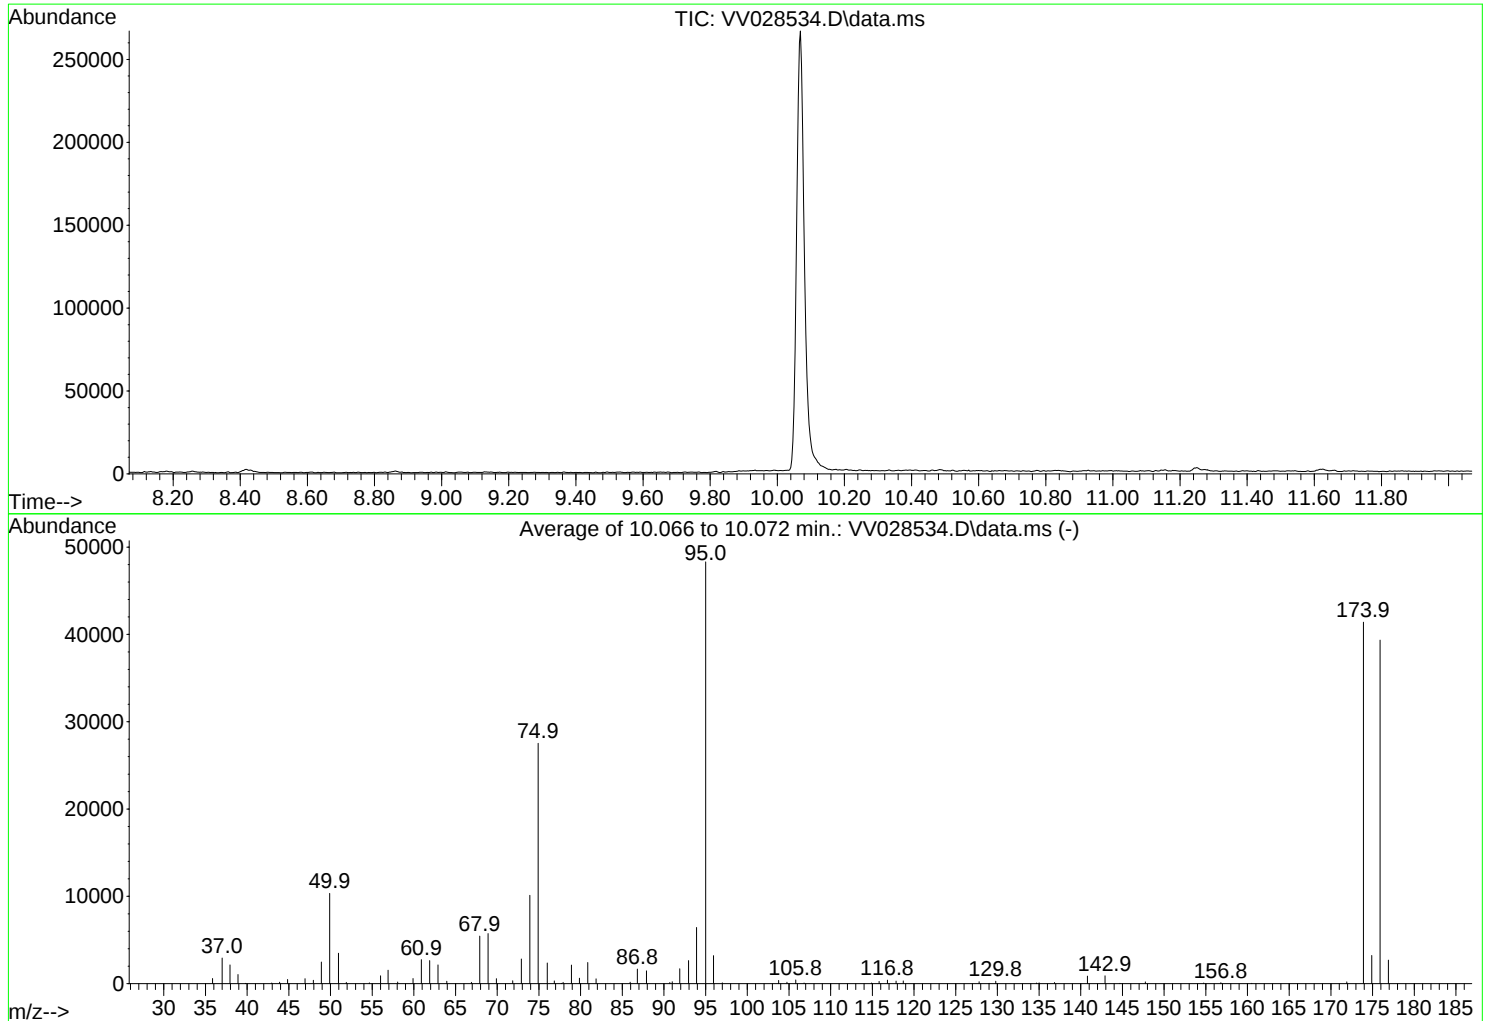

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	10341	PASS
75	95	30	80	57.0	27536	PASS
95	95	100	100	100.0	48315	PASS
96	95	5	9	6.7	3214	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.7	41400	PASS
175	174	5	9	7.8	3232	PASS
176	174	95	105	95.1	39352	PASS
177	176	5	10	6.9	2701	PASS

m/z	Abundance
35.90	749.0
37.80	430.0
39.80	469.0
44.00	473.0
54.60	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB330

m/z	Abundance
35.90	1367.0
37.00	3092.0
38.00	2684.0
38.90	1007.0
39.80	480.0
43.90	621.0
44.90	521.0
47.00	581.0
48.00	460.0
48.90	2484.0
49.90	10698.0
50.90	3548.0
51.90	163.0
54.80	190.0
56.00	992.0
56.90	1585.0
58.10	152.0
59.90	627.0
60.90	2665.0
61.90	2738.0
62.90	2192.0
63.90	263.0
66.90	152.0
67.90	5688.0
68.90	5763.0
69.90	601.0
71.80	323.0
72.90	2885.0
73.90	10416.0
74.90	28224.0
76.00	2417.0
76.80	309.0
77.70	137.0
78.90	2170.0
79.80	584.0
80.90	2359.0
81.90	540.0
86.00	130.0
86.80	1645.0
87.90	1571.0
91.00	224.0
91.90	1674.0
93.00	2662.0
93.90	6658.0
95.00	49256.0
96.00	3432.0
97.00	152.0
103.80	342.0
104.70	166.0
105.80	443.0
114.90	125.0
115.80	247.0
116.80	471.0
117.80	280.0
118.70	287.0
127.80	197.0
129.00	117.0
129.80	276.0
134.70	133.0
136.90	147.0
140.80	891.0
142.90	885.0
147.80	181.0
154.70	119.0
156.80	115.0
171.90	173.0
173.90	40608.0
174.90	3204.0
175.90	38824.0
176.90	2713.0

Instrument :
MSVOA_V
ClientSampleId :
BFB330

m/z	Abundance
35.90	1376.0
37.00	3063.0
38.00	2624.0
38.90	1114.0
39.90	498.0
42.90	104.0
43.90	666.0
44.80	480.0
46.90	592.0
47.90	385.0
48.90	2565.0
49.90	10682.0
50.90	3620.0
51.90	147.0
54.70	203.0
56.00	893.0
56.90	1609.0
58.00	199.0
59.90	602.0
60.90	2843.0
61.90	2739.0
62.90	2228.0
63.90	275.0
66.90	152.0
67.90	5574.0
68.90	5974.0
69.90	613.0
71.90	344.0
72.90	2950.0
73.90	10530.0
74.90	28400.0
76.00	2408.0
76.90	306.0
77.90	192.0
78.90	2183.0
79.80	627.0
80.90	2533.0
81.90	586.0
85.90	167.0
86.80	1744.0
87.90	1490.0
90.70	204.0
91.00	226.0
91.90	1756.0
93.00	2785.0
93.90	6721.0
95.00	49832.0
96.00	3342.0
97.00	107.0
103.80	385.0
104.70	182.0
105.80	456.0
106.80	103.0
114.90	114.0
115.80	264.0
116.80	397.0
117.80	305.0
118.70	312.0
127.80	231.0
129.80	286.0
135.00	140.0
136.80	134.0
140.80	891.0
142.90	980.0
147.80	218.0
156.80	117.0
160.50	104.0
171.90	226.0
173.90	43008.0
174.90	3358.0
175.90	40888.0
176.90	2800.0

Instrument :
MSVOA_V
ClientSampleId :
BFB330

m/z	Abundance
35.90	1267.0
37.00	2635.0
38.00	2392.0
38.90	1011.0
39.90	547.0
43.00	109.0
43.90	628.0
44.90	414.0
46.90	519.0
47.90	308.0
48.90	2373.0
49.90	9643.0
51.00	3277.0
51.90	142.0
54.70	214.0
56.00	784.0
56.90	1422.0
58.00	210.0
59.90	563.0
60.90	2729.0
61.90	2464.0
62.90	2008.0
64.00	297.0
66.90	146.0
67.90	5055.0
68.90	5477.0
69.90	497.0
71.90	342.0
72.90	2609.0
73.90	9408.0
74.90	25984.0
76.00	2269.0
76.90	299.0
77.90	274.0
78.90	2049.0
79.90	658.0
80.80	2344.0
81.80	521.0
85.90	209.0
86.80	1638.0
87.90	1350.0
90.70	190.0
91.00	203.0
91.90	1714.0
92.90	2469.0
93.90	5950.0
95.00	45856.0
95.90	2869.0
103.70	374.0
104.80	138.0
105.80	375.0
106.80	108.0
115.80	240.0
116.80	320.0
117.90	296.0
118.70	321.0
127.80	225.0
129.80	269.0
134.70	114.0
135.00	120.0
136.80	133.0
140.80	803.0
142.90	835.0
144.70	101.0
147.70	201.0
154.80	112.0
156.80	107.0
171.90	219.0
173.90	40584.0
174.90	3133.0
175.90	38344.0
176.90	2589.0

Instrument :
MSVOA_V
ClientSampleId :
BFB330