

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102122\
 Data File : VW028670.D
 Acq On : 21 Oct 2022 18:43
 Operator : SY/MD
 Sample : N5216-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA75

Quant Time: Oct 21 23:05:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 21 22:58:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.590	114	226922	5.000	ug/L	-0.01
28) Chlorobenzene-d5	8.853	117	144495	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	81363	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.294	65	87350	3.888	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%
7) Chloroethane-d5	1.558	69	73251	4.148	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.000%
11) 1,1-Dichloroethene-d2	2.095	63	123571	3.165	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	3.953	46	171797	40.628	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.260%
24) Chloroform-d	4.342	84	141494	4.246	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.000%
26) 1,2-Dichloroethane-d4	5.027	65	90538	5.016	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.034	84	314024	4.995	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
36) 1,2-Dichloropropane-d6	6.043	67	106892	5.422	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.400%
41) Toluene-d8	7.310	98	228199	5.019	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
43) trans-1,3-Dichloroprop...	7.622	79	21427	4.477	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.114	63	98015	49.327	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.660%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	50010	5.371	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.400%
66) 1,2-Dichlorobenzene-d4	11.615	152	76878	5.257	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.127	85	900	0.082	ug/L #	75
3) Chloromethane	1.230	50	1104	0.050	ug/L #	83
8) Chloroethane	1.574	64	194399	13.584	ug/L	97
10) 1,1,2-Trichloro-1,2,2-...	2.098	101	1474	0.095	ug/L #	29
13) Acetone	2.236	43	42348	15.623	ug/L	88
14) Carbon disulfide	2.278	76	6039	0.172	ug/L #	67
15) Methyl Acetate	2.513	43	44906	5.568	ug/L #	60
17) Methyl tert-butyl Ether	2.773	73	17084	0.427	ug/L #	1
18) trans-1,2-Dichloroethene	2.744	96	3513	0.220	ug/L	95
19) 1,1-Dichloroethane	3.175	63	4154	0.111	ug/L #	80
22) cis-1,2-Dichloroethene	3.892	96	1070	0.058	ug/L #	87
27) 1,2-Dichloroethane	5.082	62	238274	10.774	ug/L #	78
30) Cyclohexane	4.654	56	108484	3.977	ug/L	99
35) Methylcyclohexane	6.085	83	78840	3.211	ug/L #	86
38) Bromodichloromethane	6.509	83	898	0.052	ug/L #	23
39) cis-1,3-Dichloropropene	6.976	75	2558	0.136	ug/L #	47
42) Toluene	7.381	91	67305	1.199	ug/L	100
44) trans-1,3-Dichloropropene	7.831	75	1983	0.149	ug/L	93
52) Ethylbenzene	9.008	91	131202	2.261	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028670.D
 Acq On : 21 Oct 2022 18:43
 Operator : SY/MD
 Sample : N5216-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA75


Quant Time: Oct 21 23:05:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 21 22:58:36 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

53) m,p-Xylene	9.136	106	113974	5.375	ug/L	98
54) o-Xylene	9.538	106	222956	10.601	ug/L	97
55) Styrene	9.535	104	14456	0.403	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	10.262	83	14184	1.409	ug/L #	32
60) Isopropylbenzene	9.924	105	2311206	33.989	ug/L #	84
61) 1,2,3-Trichloropropane	11.265	75	103269	11.712	ug/L #	50
62) 1,3,5-Trimethylbenzene	10.908	105	131549	6.735	ug/L	96
63) 1,2,4-Trimethylbenzene	10.908	105	131549	2.501	ug/L	100
64) 1,3-Dichlorobenzene	11.175	146	37097	1.378	ug/L	96
65) 1,4-Dichlorobenzene	11.265	146	258069	9.495	ug/L	99
67) 1,2-Dichlorobenzene	11.635	146	110580	4.417	ug/L	97
68) 1,2-Dibromo-3-chloropr...	12.403	75	5328	3.447	ug/L #	9
70) 1,2,4-trichlorobenzene	13.255	180	1204	0.080	ug/L #	16
71) Naphthalene	13.493	128	89264	3.495	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 21 23:05:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 21 22:58:36 2022
Response via : Initial Calibration







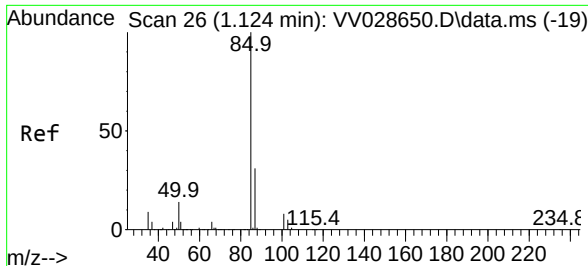

#2
 Dichlorodifluoromethane
 Concen: 0.082 ug/L
 RT: 1.127 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV028670.D
 Acq: 21 Oct 2022 18:43




Instrument :
 MSVOA_V
 ClientSampleId :
 BHA75


Tgt Ion: 85 Resp: 900
 Ion Ratio Lower Upper
 85 100
 87 47.6 26.6 40.0#

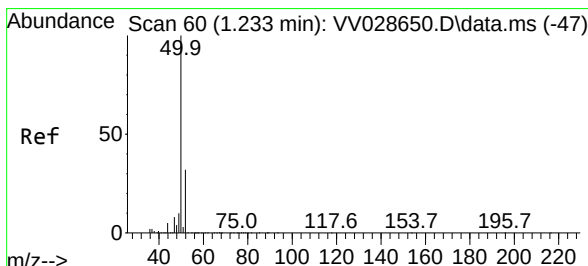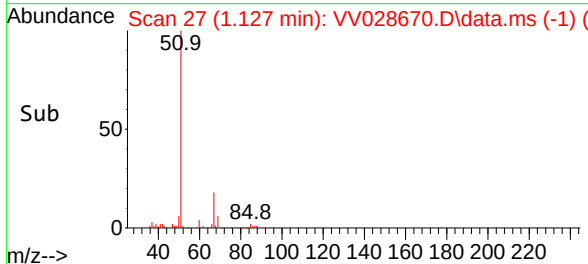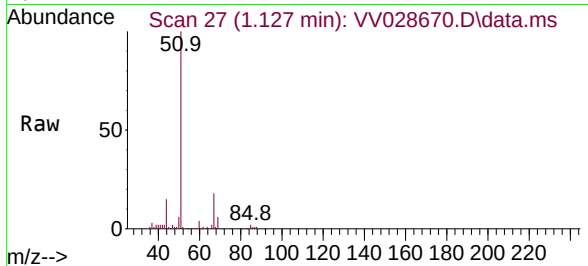

#3
 Chloromethane
 Concen: 0.050 ug/L
 RT: 1.230 min Scan# 59
 Delta R.T. -0.003 min
 Lab File: VV028670.D
 Acq: 21 Oct 2022 18:43

Tgt Ion: 50 Resp: 1104
 Ion Ratio Lower Upper
 50 100
 52 40.7 21.8 40.6#


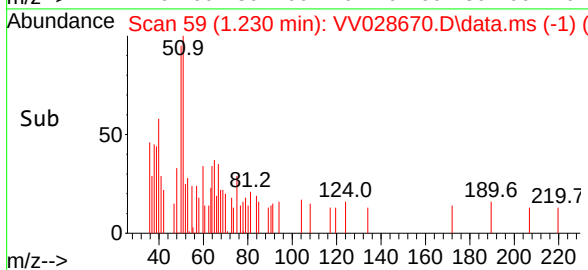

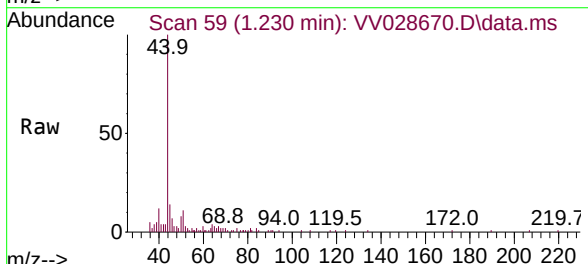




#8
Chloroethane
Concen: 13.584 ug/L
RT: 1.574 min Scan# 1
Delta R.T. -0.003 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion: 64 Resp: 194399
Ion Ratio Lower Upper
64 100
66 32.7 23.9 44.5

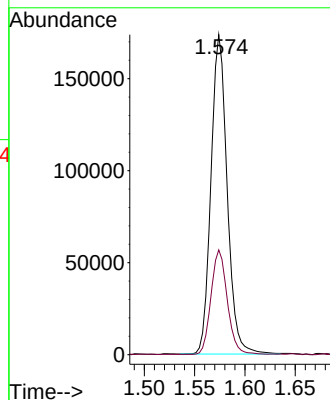

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.095 ug/L
RT: 2.098 min Scan# 329
Delta R.T. -0.007 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion: 101 Resp: 1474
Ion Ratio Lower Upper
101 100
85 5.0 37.0 55.6#
151 2.8 50.2 75.2#



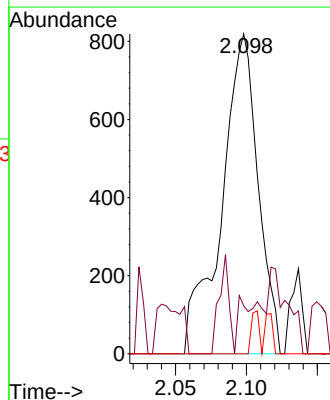
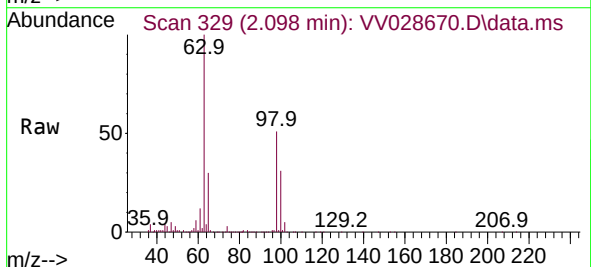




#13
Acetone
Concen: 15.623 ug/L
RT: 2.236 min Scan# 31
Delta R.T. -0.007 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion: 43 Resp: 42348
Ion Ratio Lower Upper
43 100
58 19.2 0.0 50.2

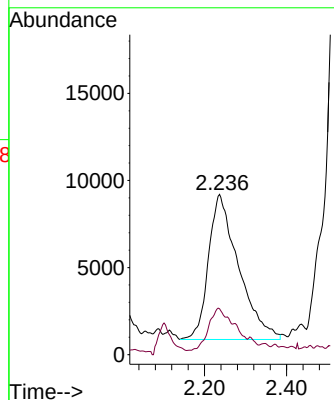

#14
Carbon disulfide
Concen: 0.172 ug/L
RT: 2.278 min Scan# 385
Delta R.T. -0.003 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion: 76 Resp: 6039
Ion Ratio Lower Upper
76 100
78 20.9 7.1 10.7#



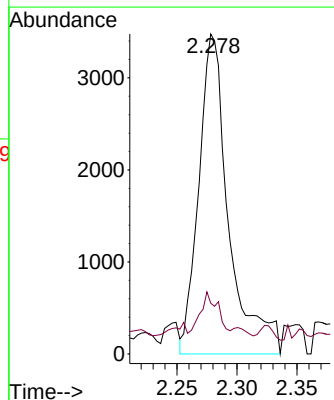





#15
Methyl Acetate
Concen: 5.568 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.067 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion: 43 Resp: 44906
Ion Ratio Lower Upper
43 100
74 0.7 14.9 22.3#

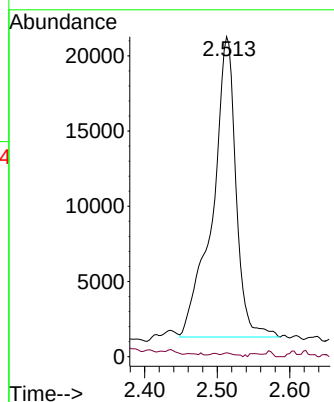

#17
Methyl tert-butyl Ether
Concen: 0.427 ug/L
RT: 2.773 min Scan# 539
Delta R.T. 0.003 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion: 73 Resp: 17084
Ion Ratio Lower Upper
73 100
43 178.4 18.0 27.0#
57 589.8 20.0 30.0#



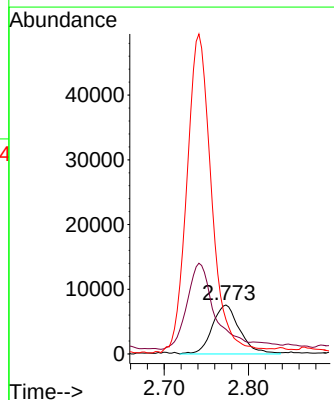





#18
trans-1,2-Dichloroethene
Concen: 0.220 ug/L
RT: 2.744 min Scan# 51
Delta R.T. 0.003 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion: 96 Resp: 3513
Ion Ratio Lower Upper
96 100
61 170.8 114.3 212.3
98 61.9 45.0 83.6

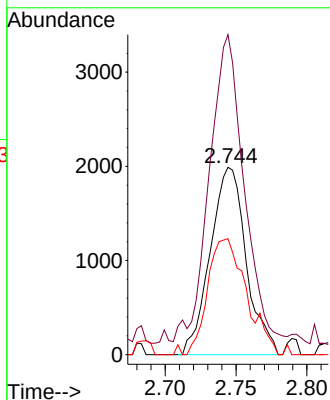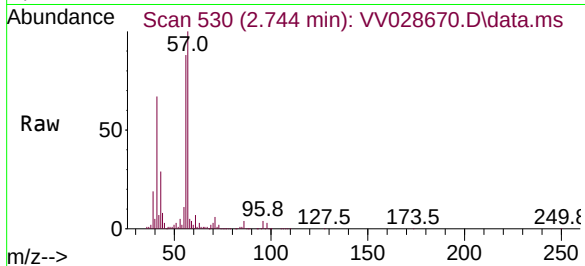

#19
1,1-Dichloroethane
Concen: 0.111 ug/L
RT: 3.175 min Scan# 664
Delta R.T. 0.003 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion: 63 Resp: 4154
Ion Ratio Lower Upper
63 100
65 42.8 23.1 42.9
83 22.1 7.9 14.7#


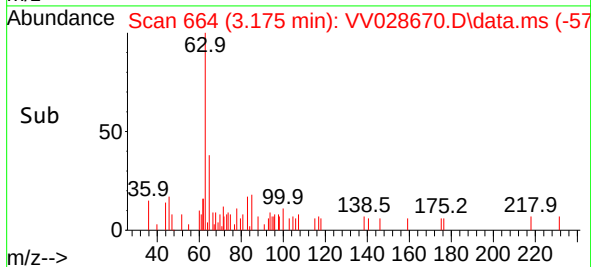
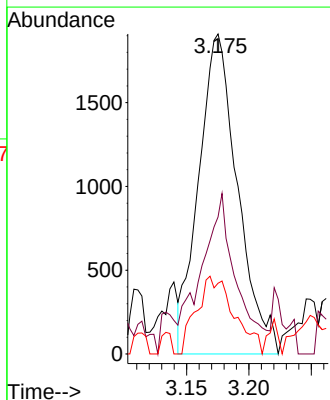
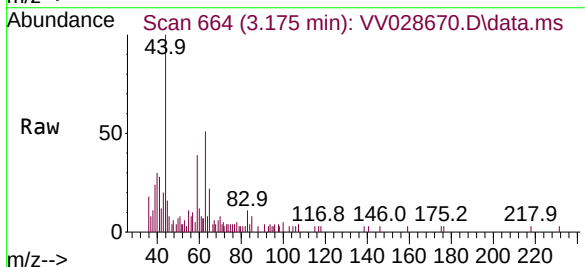




#22
 cis-1,2-Dichloroethene
 Concen: 0.058 ug/L
 RT: 3.892 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VV028670.D
 Acq: 21 Oct 2022 18:43




Instrument :
 MSVOA_V
 ClientSampleId :
 BHA75


Tgt Ion: 96 Resp: 1070
 Ion Ratio Lower Upper
 96 100
 61 160.9 101.4 188.2
 68 10.8 0.5 0.9#

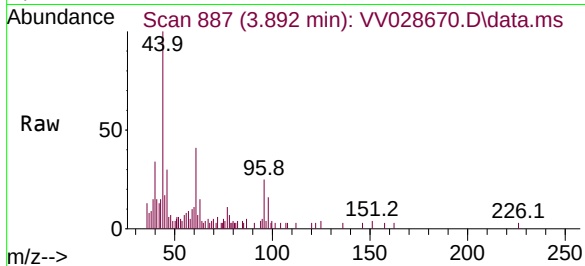

#27
 1,2-Dichloroethane
 Concen: 10.774 ug/L
 RT: 5.082 min Scan# 1257
 Delta R.T. -0.039 min
 Lab File: VV028670.D
 Acq: 21 Oct 2022 18:43

Tgt Ion: 62 Resp: 238274
 Ion Ratio Lower Upper
 62 100
 98 0.4 6.6 9.8#




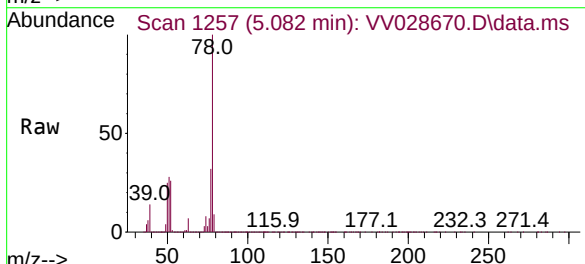




#30
Cyclohexane
Concen: 3.977 ug/L
RT: 4.654 min Scan# 1121
Delta R.T. 0.010 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion: 56 Resp: 108484
Ion Ratio Lower Upper
56 100
69 27.2 22.6 34.0
84 75.6 60.4 90.6



#35
Methylcyclohexane
Concen: 3.211 ug/L
RT: 6.085 min Scan# 1569
Delta R.T. -0.019 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion: 83 Resp: 78840
Ion Ratio Lower Upper
83 100
55 106.9 70.0 105.0#
98 45.2 35.6 53.4









#38
Bromodichloromethane
Concen: 0.052 ug/L
RT: 6.509 min Scan# 1
Delta R.T. 0.013 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion: 83 Resp: 898
Ion Ratio Lower Upper
83 100
85 0.0 45.1 83.9#
127 16.6 5.7 8.5#



#39
cis-1,3-Dichloropropene
Concen: 0.136 ug/L
RT: 6.976 min Scan# 1846
Delta R.T. -0.042 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion: 75 Resp: 2558
Ion Ratio Lower Upper
75 100
77 61.0 22.1 41.1#





#42

Toluene

Concen: 1.199 ug/L

RT: 7.381 min Scan# 11

Delta R.T. 0.006 min

Lab File: VV028670.D

Acq: 21 Oct 2022 18:43

Instrument :

MSVOA_V

ClientSampleId :





BHA75

Tgt Ion: 91 Resp: 67305

Ion Ratio Lower Upper

91 100

92 57.8 40.5 75.3

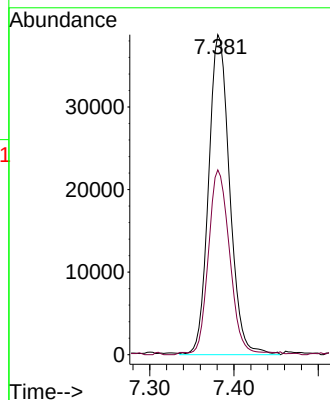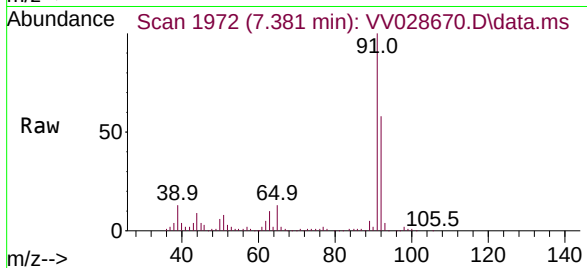

#44

trans-1,3-Dichloropropene

Concen: 0.149 ug/L

RT: 7.831 min Scan# 2112

Delta R.T. 0.186 min

Lab File: VV028670.D




Acq: 21 Oct 2022 18:43


Tgt Ion: 75 Resp: 1983

Ion Ratio Lower Upper

75 100

77 36.5 22.6 42.0

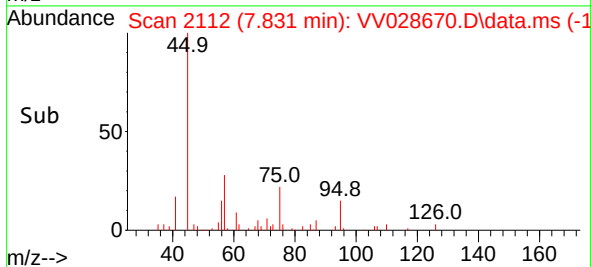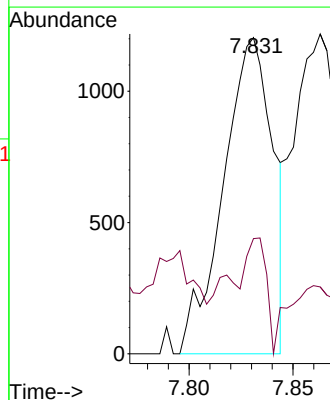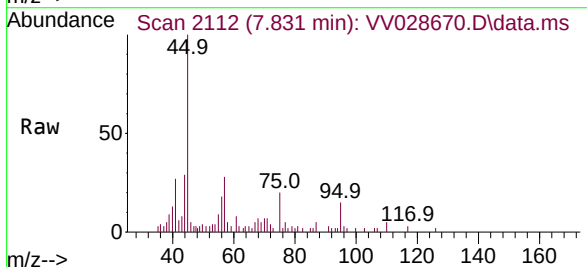



#52

Ethylbenzene

Concen: 2.261 ug/L

RT: 9.008 min Scan# 2476

Delta R.T. 0.006 min

Lab File: VV028670.D

Acq: 21 Oct 2022 18:43

Instrument :

MSVOA_V

ClientSampleId :





BHA75

Tgt Ion: 91 Resp: 131202

Ion Ratio Lower Upper

91 100

106 29.6 21.3 39.6

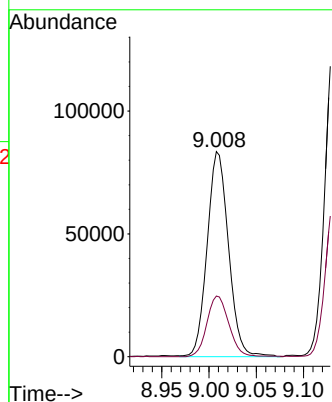

#53

m,p-Xylene

Concen: 5.375 ug/L

RT: 9.136 min Scan# 2518

Delta R.T. 0.006 min

Lab File: VV028670.D




Acq: 21 Oct 2022 18:43


Tgt Ion:106 Resp: 113974

Ion Ratio Lower Upper

106 100

91 210.5 145.5 270.1







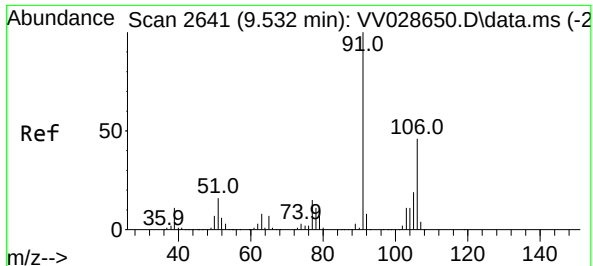

#54
o-Xylene
Concen: 10.601 ug/L
RT: 9.538 min Scan# 2642
Delta R.T. 0.006 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion:106 Resp: 222956
Ion Ratio Lower Upper
106 100
91 222.3 159.0 295.4

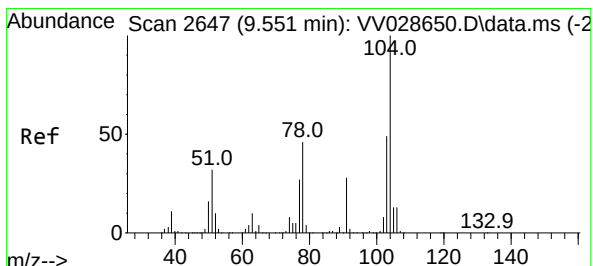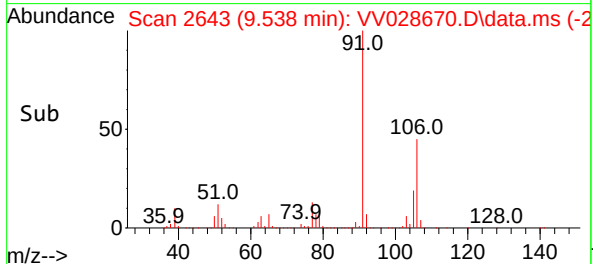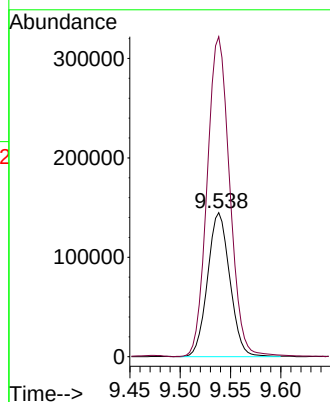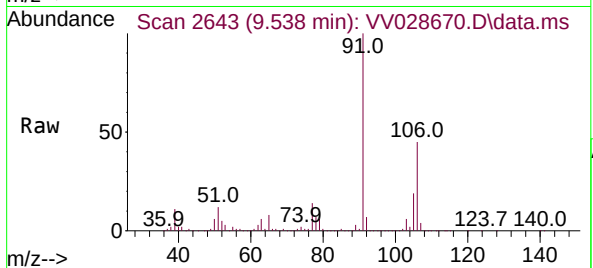

#55
Styrene
Concen: 0.403 ug/L
RT: 9.535 min Scan# 2642
Delta R.T. -0.016 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion:104 Resp: 14456
Ion Ratio Lower Upper
104 100
78 299.5 32.8 61.0#

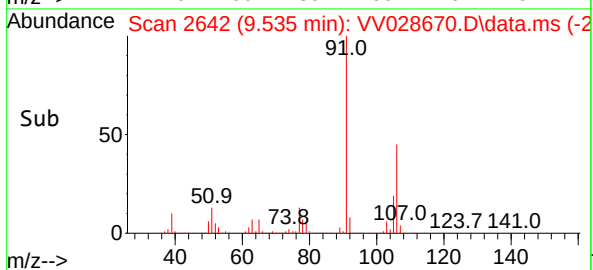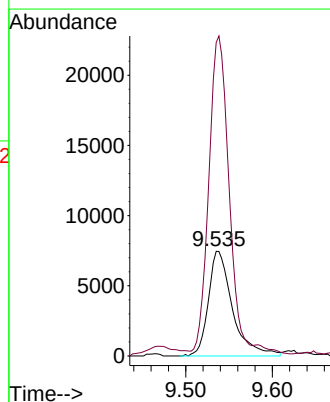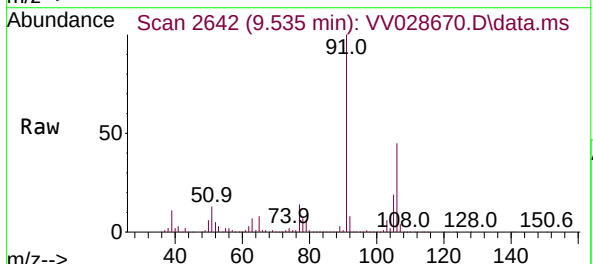



#57

1,1,2-Tetrachloroethane

Concen: 1.409 ug/L

RT: 10.262 min Scan# 2868

Delta R.T. 0.026 min

Lab File: VV028670.D

Acq: 21 Oct 2022 18:43

Instrument :

MSVOA_V

ClientSampleId :

BHA75





Tgt Ion: 83 Resp: 14184

Ion Ratio Lower Upper

83 100

85 4.9 43.0 80.0#

131 0.0 6.5 9.7#

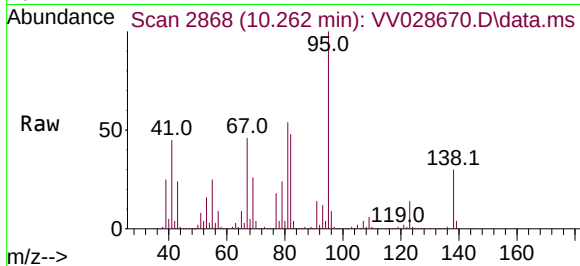

#60

Isopropylbenzene

Concen: 33.989 ug/L

RT: 9.924 min Scan# 2763

Delta R.T. 0.003 min

Lab File: VV028670.D

Acq: 21 Oct 2022 18:43




Tgt Ion: 105 Resp: 2311206


Ion Ratio Lower Upper

105 100

120 25.4 20.1 30.1

77 0.0 13.4 20.0#

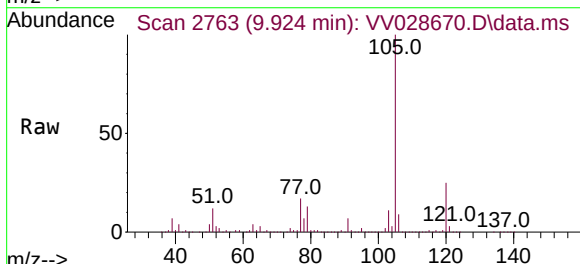



#61

1,2,3-Trichloropropane

Concen: 11.712 ug/L

RT: 11.265 min Scan# 3180

Delta R.T. 0.997 min

Lab File: VV028670.D

Acq: 21 Oct 2022 18:43

Instrument :

MSVOA_V

ClientSampleId :

BHA75





Tgt Ion: 75 Resp: 103269

Ion Ratio Lower Upper

75 100

77 0.0 25.2 37.8#

110 9.3 27.9 41.9#

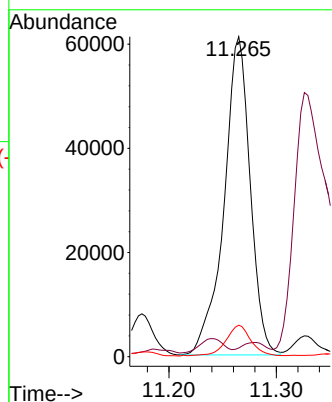

#62

1,3,5-Trimethylbenzene

Concen: 6.735 ug/L

RT: 10.908 min Scan# 3069

Delta R.T. 0.379 min

Lab File: VV028670.D




Acq: 21 Oct 2022 18:43


Tgt Ion: 105 Resp: 131549

Ion Ratio Lower Upper

105 100

120 45.2 38.3 57.5







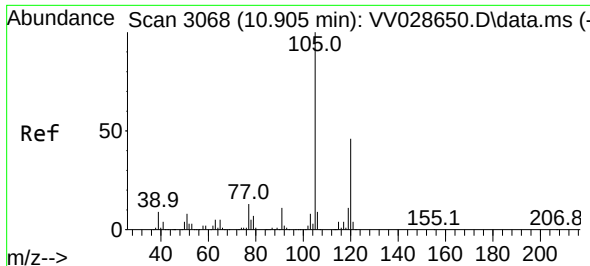

#63
 1,2,4-Trimethylbenzene
 Concen: 2.501 ug/L
 RT: 10.908 min Scan# 3069
 Delta R.T. 0.003 min
 Lab File: VV028670.D
 Acq: 21 Oct 2022 18:43




Instrument :
 MSVOA_V
 ClientSampleId :
 BHA75


Tgt Ion:105 Resp: 131549
 Ion Ratio Lower Upper
 105 100
 120 45.2 36.2 54.2

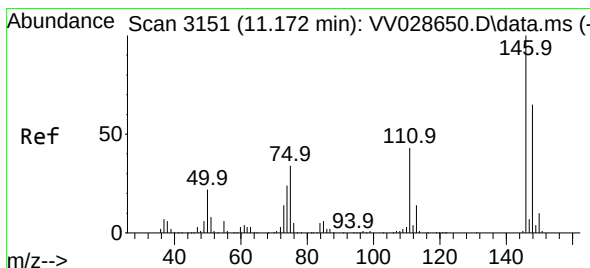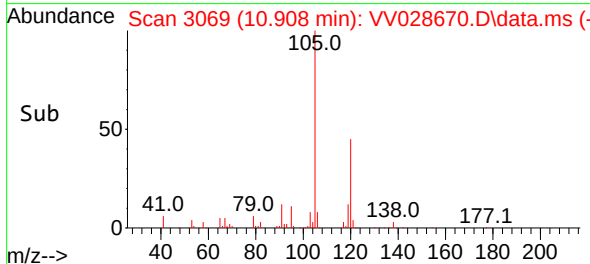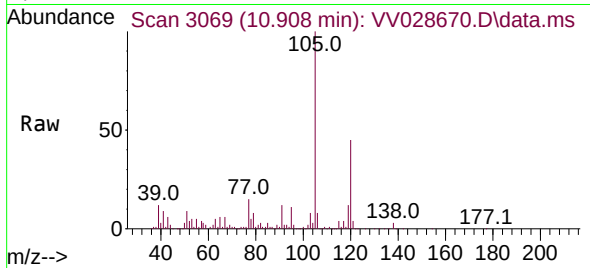

#64
 1,3-Dichlorobenzene
 Concen: 1.378 ug/L
 RT: 11.175 min Scan# 3152
 Delta R.T. 0.003 min
 Lab File: VV028670.D
 Acq: 21 Oct 2022 18:43

Tgt Ion:146 Resp: 37097
 Ion Ratio Lower Upper
 146 100
 111 43.4 29.0 53.9
 148 60.4 44.5 82.7


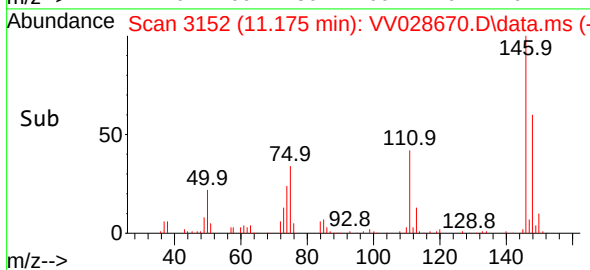

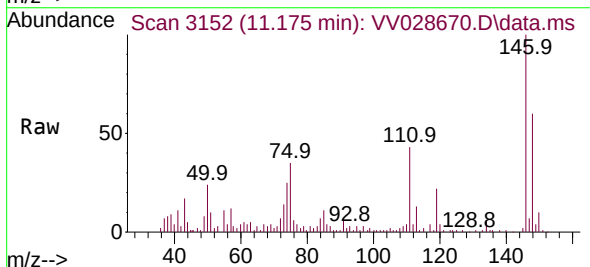




#65
1,4-Dichlorobenzene
Concen: 9.495 ug/L
RT: 11.265 min Scan# 3180
Delta R.T. -0.000 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion:146 Resp: 258069
Ion Ratio Lower Upper
146 100
111 39.9 28.6 53.2
148 63.9 44.3 82.3



#67
1,2-Dichlorobenzene
Concen: 4.417 ug/L
RT: 11.635 min Scan# 3295
Delta R.T. 0.003 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion:146 Resp: 110580
Ion Ratio Lower Upper
146 100
111 46.8 36.2 54.4
148 65.5 50.6 75.8




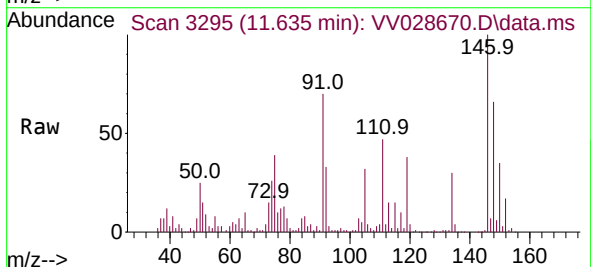


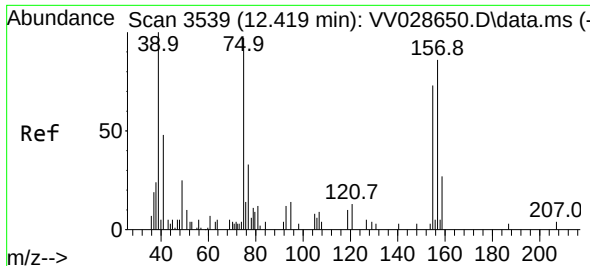

#68
1,2-Dibromo-3-chloropropane
Concen: 3.447 ug/L
RT: 12.403 min Scan# 3539
Delta R.T. -0.016 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43




Instrument :
MSVOA_V
ClientSampleId :
BHA75


Tgt Ion: 75 Resp: 5328
Ion Ratio Lower Upper
75 100
155 0.0 58.2 87.2#
157 0.0 71.5 107.3#

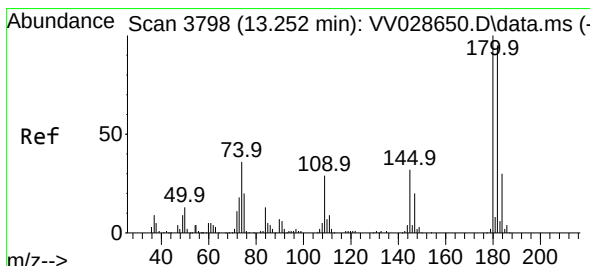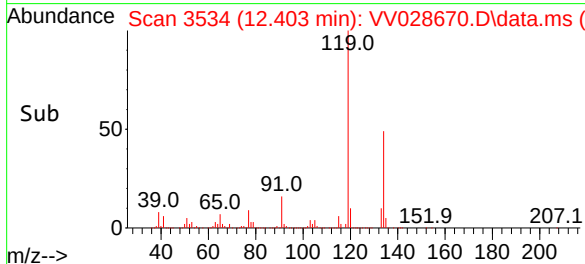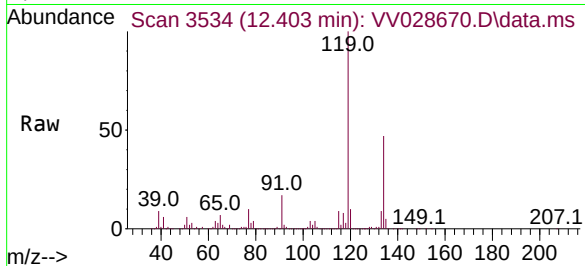

#70
1,2,4-trichlorobenzene
Concen: 0.080 ug/L
RT: 13.255 min Scan# 3799
Delta R.T. 0.003 min
Lab File: VV028670.D
Acq: 21 Oct 2022 18:43

Tgt Ion:180 Resp: 1204
Ion Ratio Lower Upper
180 100
182 83.1 74.7 112.1
145 197.5 25.5 38.3#

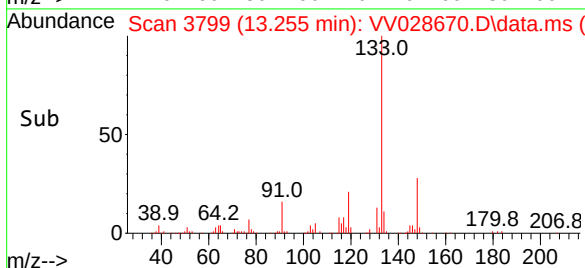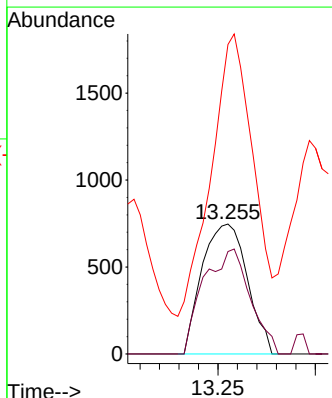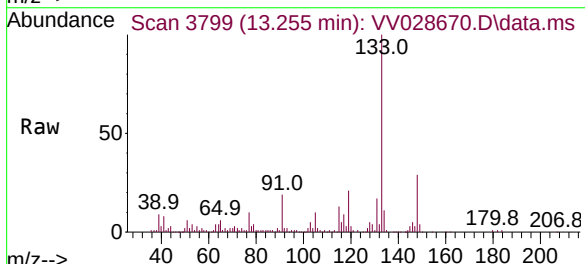



#71

Naphthalene

Concen: 3.495 ug/L

RT: 13.493 min Scan# 3873

Delta R.T. -0.000 min

Lab File: VV028670.D


Acq: 21 Oct 2022 18:43

Instrument :

MSVOA_V

ClientSampleId :

BHA75



Tgt Ion:128 Resp: 89264

Ion Ratio Lower Upper

128 100

129 10.7 8.9 13.3

127 13.6 10.2 15.4

