




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028653.D
 Acq On : 21 Oct 2022 11:30
 Operator : SY/MD
 Sample : N5216-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD1

Manual IntegrationsAPPROVED

Quant Time: Oct 21 23:00:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 21 22:58:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

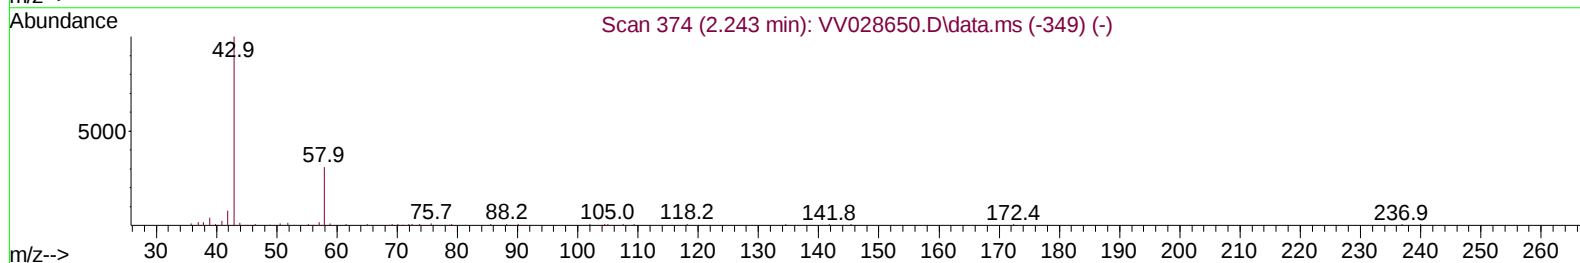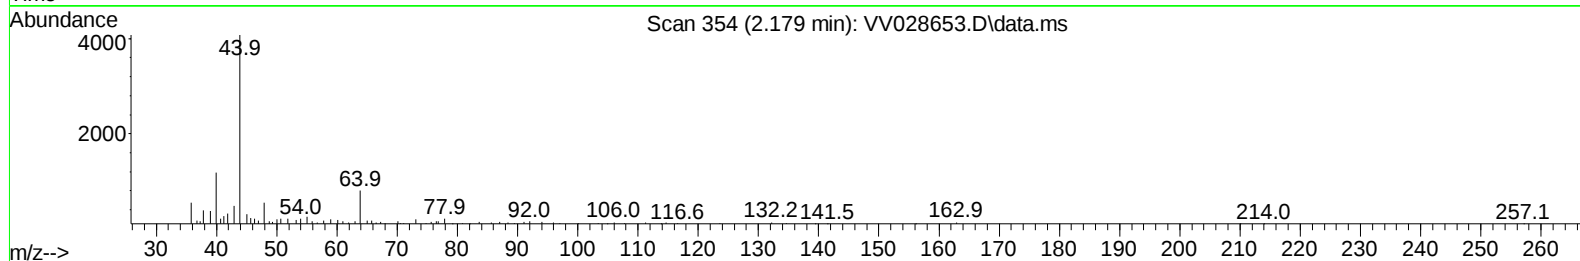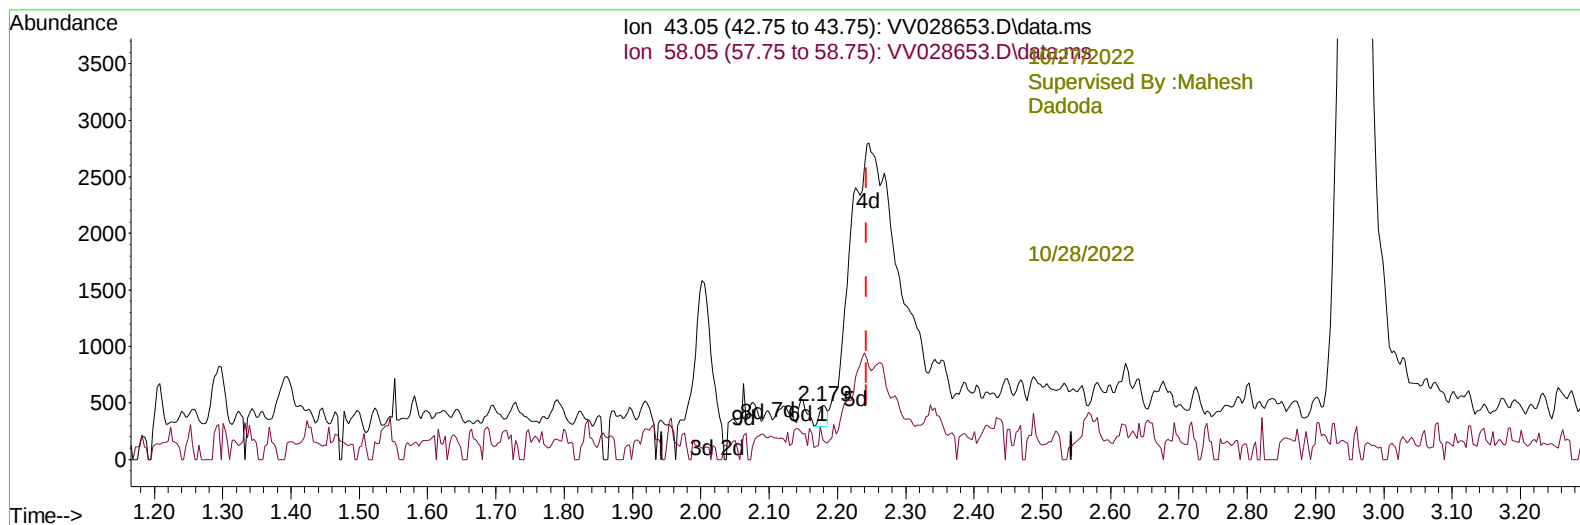

TIC: VV028653.D\data.ms

(13) Acetone (T)

2.179min (-0.064) 0.05 ug/L

response 142

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.10	41.55
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028653.D
 Acq On : 21 Oct 2022 11:30
 Operator : SY/MD
 Sample : N5216-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD1

Manual IntegrationsAPPROVED

Quant Time: Oct 21 23:00:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 21 22:58:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

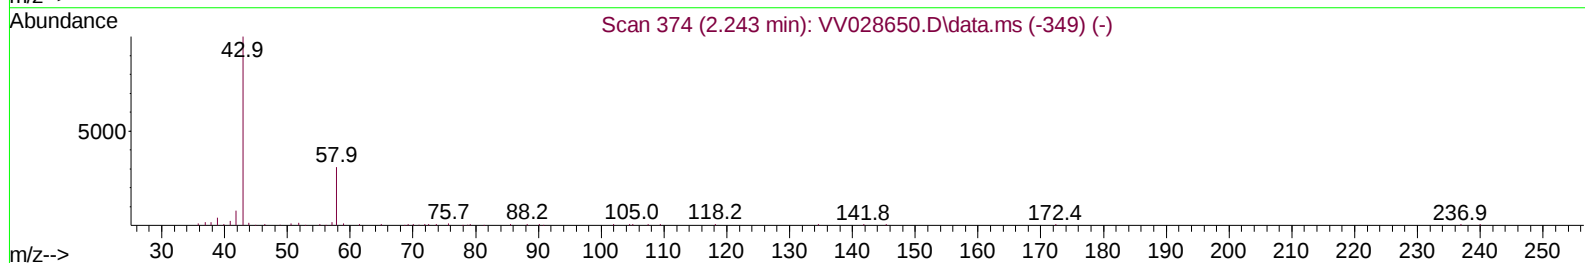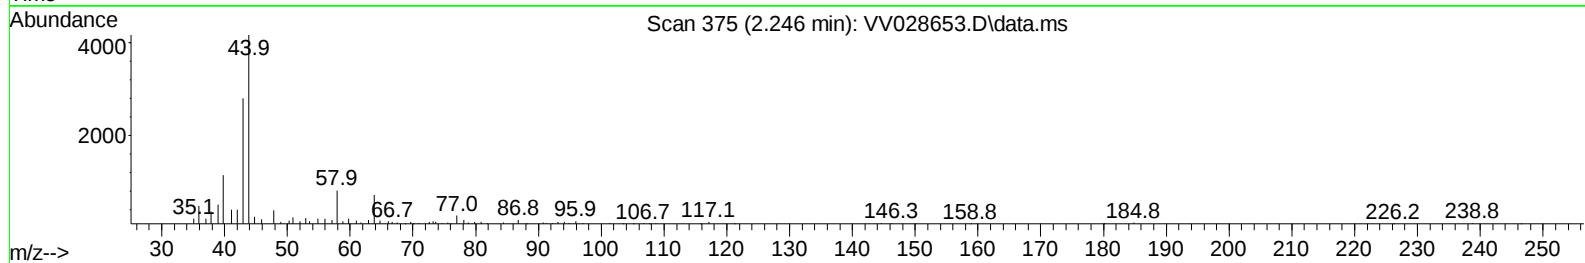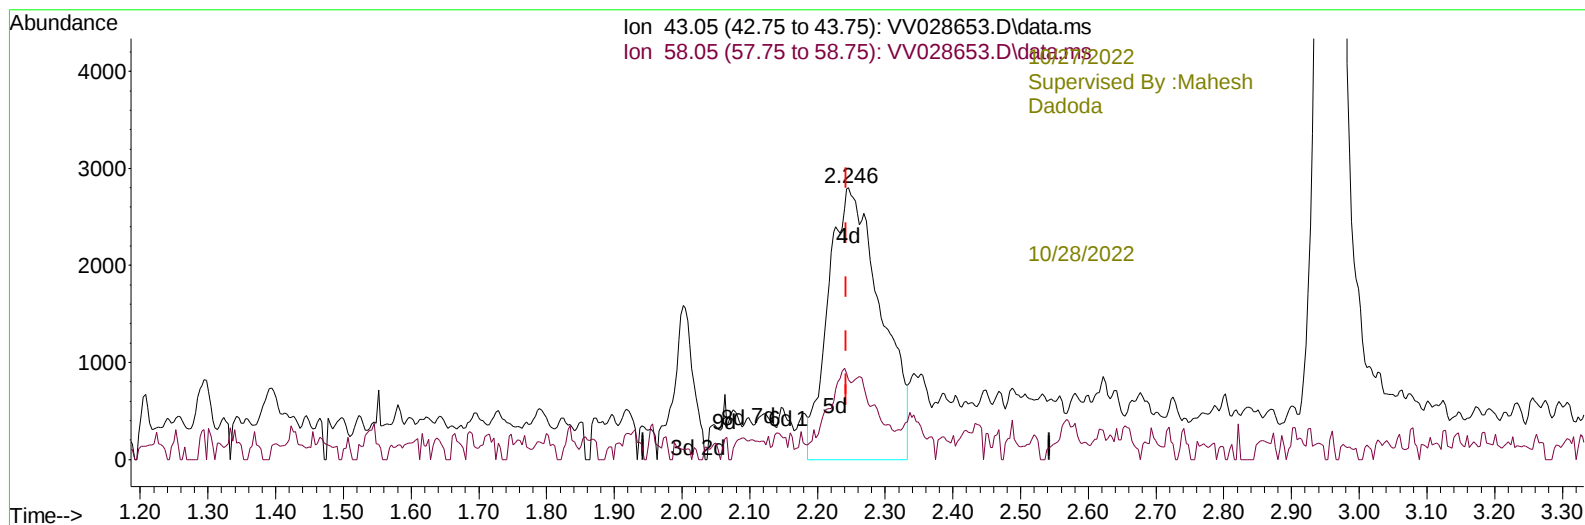

TIC: VV028653.D\data.ms

(13) Acetone (T)

2.246min (+ 0.003) 5.81 ug/L m

response 15112

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	25.10	0.39
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028653.D
 Acq On : 21 Oct 2022 11:30
 Operator : SY/MD
 Sample : N5216-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD1

Manual IntegrationsAPPROVED

Quant Time: Oct 21 23:00:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 21 22:58:36 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----10/27/2022							
Supervised By :Mahesh							
Padoda							
Internal Standards							
1) 1,4-Difluorobenzene	5.603	114		217670	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117		140267	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152		61110	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.294	65		103650	4.810	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.200%	
7) Chloroethane-d5	1.558	69		84167	4.969	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2	2.095	63		146072	3.900	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.000%	
20) 2-Butanone-d5	3.957	46		203632	50.204	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.400%	
24) Chloroform-d	4.333	84		168228	5.263	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.200%	
26) 1,2-Dichloroethane-d4	5.024	65		87590	5.059	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%	
32) Benzene-d6	5.031	84		341885	5.602	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.000%	
36) 1,2-Dichloropropane-d6	6.056	67		118206	6.177	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	123.600%	
41) Toluene-d8	7.301	98		232948	5.278	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.600%	
43) trans-1,3-Dichloroprop...	7.616	79		18786	4.044	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.800%	
46) 2-Hexanone-d5	8.104	63		90585	46.962	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.920%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84		45740	5.060	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	11.616	152		57664	5.250	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%	
Target Compounds							
						Qvalue	
13) Acetone	2.246	43		15112m	5.812	ug/L	
25) Chloroform	4.362	83		89038	2.626	ug/L	98
42) Toluene	7.375	91		11118	0.204	ug/L	97
53) m,p-Xylene	9.133	106		2175	0.106	ug/L	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028653.D
Acq On : 21 Oct 2022 11:30
Operator : SY/MD
Sample : N5216-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD1

Manual IntegrationsAPPROVED

Quant Time: Oct 21 23:00:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 21 22:58:36 2022
Response via : Initial Calibration

Reviewed By :Krupa
Patel

