

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102122\
 Data File : VW028657.D
 Acq On : 21 Oct 2022 13:05
 Operator : SY/MD
 Sample : N5163-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD716

Quant Time: Oct 21 23:01:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 21 22:58:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	220825	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	147158	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	65530	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	93602	4.281	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.600%
7) Chloroethane-d5	1.565	69	74309	4.324	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.400%
11) 1,1-Dichloroethene-d2	2.102	63	134452	3.539	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.800%
20) 2-Butanone-d5	3.957	46	235023	57.115	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.240%
24) Chloroform-d	4.336	84	150792	4.650	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	5.024	65	83645	4.762	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%
32) Benzene-d6	5.031	84	315749	4.931	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
36) 1,2-Dichloropropane-d6	6.063	67	73029	3.638	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	72.800%
41) Toluene-d8	7.310	98	182623	3.944	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.800%
43) trans-1,3-Dichloroprop...	7.622	79	17360	3.562	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.200%
46) 2-Hexanone-d5	8.108	63	90110	44.528	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.060%
56) 1,1,2,2-Tetrachloroeth...	10.211	84	44422	4.684	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	11.616	152	57332	4.867	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds						
					Qvalue	
33) Benzene	5.082	78	35411	0.513	ug/L	100
42) Toluene	7.384	91	69644	1.218	ug/L	99
53) m,p-Xylene	9.137	106	7969	0.369	ug/L	98
54) o-Xylene	9.539	106	13434	0.627	ug/L	96
62) 1,3,5-Trimethylbenzene	10.532	105	2828	0.180	ug/L	96
63) 1,2,4-Trimethylbenzene	10.911	105	3152	0.074	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028657.D
Acq On : 21 Oct 2022 13:05
Operator : SY/MD
Sample : N5163-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD716

Quant Time: Oct 21 23:01:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 21 22:58:36 2022
Response via : Initial Calibration




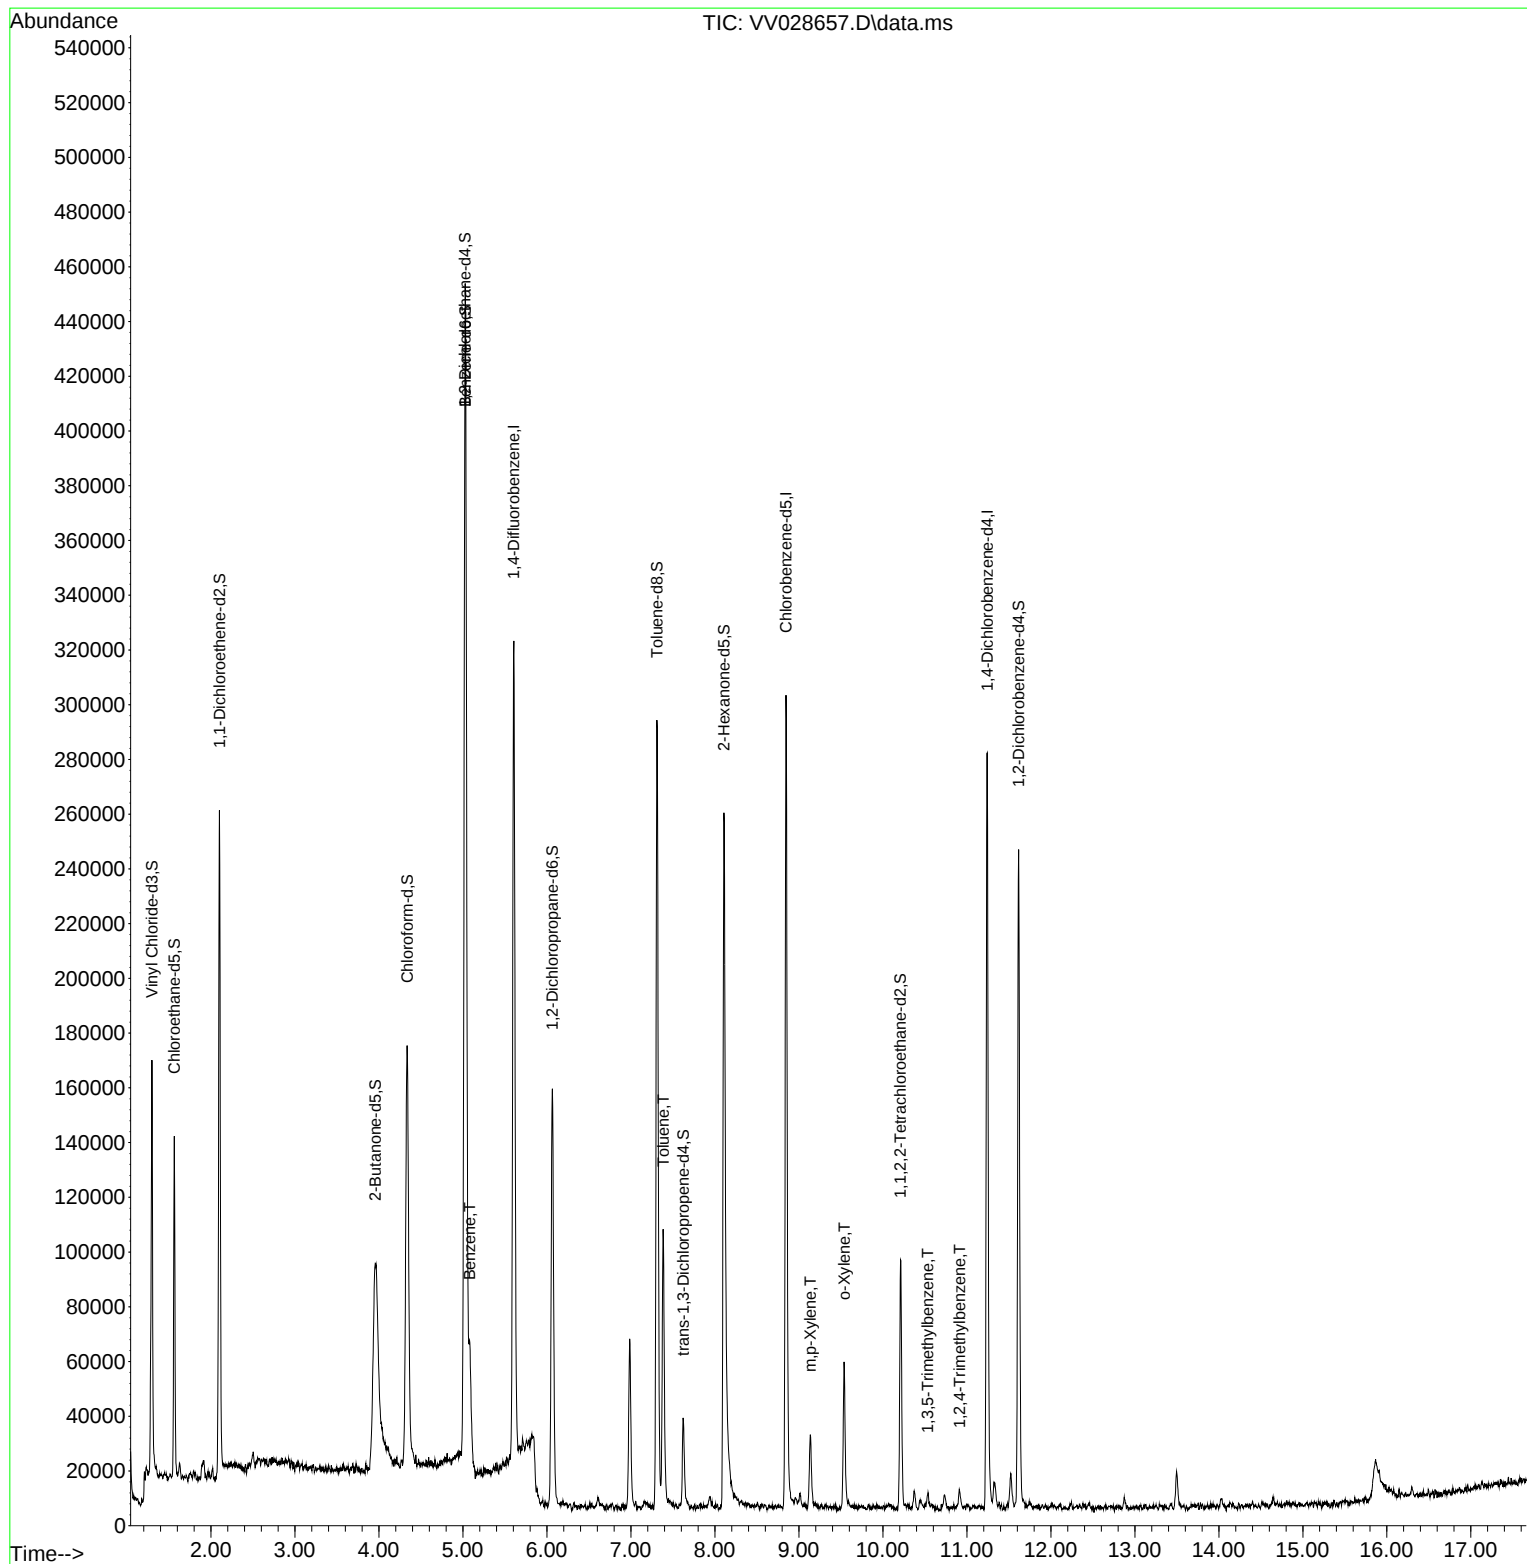


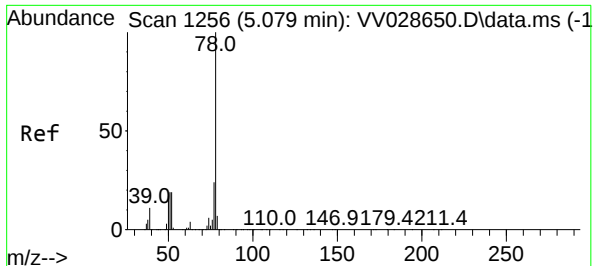

#33
Benzene
Concen: 0.513 ug/L
RT: 5.082 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV028657.D
Acq: 21 Oct 2022 13:05




Instrument :
MSVOA_V
ClientSampleId :
BD716


Tgt Ion: 78 Resp: 35411

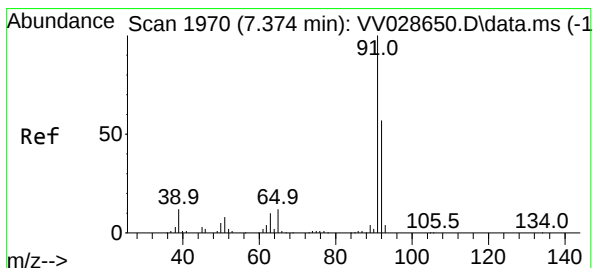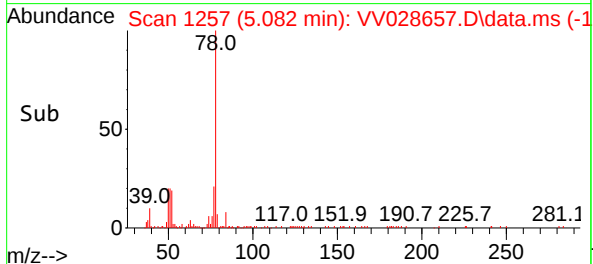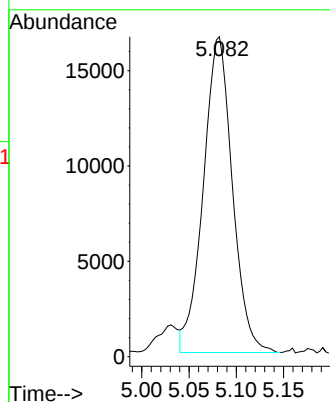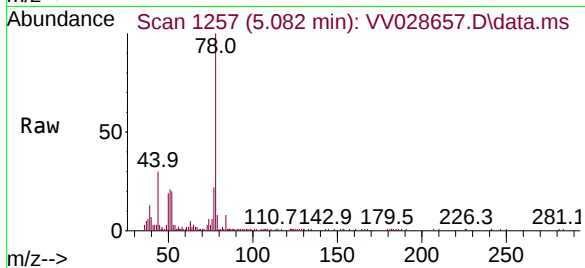

#42
Toluene
Concen: 1.218 ug/L
RT: 7.384 min Scan# 1973
Delta R.T. 0.010 min
Lab File: VV028657.D
Acq: 21 Oct 2022 13:05

Tgt Ion: 91 Resp: 69644
Ion Ratio Lower Upper
91 100
92 57.0 40.5 75.3


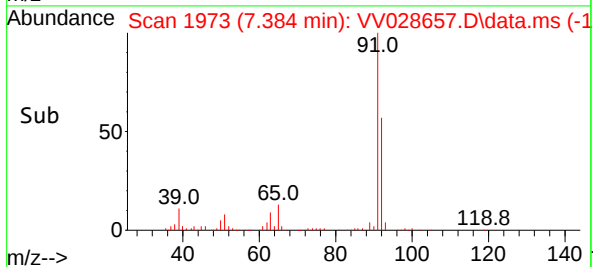
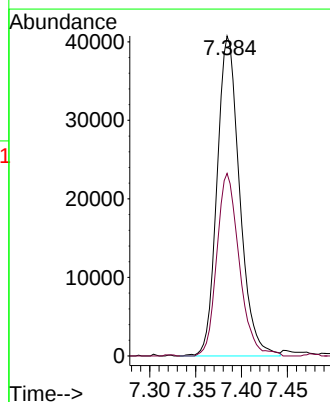
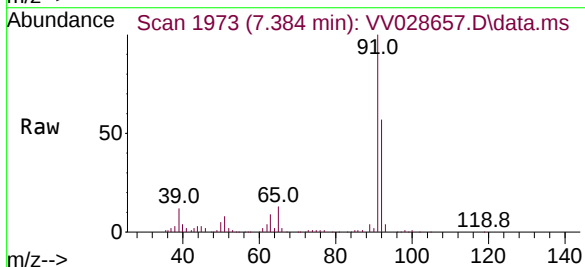


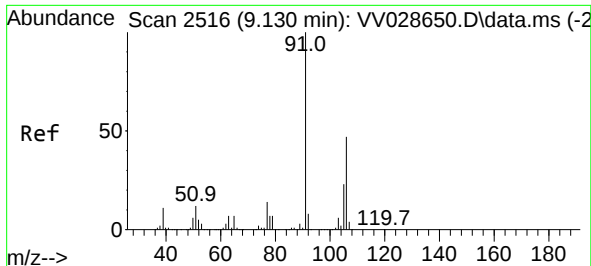

#53
m,p-Xylene
Concen: 0.369 ug/L
RT: 9.137 min Scan# 2516
Delta R.T. 0.007 min
Lab File: VV028657.D
Acq: 21 Oct 2022 13:05




Instrument :
MSVOA_V
ClientSampleId :
BD716


Tgt Ion:106 Resp: 7969
Ion Ratio Lower Upper
106 100
91 211.2 145.5 270.1

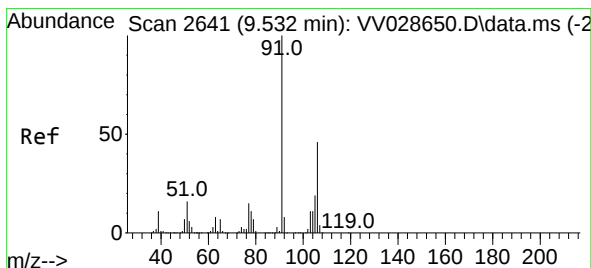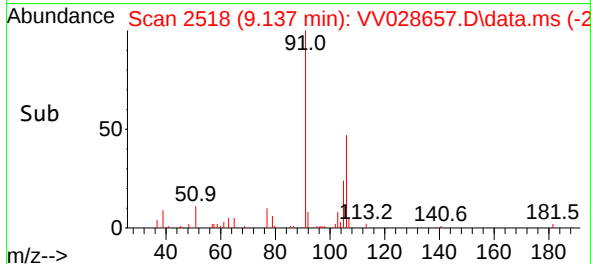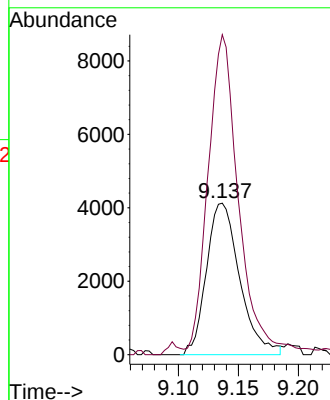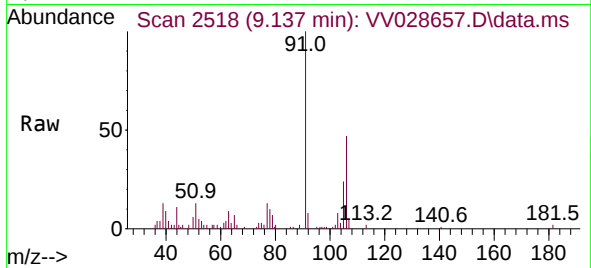

#54
o-Xylene
Concen: 0.627 ug/L
RT: 9.539 min Scan# 2643
Delta R.T. 0.007 min
Lab File: VV028657.D
Acq: 21 Oct 2022 13:05

Tgt Ion:106 Resp: 13434
Ion Ratio Lower Upper
106 100
91 220.9 159.0 295.4

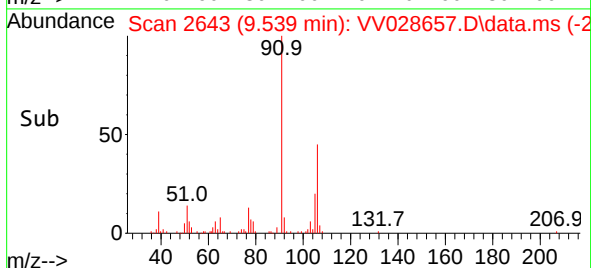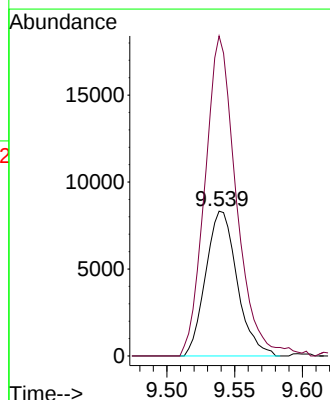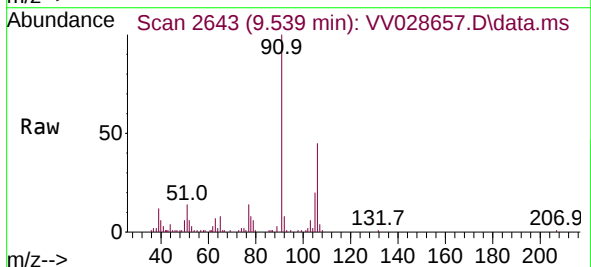

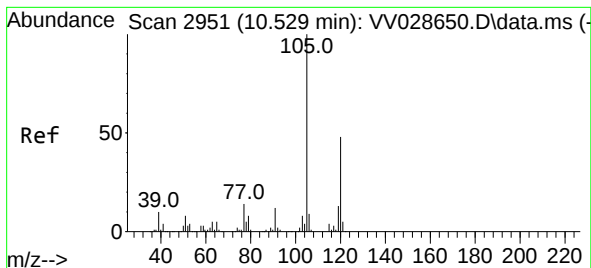

#62

1,3,5-Trimethylbenzene

Concen: 0.180 ug/L

RT: 10.532 min Scan# 2951

Delta R.T. 0.003 min

Lab File: VV028657.D

Acq: 21 Oct 2022 13:05

Instrument :

MSVOA_V

ClientSampleId :





BD716

Tgt Ion:105 Resp: 2828

Ion Ratio Lower Upper

105 100

120 50.5 38.3 57.5

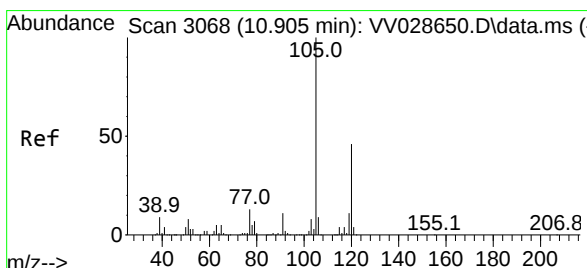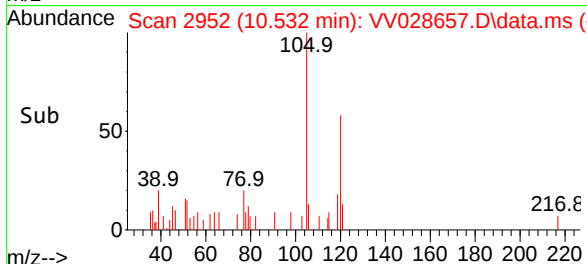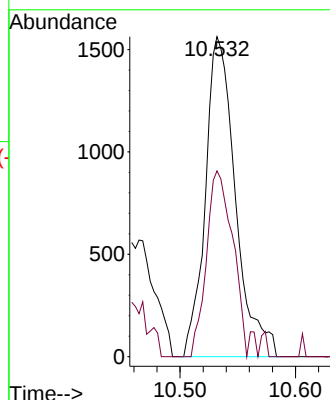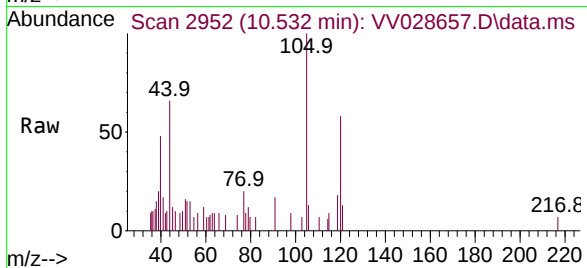

#63

1,2,4-Trimethylbenzene

Concen: 0.074 ug/L

RT: 10.911 min Scan# 3070

Delta R.T. 0.007 min

Lab File: VV028657.D

Acq: 21 Oct 2022 13:05

Tgt Ion:105 Resp: 3152

Ion Ratio Lower Upper

105 100

120 43.6 36.2 54.2

