

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028652.D
 Acq On : 21 Oct 2022 11:06
 Operator : SY/MD
 Sample : N5144-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	49	62	65	rBV	10243	19701	2.24%	0.337%
2	1.301	74	81	97	rVB	143024	150702	17.10%	2.578%
3	1.564	156	163	174	rBV	125891	138479	15.72%	2.369%
4	2.101	321	330	340	rVB	247666	344861	39.14%	5.901%
5	2.497	450	453	464	rVB2	17878	23146	2.63%	0.396%
6	3.963	889	909	924	rBV	67319	262456	29.79%	4.491%
7	4.339	1012	1026	1046	rVB	148521	367066	41.66%	6.280%
8	5.034	1228	1242	1263	rBV2	406215	881090	100.00%	15.075%
9	5.609	1409	1421	1439	rBV	289652	567776	64.44%	9.715%
10	6.066	1552	1563	1578	rVB	230777	441816	50.14%	7.559%
11	6.976	1835	1846	1857	rBV	81949	138936	15.77%	2.377%
12	7.301	1935	1947	1964	rBV	313204	540098	61.30%	9.241%
13	7.616	2035	2045	2057	rBV2	34303	55749	6.33%	0.954%
14	8.108	2187	2198	2232	rBV2	240091	517378	58.72%	8.852%
15	8.844	2415	2427	2446	rBV	278241	457175	51.89%	7.822%
16	10.210	2842	2852	2864	rBV	87056	134102	15.22%	2.294%
17	11.239	3162	3172	3189	rBV	259919	407543	46.25%	6.973%
18	11.615	3274	3289	3311	rBV	231920	375821	42.65%	6.430%
19	15.873	4597	4613	4614	rBV	10174	20680	2.35%	0.354%




Sum of corrected areas: 5844575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028652.D
Acq On : 21 Oct 2022 11:06
Operator : SY/MD
Sample : N5144-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

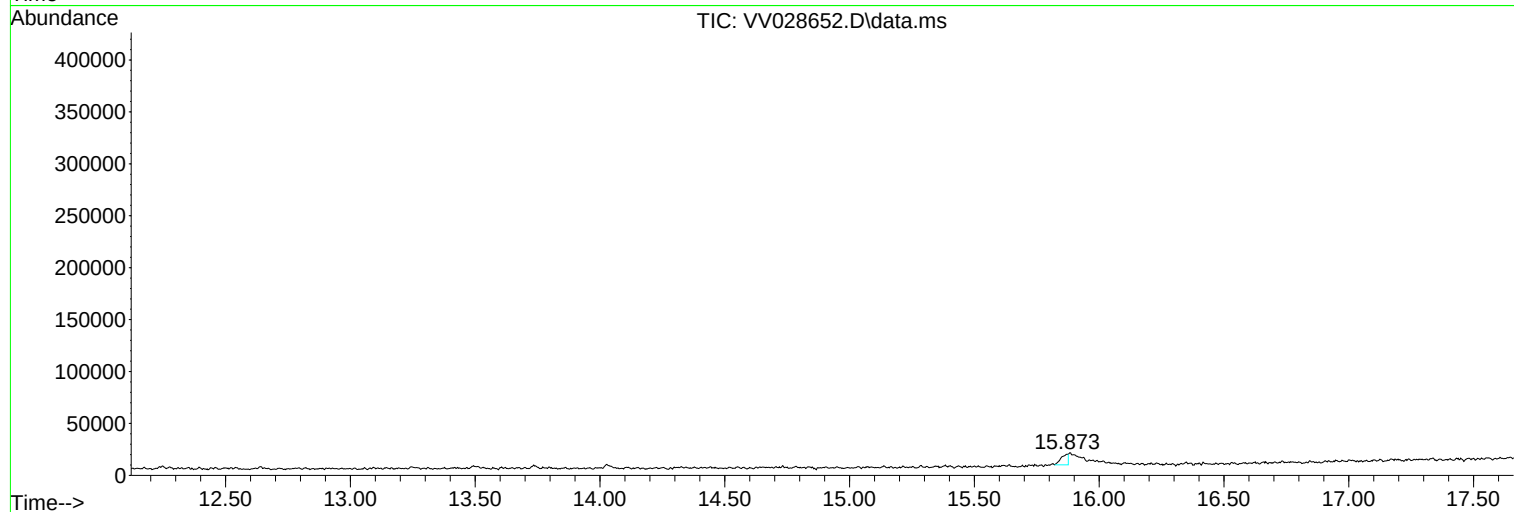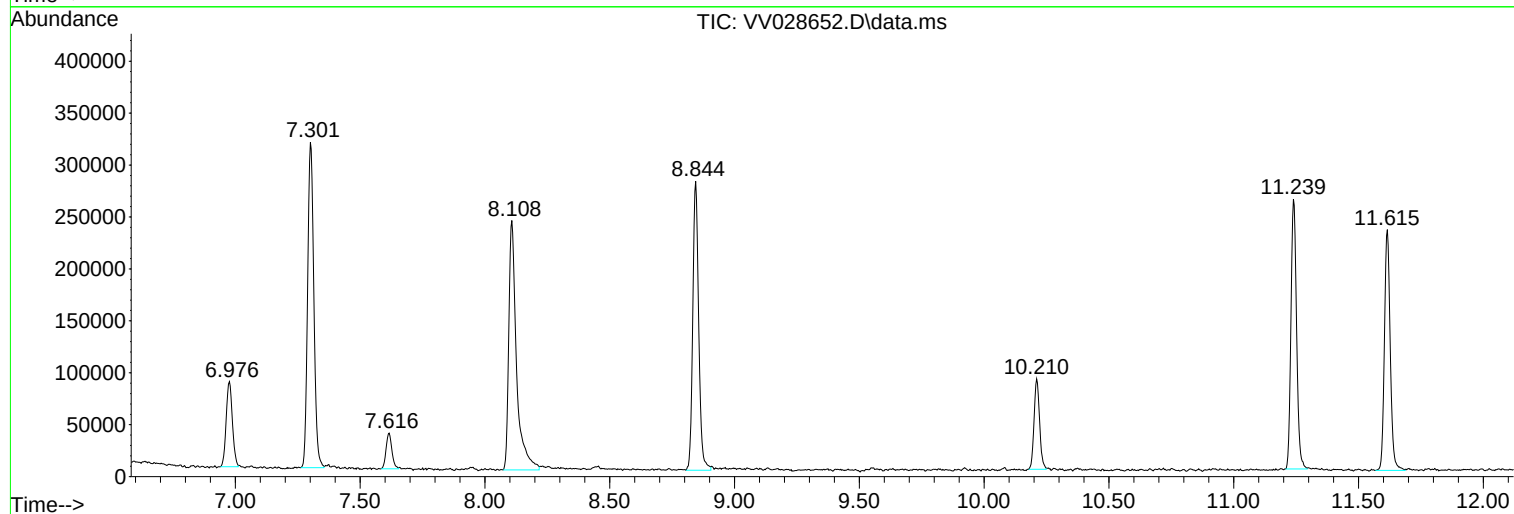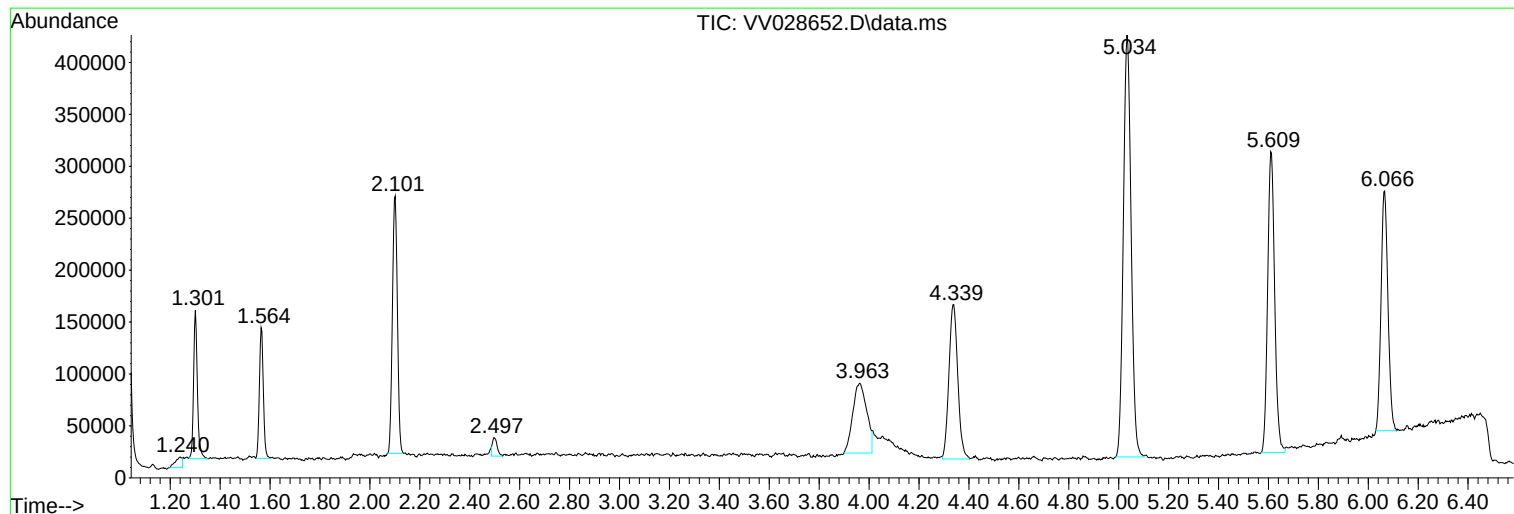

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028652.D
Acq On : 21 Oct 2022 11:06
Operator : SY/MD
Sample : N5144-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028652.D
Acq On : 21 Oct 2022 11:06
Operator : SY/MD
Sample : N5144-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc