

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028656.D
 Acq On : 21 Oct 2022 12:41
 Operator : SY/MD
 Sample : N5163-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD711

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	74	80	93	rVV	149157	154649	23.11%	2.940%
2	1.558	154	161	174	rVB	118474	138051	20.63%	2.624%
3	2.101	319	330	344	rVB	220802	319314	47.71%	6.070%
4	2.301	382	392	397	rBV5	6136	11536	1.72%	0.219%
5	3.928	883	898	901	rBV2	28290	66507	9.94%	1.264%
6	4.343	1013	1027	1045	rBV	108823	266831	39.87%	5.072%
7	5.040	1227	1244	1269	rBV2	267442	669315	100.00%	12.723%
8	5.613	1411	1422	1450	rBV	197236	409729	61.22%	7.789%
9	6.066	1545	1563	1586	rBV	156037	325206	48.59%	6.182%
10	6.982	1837	1848	1862	rBV2	56839	109095	16.30%	2.074%
11	7.310	1938	1950	1967	rBV	302176	540488	80.75%	10.274%
12	7.387	1968	1974	1985	rVB2	13580	27530	4.11%	0.523%
13	7.622	2038	2047	2060	rBV2	31280	57076	8.53%	1.085%
14	7.973	2147	2156	2170	rVB3	24788	42076	6.29%	0.800%
15	8.092	2182	2193	2225	rBV2	234152	563583	84.20%	10.713%
16	8.847	2415	2428	2448	rBV	307480	515606	77.03%	9.801%
17	9.140	2508	2519	2529	rBV3	10958	20235	3.02%	0.385%
18	9.538	2635	2643	2655	rBV3	5289	10688	1.60%	0.203%
19	10.210	2840	2852	2864	rBV	91225	150038	22.42%	2.852%
20	10.374	2894	2903	2912	rVB10	7206	11359	1.70%	0.216%
21	11.243	3161	3173	3194	rBV	278244	452680	67.63%	8.605%
22	11.616	3275	3289	3310	rBV	242332	398918	59.60%	7.583%




Sum of corrected areas: 5260510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028656.D
Acq On : 21 Oct 2022 12:41
Operator : SY/MD
Sample : N5163-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD711

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

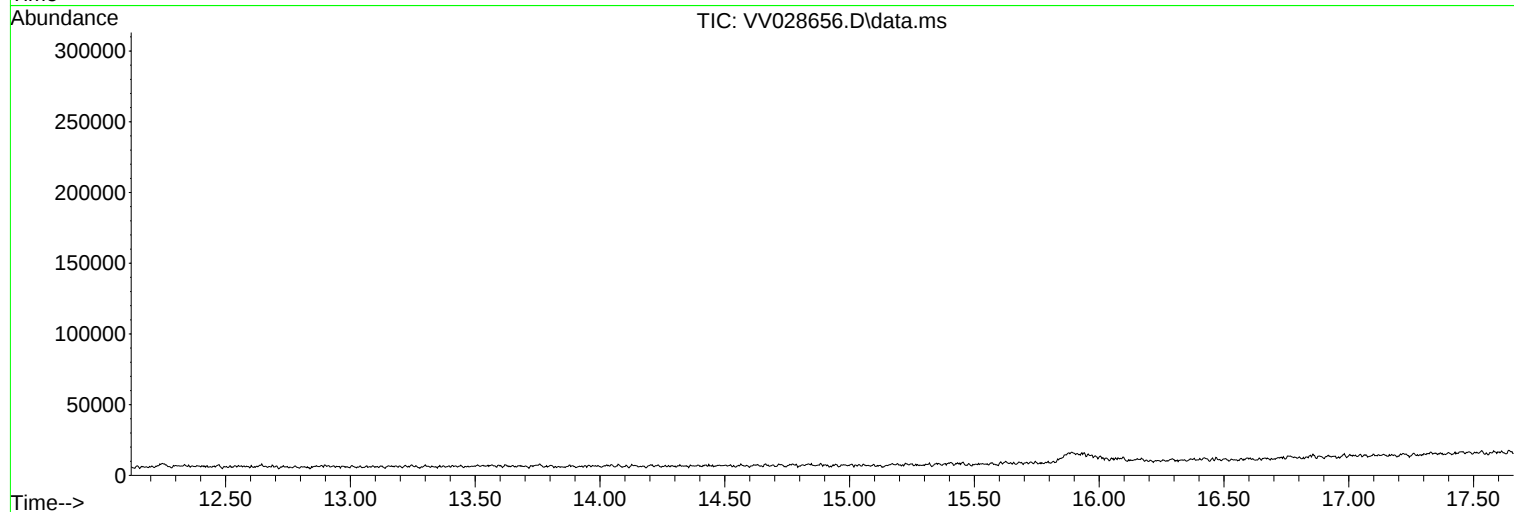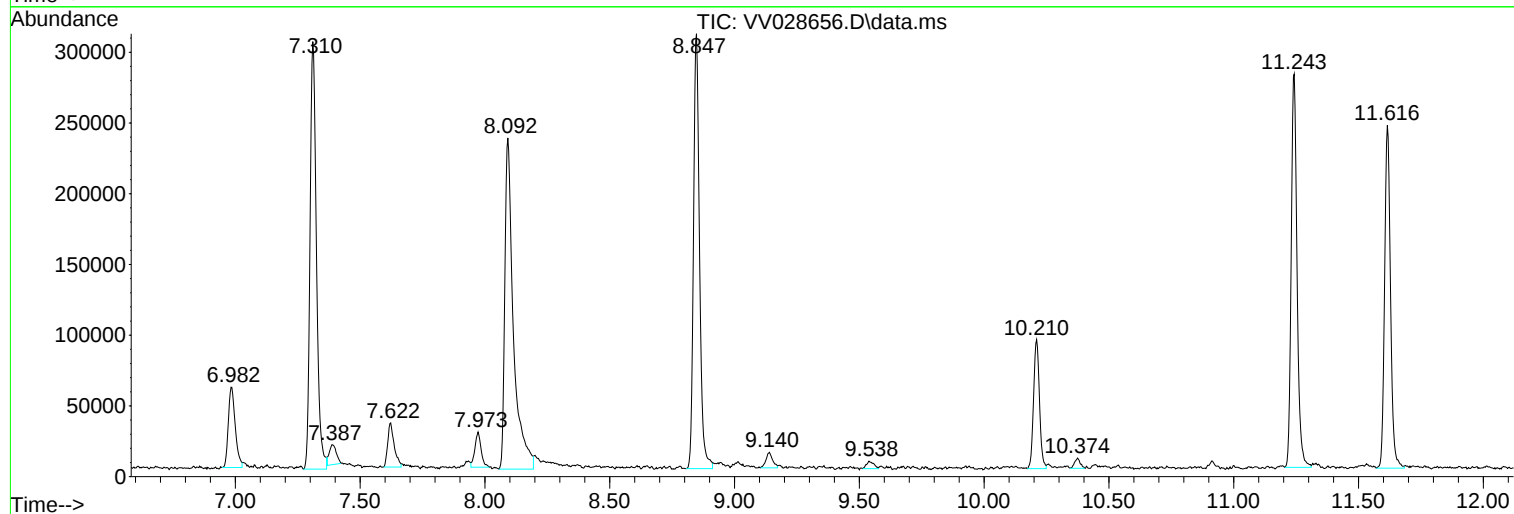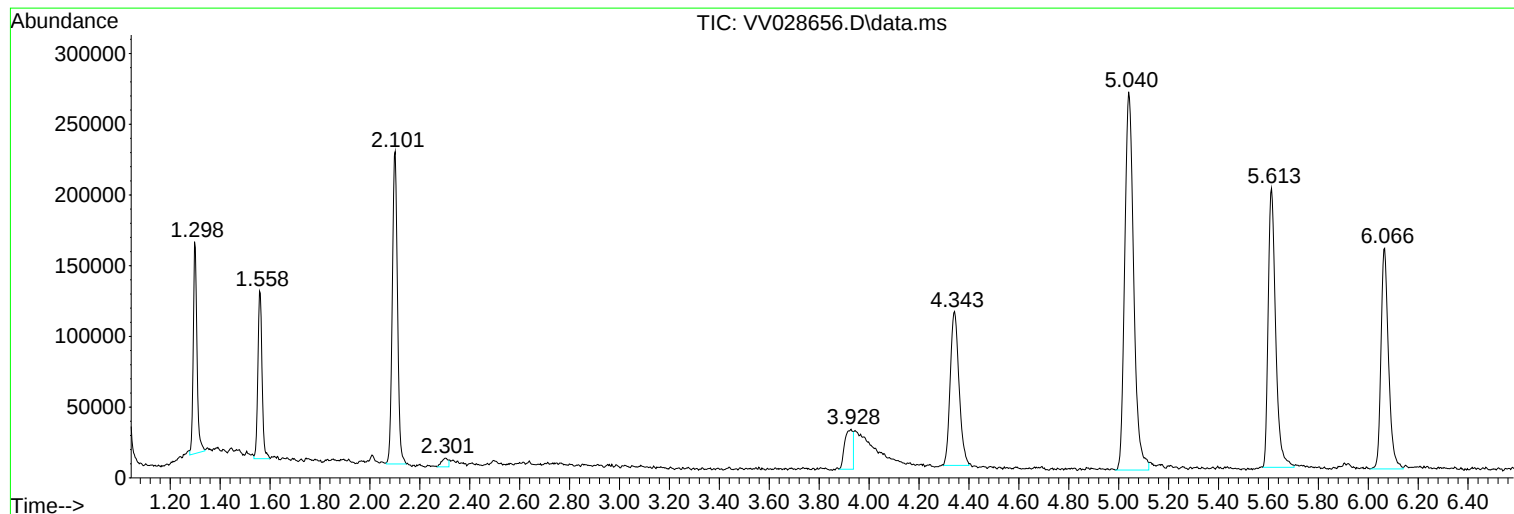

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028656.D
Acq On : 21 Oct 2022 12:41
Operator : SY/MD
Sample : N5163-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD711

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028656.D
Acq On : 21 Oct 2022 12:41
Operator : SY/MD
Sample : N5163-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD711

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc