

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028658.D
 Acq On : 21 Oct 2022 13:30
 Operator : SY/MD
 Sample : N5163-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD717

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	49	60	66	rBV3	25106	40044	4.31%	0.659%
2	1.297	74	80	94	rVB	139992	145338	15.65%	2.393%
3	1.564	155	163	172	rVB	122582	139290	15.00%	2.293%
4	2.098	320	329	343	rBV	245882	343300	36.97%	5.651%
5	3.950	891	905	933	rVB2	74677	281026	30.27%	4.626%
6	4.336	1011	1025	1046	rVB2	160943	427604	46.05%	7.039%
7	5.030	1227	1241	1266	rVB3	422065	928539	100.00%	15.285%
8	5.606	1409	1420	1437	rBV	265351	500294	53.88%	8.236%
9	6.059	1550	1561	1584	rBV2	235820	467135	50.31%	7.690%
10	6.972	1832	1845	1862	rBV	65927	120736	13.00%	1.988%
11	7.162	1893	1904	1913	rBV3	13317	24720	2.66%	0.407%
12	7.300	1929	1947	1961	rBV	299437	516113	55.58%	8.496%
13	7.374	1961	1970	1983	rVB	68729	119780	12.90%	1.972%
14	7.616	2034	2045	2059	rBV2	31036	55114	5.94%	0.907%
15	8.107	2185	2198	2225	rBV	252838	526176	56.67%	8.662%
16	8.844	2416	2427	2446	rBV	256036	424327	45.70%	6.985%
17	9.005	2468	2477	2487	rBV3	10442	16679	1.80%	0.275%
18	9.130	2506	2516	2530	rBV2	33823	60566	6.52%	0.997%
19	9.535	2633	2642	2652	rBV2	13559	24396	2.63%	0.402%
20	10.210	2840	2852	2865	rBV	91861	145002	15.62%	2.387%
21	10.371	2895	2902	2912	rVB4	8577	12493	1.35%	0.206%
22	11.239	3161	3172	3188	rBV	236594	377363	40.64%	6.212%
23	11.615	3277	3289	3305	rBV	237045	378624	40.78%	6.233%




Sum of corrected areas: 6074659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028658.D
Acq On : 21 Oct 2022 13:30
Operator : SY/MD
Sample : N5163-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD717

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

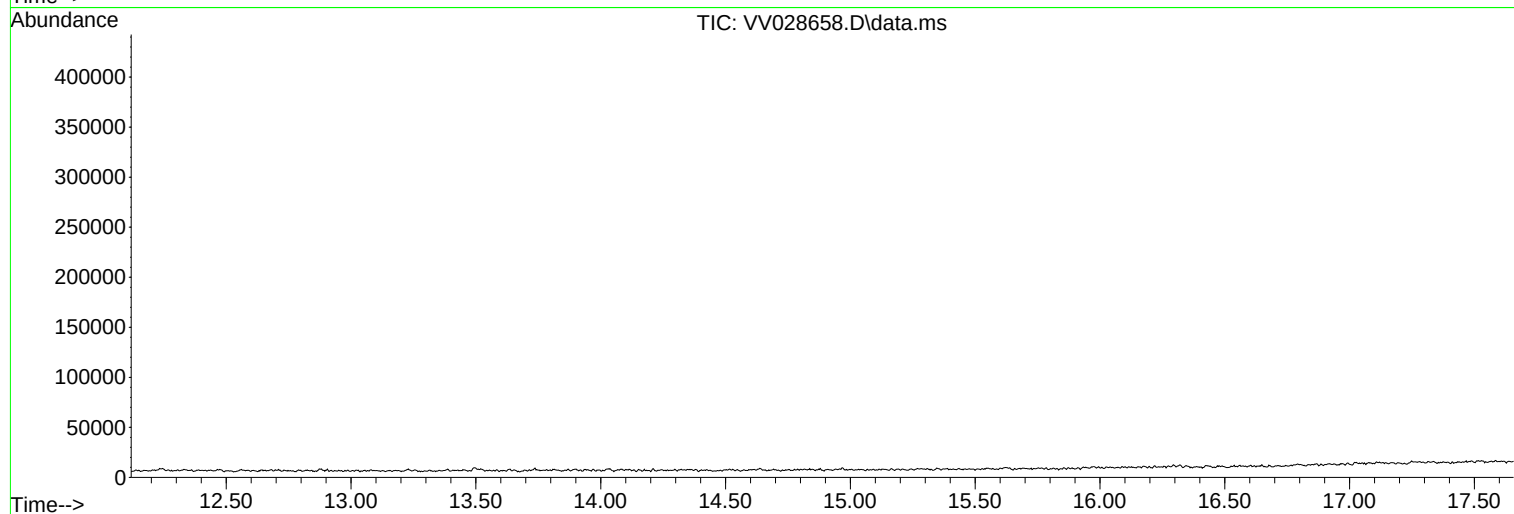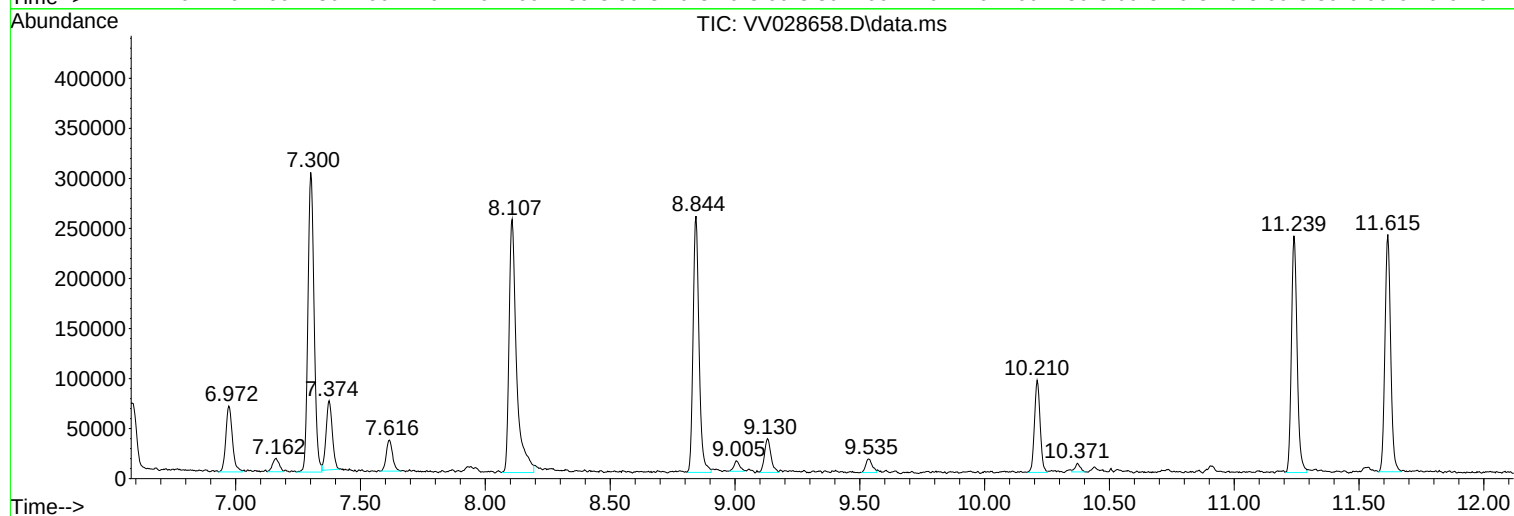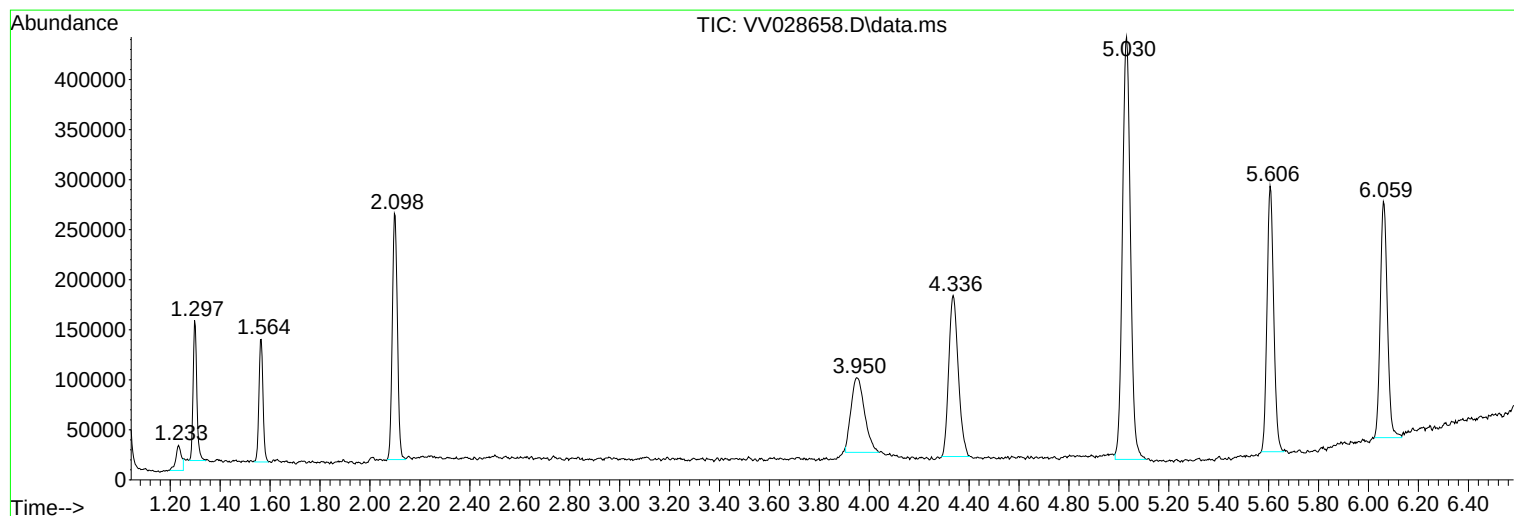

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028658.D
Acq On : 21 Oct 2022 13:30
Operator : SY/MD
Sample : N5163-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD717

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028658.D
Acq On : 21 Oct 2022 13:30
Operator : SY/MD
Sample : N5163-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD717

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc