

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028665.D
 Acq On : 21 Oct 2022 16:22
 Operator : SY/MD
 Sample : N5216-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	48	60	62	rBV10	10848	15858	1.66%	0.263%
2	1.298	73	80	95	rVB	130961	139572	14.58%	2.313%
3	1.561	155	162	178	rBV	117927	136544	14.26%	2.263%
4	2.101	318	330	341	rBV	233359	330591	34.54%	5.479%
5	3.953	890	906	927	rBV2	75028	266338	27.82%	4.414%
6	4.339	1011	1026	1052	rVB4	177123	543084	56.73%	9.001%
7	5.031	1227	1241	1263	rVB2	433588	957239	100.00%	15.865%
8	5.606	1409	1420	1434	rBV	264908	503437	52.59%	8.344%
9	6.063	1550	1562	1580	rBV	235316	470595	49.16%	7.800%
10	6.966	1832	1843	1855	rVB	80959	139469	14.57%	2.312%
11	7.294	1933	1945	1959	rBV	316713	535662	55.96%	8.878%
12	7.368	1961	1968	1977	rVB	12664	21274	2.22%	0.353%
13	7.609	2029	2043	2051	rBV3	34847	58663	6.13%	0.972%
14	8.104	2185	2197	2228	rBV2	263711	530832	55.45%	8.798%
15	8.243	2235	2240	2256	rVB2	8600	17432	1.82%	0.289%
16	8.841	2414	2426	2446	rBV	262480	428564	44.77%	7.103%
17	10.210	2842	2852	2865	rBV	90352	139373	14.56%	2.310%
18	11.239	3159	3172	3189	rBV	247428	388186	40.55%	6.434%
19	11.522	3251	3260	3271	rBV	6726	13134	1.37%	0.218%
20	11.615	3277	3289	3301	rBV	232483	373822	39.05%	6.196%
21	12.336	3503	3513	3525	rBV	12106	23858	2.49%	0.395%




Sum of corrected areas: 6033527

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028665.D
Acq On : 21 Oct 2022 16:22
Operator : SY/MD
Sample : N5216-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

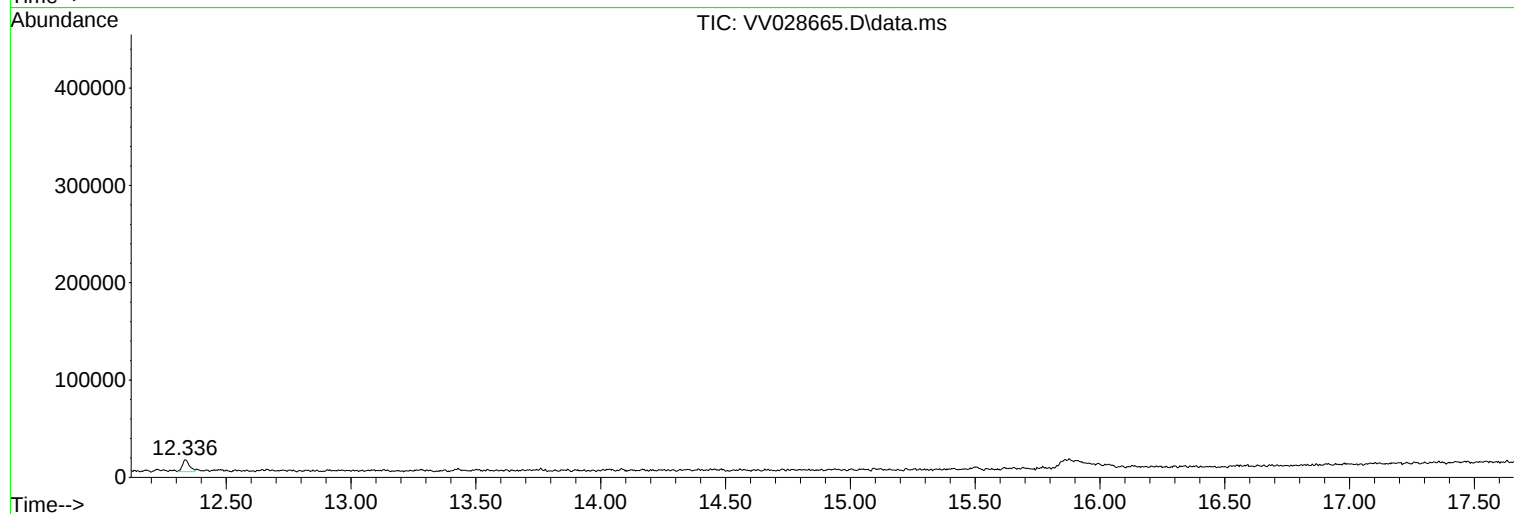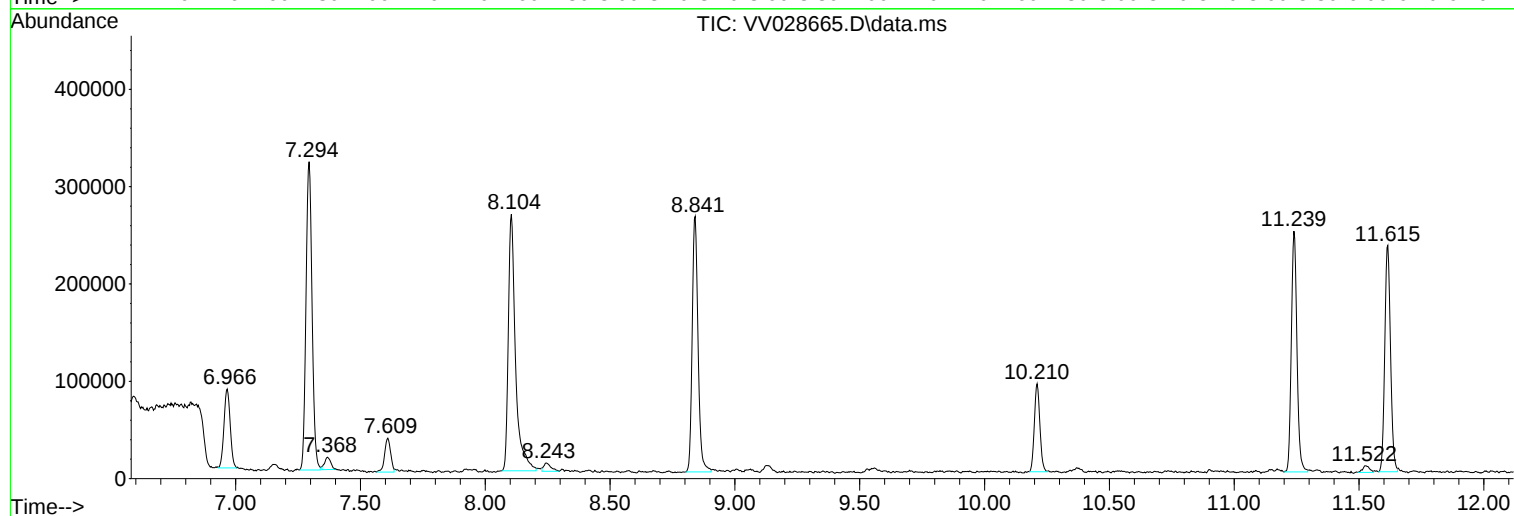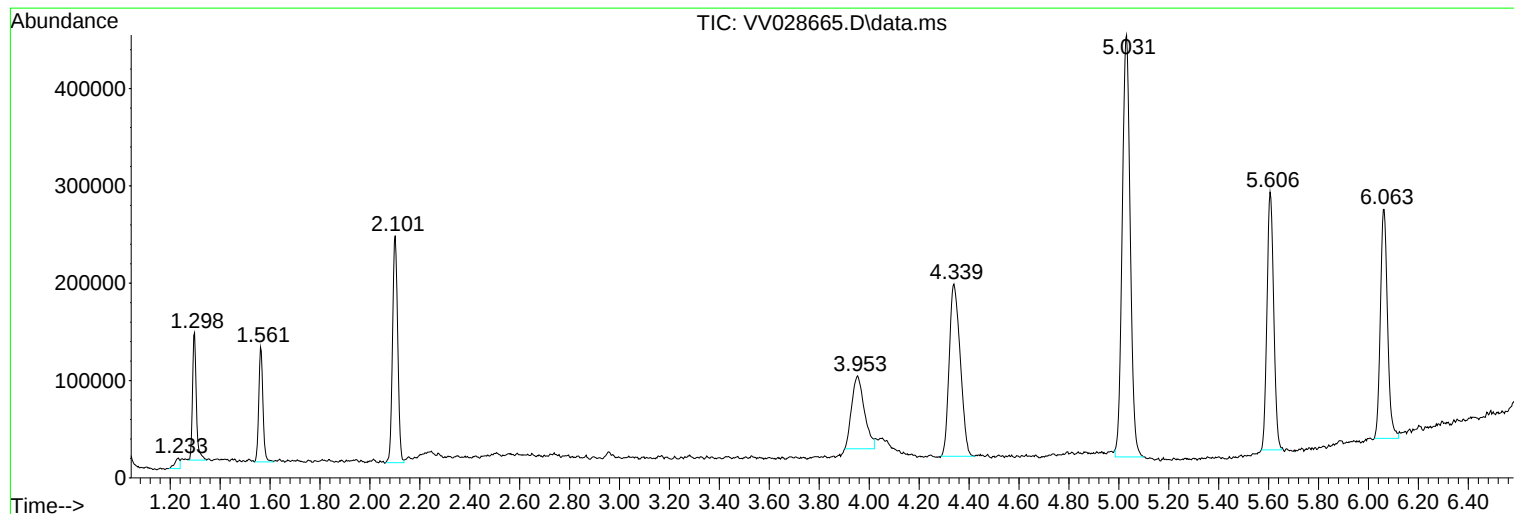

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028665.D
Acq On : 21 Oct 2022 16:22
Operator : SY/MD
Sample : N5216-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028665.D
Acq On : 21 Oct 2022 16:22
Operator : SY/MD
Sample : N5216-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
