

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028668.D
 Acq On : 21 Oct 2022 17:32
 Operator : SY/MD
 Sample : N5173-06DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXT1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028668.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	23	28	35	rBV	9845	11335	1.62%	0.171%
2	1.304	74	82	97	rBV	118409	126483	18.13%	1.905%
3	1.564	155	163	176	rBV	107543	123984	17.77%	1.867%
4	2.105	320	331	349	rVB	211131	313964	45.01%	4.728%
5	2.503	445	455	465	rBV2	18534	30235	4.33%	0.455%
6	3.908	880	892	916	rBV2	61799	210904	30.23%	3.176%
7	4.346	1013	1028	1046	rBV	111440	279412	40.05%	4.208%
8	5.043	1228	1245	1274	rBV2	273776	697598	100.00%	10.505%
9	5.616	1410	1423	1445	rBV	195345	410338	58.82%	6.179%
10	5.912	1500	1515	1533	rBV	335537	667529	95.69%	10.052%
11	6.066	1550	1563	1581	rBV	157057	321044	46.02%	4.835%
12	6.985	1838	1849	1864	rBV2	57742	114006	16.34%	1.717%
13	7.313	1940	1951	1967	rBV	300747	540628	77.50%	8.141%
14	7.622	2039	2047	2064	rBV2	31344	57214	8.20%	0.862%
15	7.969	2137	2155	2171	rBV	371661	636765	91.28%	9.589%
16	8.091	2184	2193	2228	rBV	221894	580177	83.17%	8.737%
17	8.847	2417	2428	2450	rBV	290610	502206	71.99%	7.563%
18	9.545	2637	2645	2654	rBV	4071	8151	1.17%	0.123%
19	10.210	2837	2852	2866	rBV	97396	157896	22.63%	2.378%
20	11.242	3161	3173	3192	rBV	276197	445115	63.81%	6.703%
21	11.615	3277	3289	3305	rBV	245247	405452	58.12%	6.106%




Sum of corrected areas: 6640436

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028668.D
Acq On : 21 Oct 2022 17:32
Operator : SY/MD
Sample : N5173-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXT1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

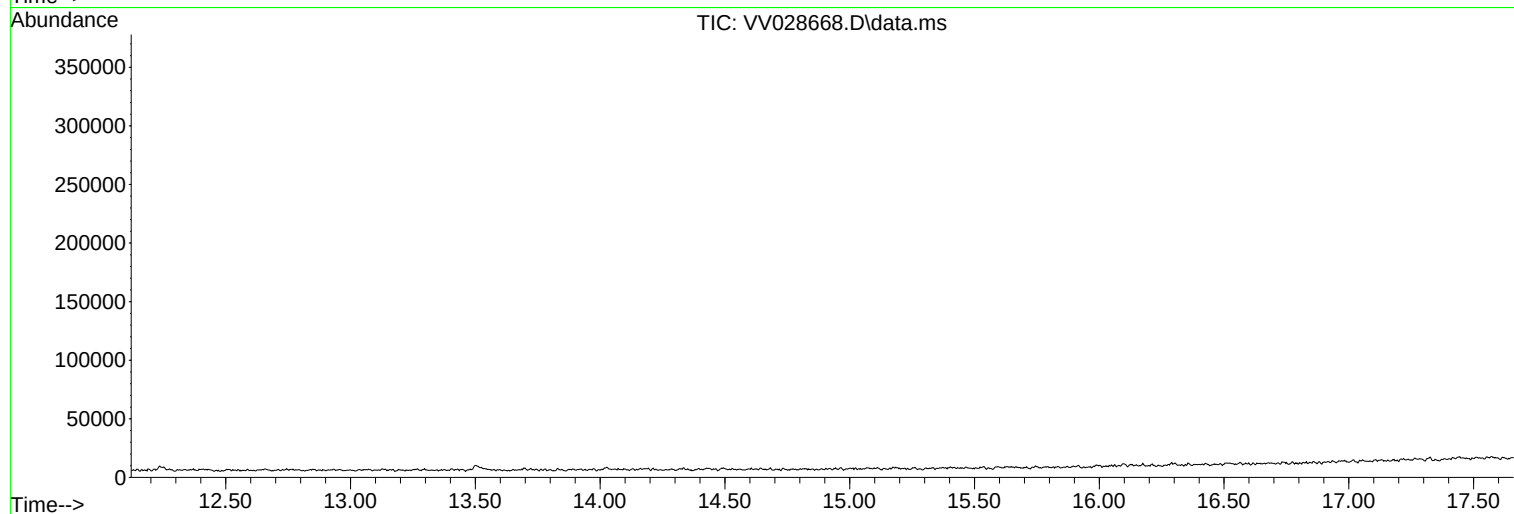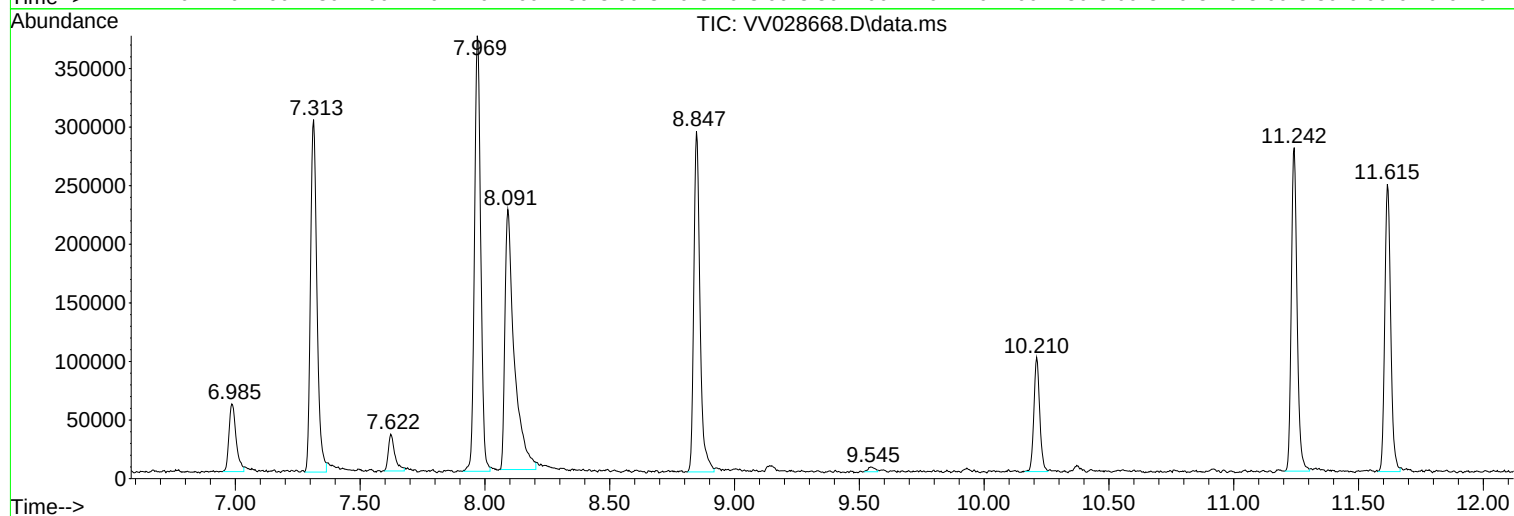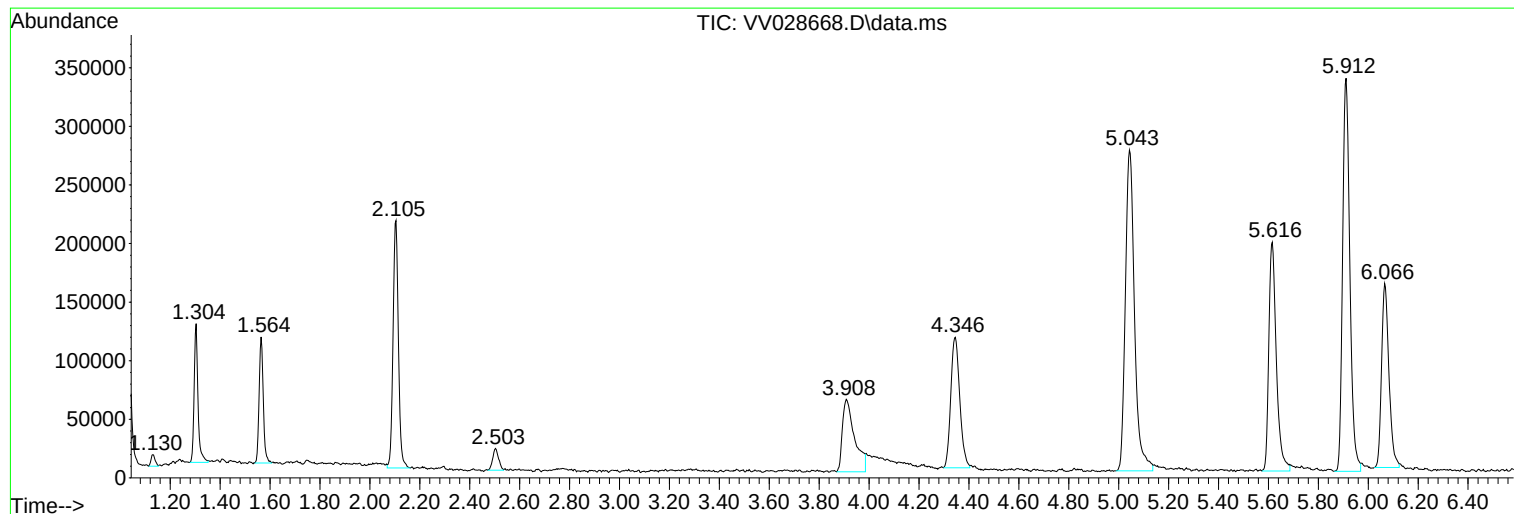

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028668.D
Acq On : 21 Oct 2022 17:32
Operator : SY/MD
Sample : N5173-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXT1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028668.D
Acq On : 21 Oct 2022 17:32
Operator : SY/MD
Sample : N5173-06DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXT1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
