

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028669.D
 Acq On : 21 Oct 2022 18:18
 Operator : SY/MD
 Sample : N5216-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA68

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	55	62	63	rBV6	8430	9889	1.36%	0.175%
2	1.294	73	79	93	rVB	147007	156916	21.56%	2.783%
3	1.558	153	161	170	rBV	123498	142292	19.55%	2.523%
4	2.095	319	328	339	rBV	244987	339850	46.69%	6.027%
5	3.963	888	909	942	rVB2	65354	334355	45.94%	5.929%
6	4.333	1007	1024	1047	rVB	118899	285534	39.23%	5.063%
7	5.034	1224	1242	1272	rBV2	311460	727887	100.00%	12.908%
8	5.609	1409	1421	1440	rBV	187235	382972	52.61%	6.791%
9	6.063	1548	1562	1589	rVB	168516	345485	47.46%	6.127%
10	6.982	1838	1848	1867	rBV	61556	120642	16.57%	2.139%
11	7.307	1937	1949	1968	rBV	316040	558879	76.78%	9.911%
12	7.619	2037	2046	2064	rBV3	32583	60081	8.25%	1.065%
13	7.937	2135	2145	2157	rBV3	10482	22955	3.15%	0.407%
14	8.098	2185	2195	2224	rBV	281395	606301	83.30%	10.752%
15	8.844	2416	2427	2445	rBV	281110	472039	64.85%	8.371%
16	10.210	2839	2852	2866	rBV	101346	164178	22.56%	2.911%
17	10.374	2891	2903	2914	rBV	16452	26540	3.65%	0.471%
18	11.239	3161	3172	3186	rBV	261880	417081	57.30%	7.396%
19	11.615	3278	3289	3306	rBV	262493	422505	58.05%	7.492%
20	12.638	3600	3607	3616	rBV	5178	9257	1.27%	0.164%
21	13.259	3792	3800	3807	rVB	6222	8118	1.12%	0.144%
22	13.496	3864	3874	3883	rBV3	8317	15073	2.07%	0.267%
23	13.738	3938	3949	3957	rBV3	6431	10273	1.41%	0.182%




Sum of corrected areas: 5639102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028669.D
Acq On : 21 Oct 2022 18:18
Operator : SY/MD
Sample : N5216-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

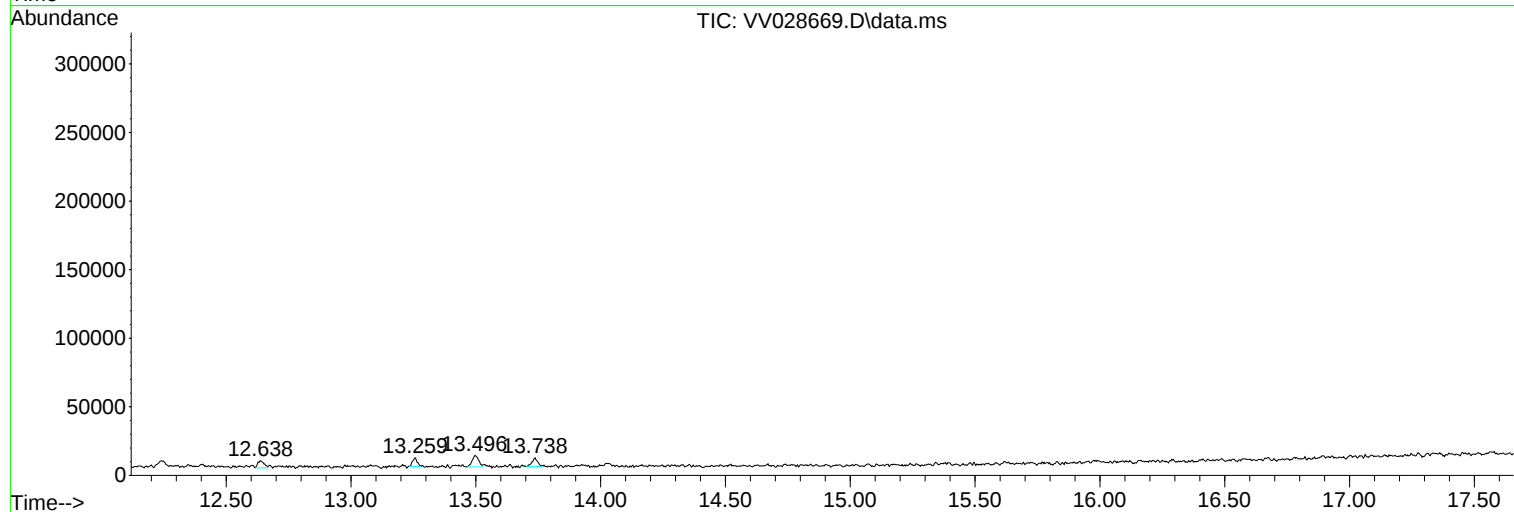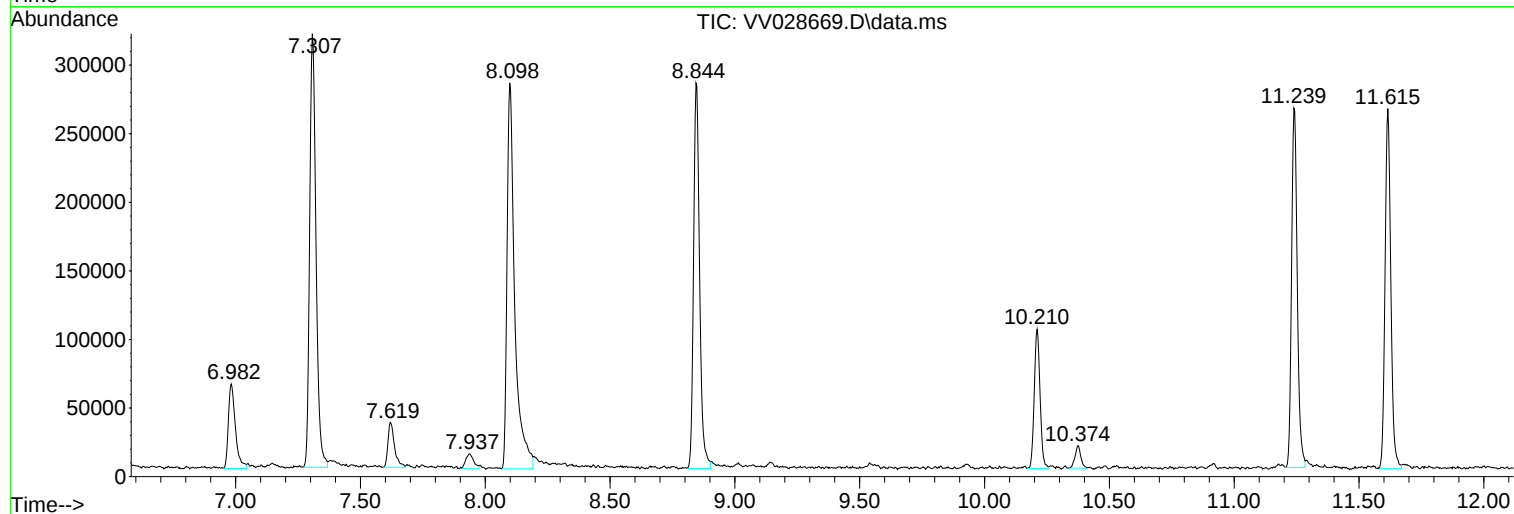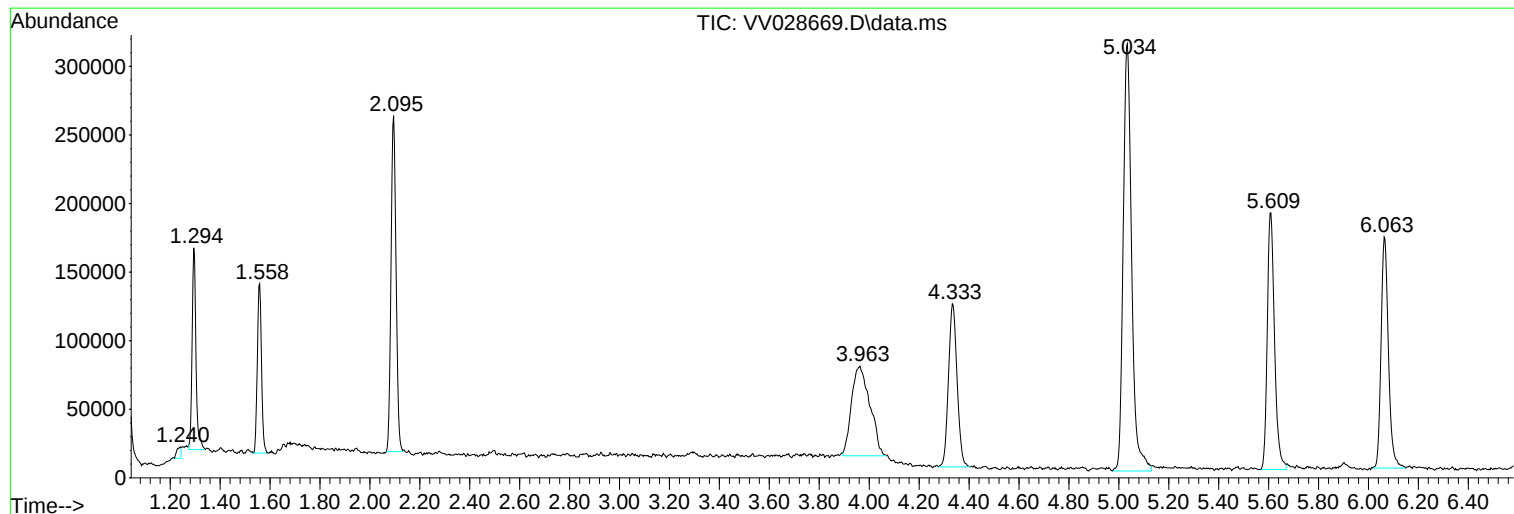

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028669.D
Acq On : 21 Oct 2022 18:18
Operator : SY/MD
Sample : N5216-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028669.D
Acq On : 21 Oct 2022 18:18
Operator : SY/MD
Sample : N5216-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc