

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028675.D
 Acq On : 21 Oct 2022 20:44
 Operator : SY/MD
 Sample : N5233-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA54

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rBV	118641	122131	17.03%	2.113%
2	1.465	125	132	142	rBV2	22221	29232	4.08%	0.506%
3	1.564	156	163	175	rBV	113610	132605	18.49%	2.294%
4	2.105	322	331	347	rVB	226667	340894	47.53%	5.897%
5	2.204	353	362	374	rVB2	31167	53438	7.45%	0.924%
6	2.291	383	389	400	rVB	7337	9567	1.33%	0.166%
7	2.500	449	454	462	rBV6	5549	7987	1.11%	0.138%
8	3.905	879	891	914	rBV2	39462	145900	20.34%	2.524%
9	4.349	1014	1029	1053	rVB3	142890	478632	66.73%	8.280%
10	5.043	1228	1245	1273	rBV2	285547	717233	100.00%	12.408%
11	5.616	1412	1423	1443	rBV	203931	424994	59.25%	7.352%
12	6.066	1549	1563	1589	rBV	165982	353007	49.22%	6.107%
13	6.985	1838	1849	1868	rBV	62861	124312	17.33%	2.151%
14	7.313	1938	1951	1970	rBV	317864	573270	79.93%	9.918%
15	7.622	2038	2047	2065	rBV2	32184	58472	8.15%	1.012%
16	8.091	2182	2193	2230	rBV	225365	614114	85.62%	10.624%
17	8.847	2413	2428	2451	rBV	307032	534375	74.51%	9.245%
18	10.210	2841	2852	2868	rBV2	97945	164003	22.87%	2.837%
19	11.243	3162	3173	3191	rBV	291385	464194	64.72%	8.031%
20	11.615	3279	3289	3306	rBV	265151	431995	60.23%	7.474%




Sum of corrected areas: 5780355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028675.D
Acq On : 21 Oct 2022 20:44
Operator : SY/MD
Sample : N5233-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

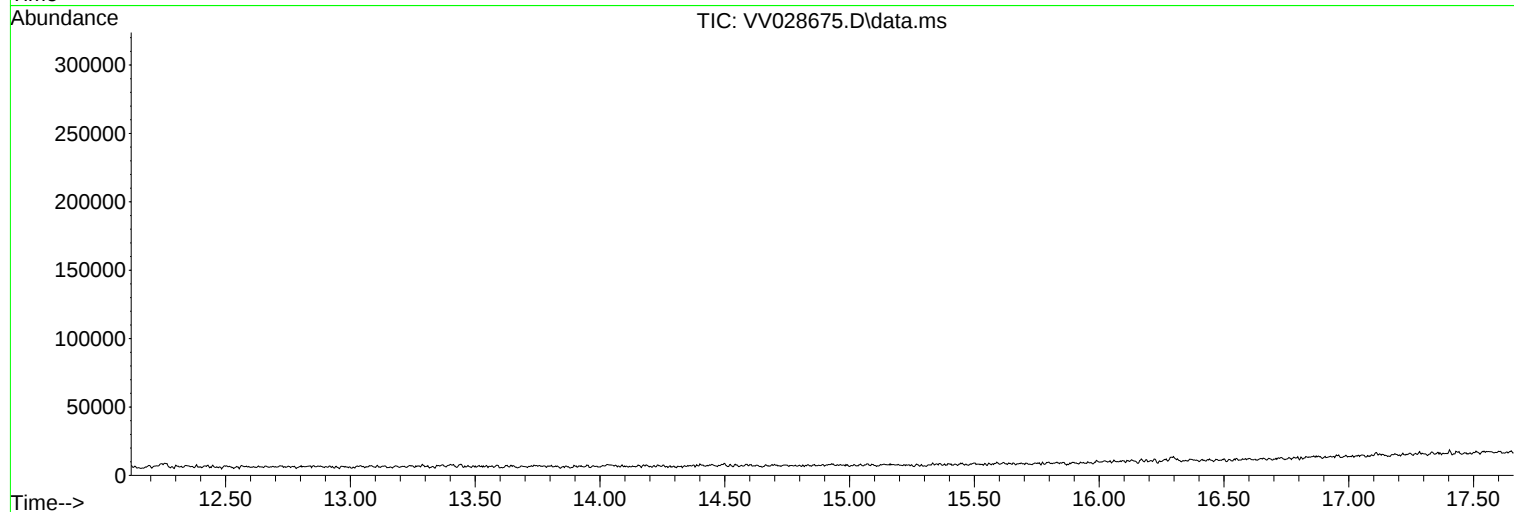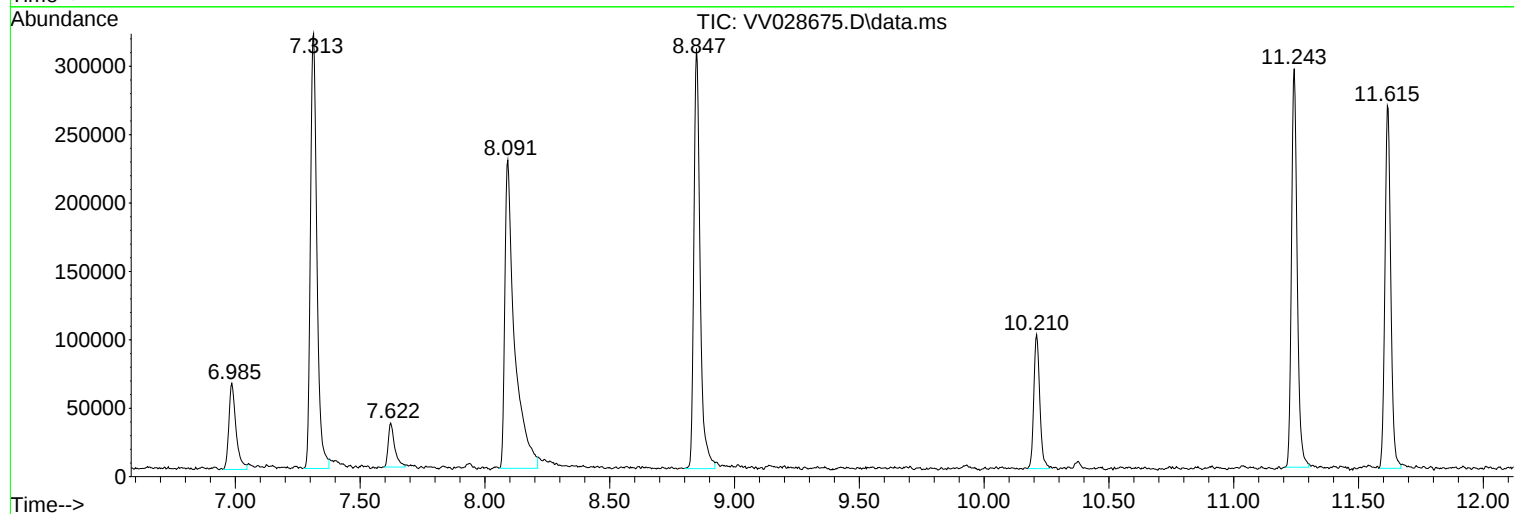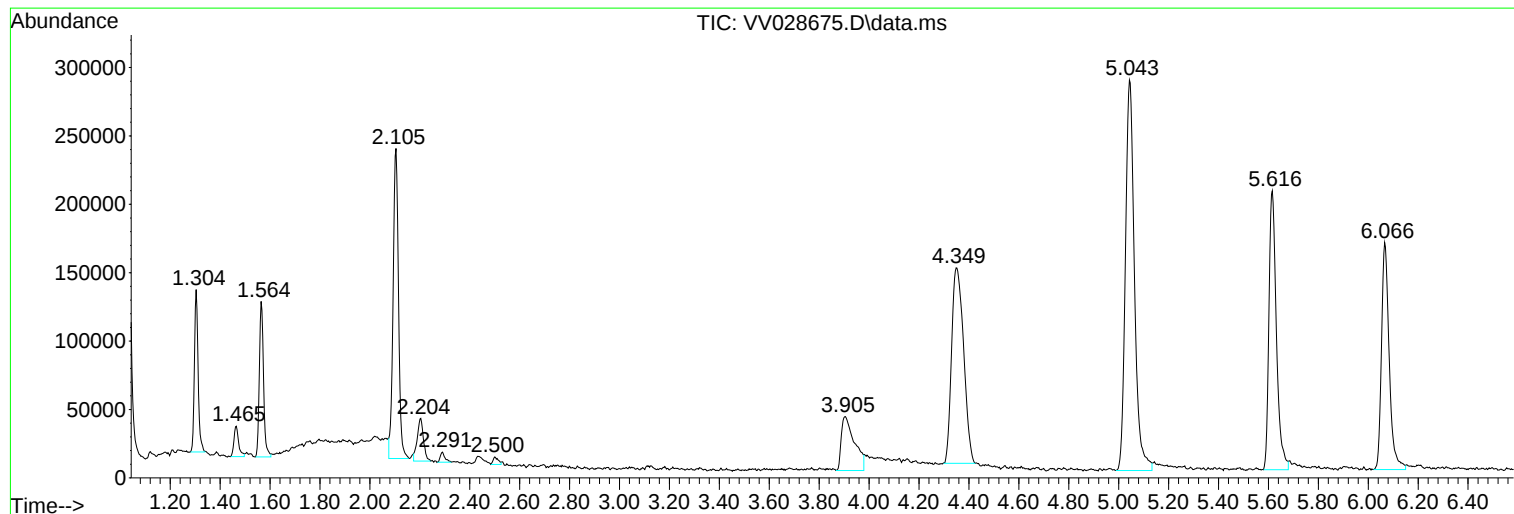

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028675.D
Acq On : 21 Oct 2022 20:44
Operator : SY/MD
Sample : N5233-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
Data File : VV028675.D
Acq On : 21 Oct 2022 20:44
Operator : SY/MD
Sample : N5233-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc