
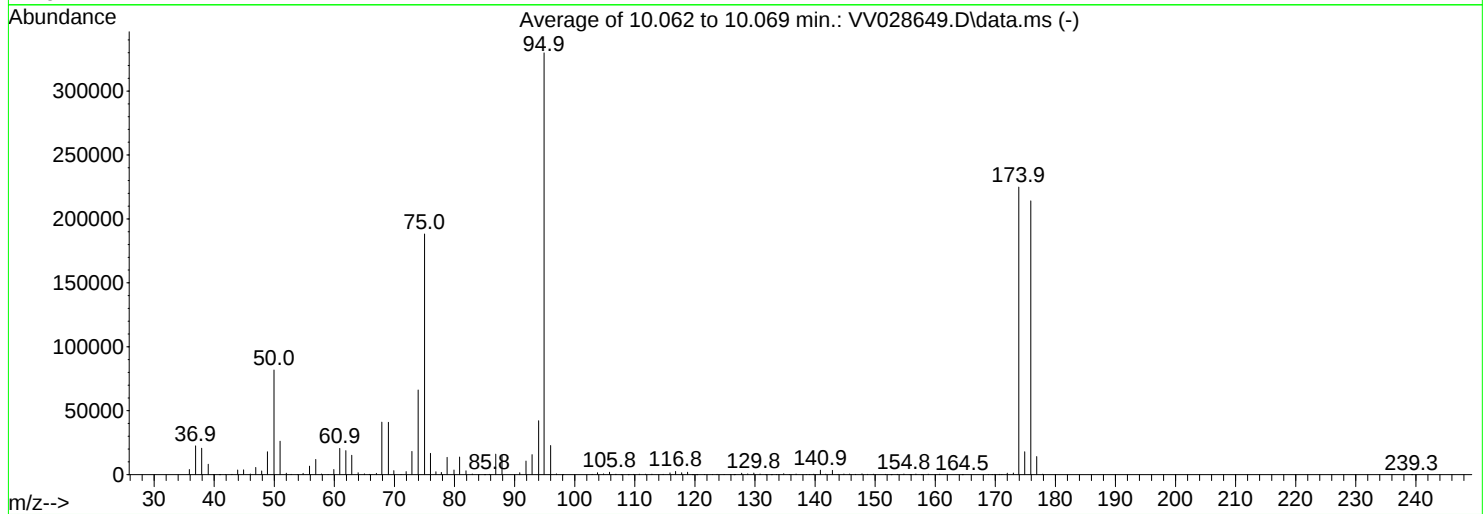


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102122\
 Data File : VV028649.D
 Acq On : 21 Oct 2022 09:36
 Operator : SY/MD
 Sample : BFB388
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB388

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102022WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Oct 26 09:07:13 2022

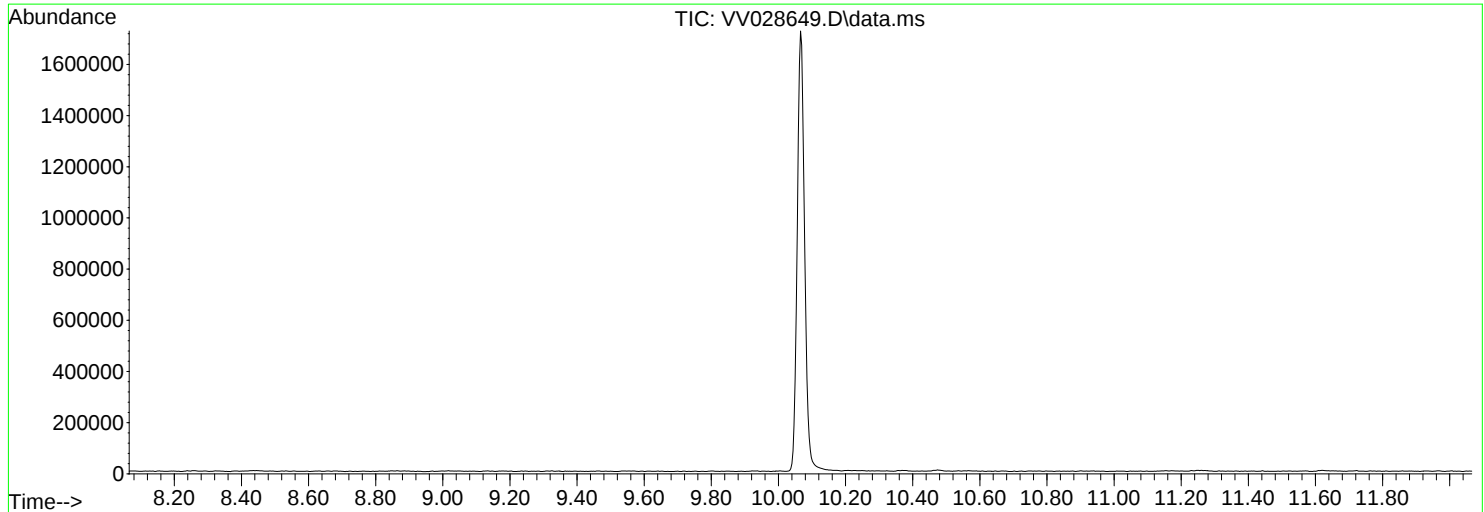

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	81824	PASS
75	95	30	80	57.1	188245	PASS
95	95	100	100	100.0	329899	PASS
96	95	5	9	6.9	22752	PASS
173	174	0.00	2	0.6	1313	PASS
174	95	50	120	68.2	224875	PASS
175	174	5	9	8.0	17909	PASS
176	174	95	105	95.2	214187	PASS
177	176	5	10	6.6	14140	PASS

m/z	Abundance
35.80	266.0
37.60	260.0
39.10	253.0
39.80	1015.0
40.90	312.0
41.80	168.0
43.00	259.0
43.90	2520.0
44.90	256.0
45.70	117.0
47.00	108.0
48.80	114.0
50.90	158.0
52.00	119.0
52.80	210.0
53.90	131.0
54.80	258.0
55.80	143.0
56.20	111.0
56.60	106.0
57.20	135.0
57.70	123.0
59.30	118.0
61.00	109.0
61.90	161.0
62.90	103.0
63.50	114.0
65.10	112.0
66.10	128.0
66.80	130.0
69.90	114.0
71.30	139.0
73.90	102.0
76.00	114.0
76.90	265.0
77.80	216.0
78.60	131.0
83.90	123.0
86.70	102.0
110.10	101.0
114.70	101.0
152.60	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
35.90	4387.0
36.90	21968.0
37.90	19784.0
39.00	8273.0
39.90	1109.0
40.90	281.0
42.00	289.0
42.90	439.0
43.90	6124.0
44.90	4048.0
46.00	497.0
46.90	5428.0
47.90	2835.0
48.90	17432.0
50.00	79632.0
51.00	25704.0
52.00	1238.0
52.80	316.0
53.90	246.0
54.80	1193.0
55.90	6559.0
56.90	11945.0
57.90	631.0
58.90	143.0
59.90	3994.0
60.90	19864.0
61.90	18584.0
63.00	14799.0
63.90	1547.0
65.00	739.0
65.80	225.0
67.00	1052.0
67.90	40624.0
69.00	39760.0
70.00	3187.0
71.00	305.0
72.00	2186.0
72.90	17696.0
74.00	64152.0
75.00	182976.0
76.00	16696.0
76.90	2390.0
77.90	1627.0
78.80	13462.0
79.90	3424.0
80.80	13120.0
81.90	2860.0
83.00	422.0
84.20	115.0
85.00	104.0
85.80	419.0
86.90	15685.0
87.90	14058.0
90.80	1424.0
91.90	10343.0
92.90	15178.0
94.00	40880.0
94.90	317760.0
96.00	22632.0
97.00	630.0
102.90	195.0
103.80	1600.0
104.80	546.0
105.80	1694.0
106.90	356.0
108.90	117.0
109.80	272.0
110.80	360.0
111.80	346.0
112.80	440.0
114.70	343.0
115.90	1320.0
116.80	2325.0
117.80	1434.0
118.80	1828.0
119.60	106.0
121.60	115.0
122.90	106.0
123.70	187.0
124.90	197.0
125.90	153.0
126.80	144.0
127.80	1144.0
128.80	613.0
129.80	1155.0
130.90	456.0
132.70	110.0
133.60	147.0
134.00	152.0
134.80	688.0
135.70	149.0
136.80	574.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

138.60	110.0
139.00	111.0
139.80	338.0
140.90	3298.0
141.80	377.0
142.90	3333.0
143.80	252.0
144.80	445.0
145.80	443.0
146.80	294.0
147.80	606.0
148.80	300.0
149.70	343.0
151.70	210.0
152.80	254.0
153.70	208.0
154.80	487.0
155.80	115.0
156.80	573.0
158.80	306.0
160.80	431.0
164.50	120.0
168.90	136.0
169.90	151.0
170.70	353.0
172.00	1056.0
173.90	210176.0
174.90	17336.0
175.90	200448.0
176.90	13433.0
177.90	383.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
35.90	4484.0
36.90	23536.0
37.90	21520.0
39.00	8633.0
39.90	1065.0
41.00	363.0
42.00	303.0
43.00	455.0
43.90	6266.0
44.90	4146.0
46.00	541.0
46.90	5824.0
47.90	2937.0
48.90	18720.0
49.90	84760.0
51.00	27408.0
52.00	1229.0
52.80	434.0
53.90	199.0
54.90	1250.0
55.90	6928.0
56.90	12338.0
57.90	720.0
59.00	118.0
59.90	4289.0
60.90	21464.0
61.90	19608.0
62.90	15898.0
64.00	1597.0
65.00	838.0
65.80	226.0
67.00	1072.0
67.90	42608.0
69.00	42640.0
69.90	3332.0
71.10	323.0
71.90	2460.0
72.90	18776.0
74.00	69008.0
75.00	194880.0
76.00	17424.0
76.90	2661.0
77.90	2036.0
78.80	14179.0
79.90	3761.0
80.80	14339.0
81.90	3108.0
83.00	481.0
83.80	108.0
84.10	103.0
86.90	16728.0
87.90	15698.0
90.80	1587.0
91.90	11068.0
92.90	16117.0
94.00	43680.0
94.90	342848.0
96.00	23336.0
96.90	715.0
102.90	205.0
103.80	1614.0
104.80	677.0
105.80	1922.0
106.90	400.0
108.90	104.0
109.80	278.0
110.70	359.0
111.80	437.0
112.80	432.0
114.70	391.0
115.90	1396.0
116.80	2603.0
117.80	1530.0
118.80	1991.0
120.30	110.0
121.60	123.0
123.00	132.0
123.70	230.0
124.90	197.0
125.90	179.0
126.70	148.0
127.80	1142.0
128.80	644.0
129.80	1278.0
130.90	480.0
132.80	105.0
133.60	154.0
134.00	147.0
134.80	744.0
135.80	177.0
136.80	562.0
138.60	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

139.10	136.0
139.80	353.0
140.90	3643.0
141.80	477.0
142.90	3550.0
143.90	289.0
144.80	478.0
145.80	501.0
146.80	331.0
147.80	678.0
148.80	324.0
149.70	377.0
151.70	214.0
152.80	203.0
153.70	242.0
154.80	566.0
156.00	132.0
156.80	562.0
157.70	110.0
158.90	430.0
160.80	423.0
168.90	116.0
169.50	161.0
170.00	211.0
170.70	304.0
172.00	1196.0
173.90	233600.0
174.90	18736.0
175.90	222720.0
176.90	14602.0
177.90	450.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
35.90	3996.0
36.90	22136.0
37.90	20736.0
39.00	8093.0
39.90	1053.0
41.00	412.0
42.00	305.0
43.00	490.0
43.90	5942.0
44.90	3869.0
46.00	555.0
46.90	5859.0
47.90	2794.0
48.90	17936.0
49.90	81080.0
51.00	25672.0
52.00	1191.0
52.80	483.0
53.80	154.0
54.00	153.0
54.90	1286.0
55.90	6690.0
56.90	11302.0
57.90	701.0
59.00	125.0
59.90	3946.0
60.90	20648.0
61.90	18824.0
62.90	15208.0
64.00	1482.0
65.00	847.0
65.90	224.0
67.00	1034.0
67.90	39920.0
69.00	40384.0
69.90	3308.0
71.00	295.0
71.90	2376.0
72.90	17824.0
74.00	65824.0
75.00	186880.0
76.00	16059.0
76.90	2652.0
77.80	2135.0
78.80	13459.0
79.90	3667.0
80.90	13842.0
81.90	2929.0
82.90	489.0
84.00	111.0
85.80	390.0
86.90	15839.0
87.90	15589.0
90.90	1670.0
91.90	10672.0
92.90	15760.0
94.00	41880.0
94.90	329088.0
96.00	22288.0
97.00	737.0
98.00	109.0
102.90	193.0
103.80	1433.0
104.80	712.0
105.80	1890.0
106.80	378.0
107.70	102.0
109.80	322.0
110.80	384.0
111.80	468.0
112.90	421.0
114.80	398.0
115.80	1316.0
116.80	2710.0
117.80	1422.0
118.80	1892.0
120.30	105.0
121.60	129.0
122.90	156.0
123.70	221.0
124.80	180.0
125.90	194.0
126.50	109.0
127.80	1068.0
128.80	588.0
129.80	1226.0
130.80	437.0
131.80	132.0
133.60	125.0
134.00	109.0
134.80	698.0
135.80	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

136.90	578.0
138.50	113.0
139.10	165.0
139.80	334.0
140.90	3582.0
141.80	458.0
142.90	3287.0
143.80	279.0
144.80	443.0
145.70	463.0
146.70	281.0
147.80	695.0
148.70	330.0
149.70	363.0
151.70	210.0
152.70	173.0
153.70	213.0
154.80	610.0
156.00	146.0
156.80	518.0
157.70	120.0
158.90	486.0
160.70	432.0
168.80	105.0
169.50	158.0
170.00	249.0
170.60	286.0
171.10	345.0
172.00	1169.0
173.00	3938.0
173.90	230848.0
174.90	17656.0
175.90	219392.0
176.90	14384.0
177.90	460.0
239.30	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388