




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028818.D
 Acq On : 01 Nov 2022 16:27
 Operator : SY/MD
 Sample : N5321-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN6DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/03/2022
 Supervised By :Mahesh Dadoda 11/03/2022

Quant Time: Nov 02 05:13:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 02 05:10:28 2022
 Response via : Initial Calibration

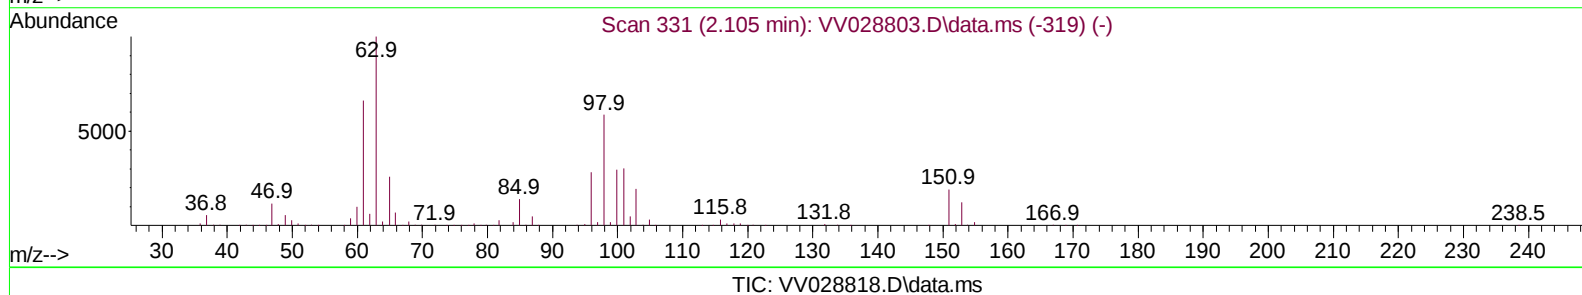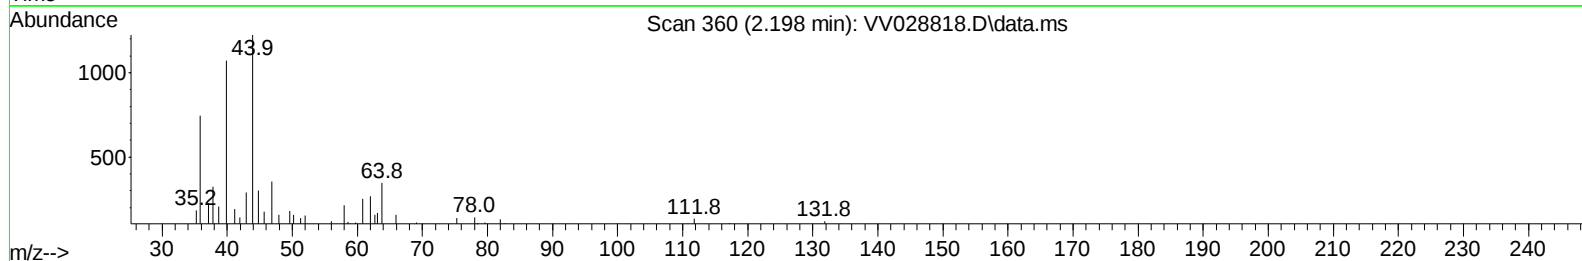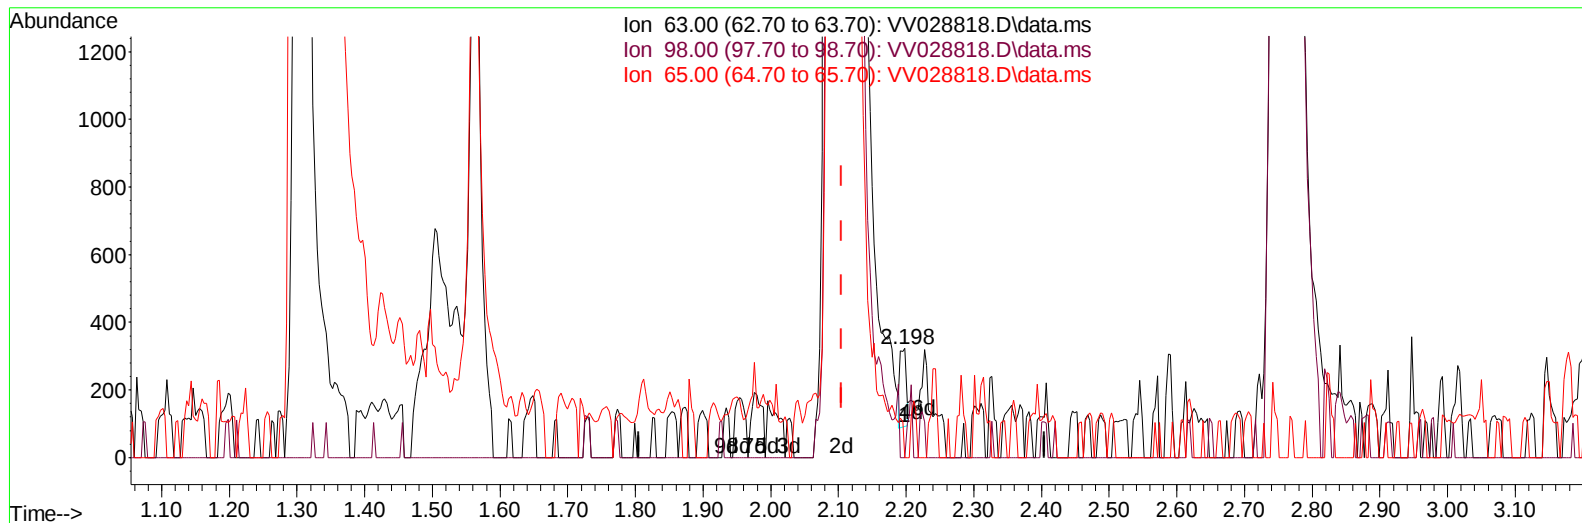

(11) 1,1-Dichloroethene-d2 (S)

2.198min (+ 0.093) 0.02 ug/L

response 145

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	62.00	45.52
65.00	23.30	17.93
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028818.D
 Acq On : 01 Nov 2022 16:27
 Operator : SY/MD
 Sample : N5321-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN6DL

Manual IntegrationsAPPROVED

Quant Time: Nov 02 05:13:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 02 05:10:28 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 11/03/2022
 Supervised By :Mahesh Dadoda 11/03/2022

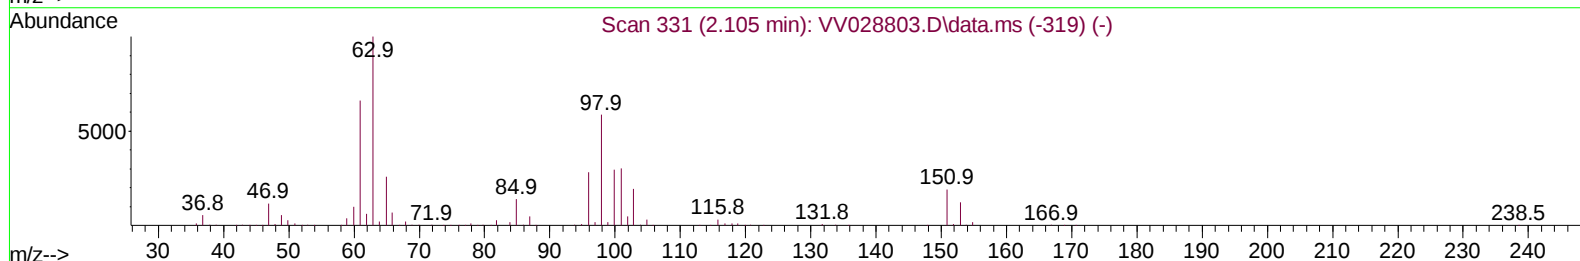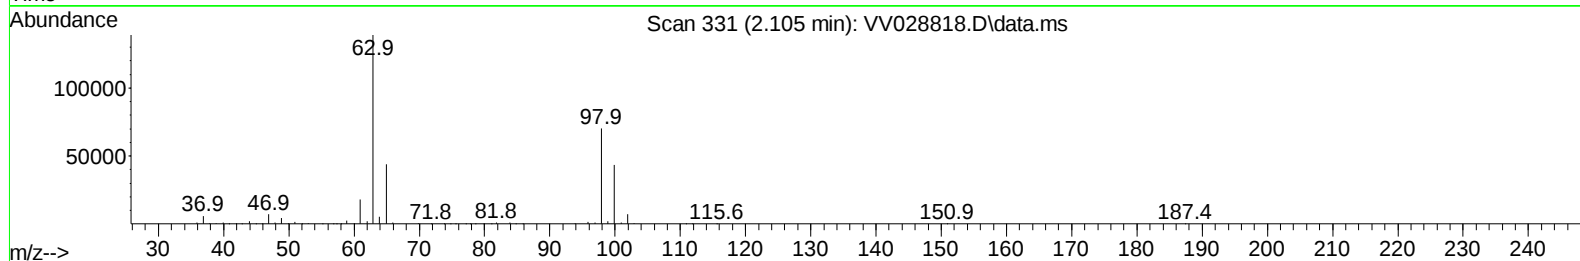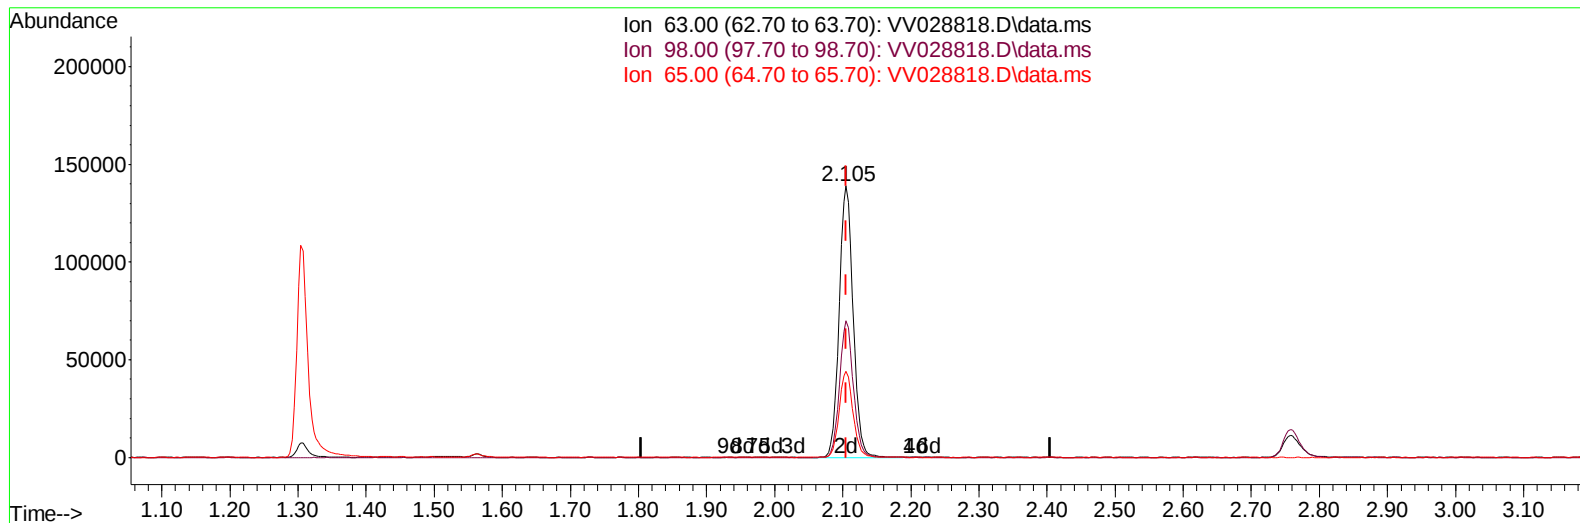

TIC: VV028818.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (+ 0.000) 26.53 ug/L m

response 198594

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	62.00	0.03#
65.00	23.30	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028818.D
 Acq On : 01 Nov 2022 16:27
 Operator : SY/MD
 Sample : N5321-12DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN6DL

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 11/03/2022
 Supervised By : Mahesh Dadoda 11/03/2022

Quant Time: Nov 02 05:13:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 02 05:10:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	415156	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	369850	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	157781	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	125066	31.778	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	63.560%	
7) Chloroethane-d5	1.561	69	122548	36.426	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	72.860%	
11) 1,1-Dichloroethene-d2	2.105	63	198594m	26.527	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	53.060%#	
21) 2-Butanone-d5	3.873	46	271341	94.714	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	94.710%	
24) Chloroform-d	4.343	84	249164	41.977	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.960%	
26) 1,2-Dichloroethane-d4	5.024	65	176387	44.932	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.860%	
32) Benzene-d6	5.044	84	501553	43.440	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.880%	
36) 1,2-Dichloropropane-d6	6.066	67	183974	46.413	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	92.820%	
41) Toluene-d8	7.310	98	422849	41.659	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	83.320%	
43) trans-1,3-Dichloroprop...	7.619	79	62879	41.302	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	82.600%	
47) 2-Hexanone-d5	8.085	63	164759	91.977	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	91.980%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	240375	45.988	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.980%	
66) 1,2-Dichlorobenzene-d4	11.616	152	142570	45.777	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	91.560%	
Target Compounds						
5) Vinyl chloride	1.311	62	9158	1.962	ug/L #	75
17) trans-1,2-Dichloroethene	2.757	96	38636	12.900	ug/L	96
20) cis-1,2-Dichloroethene	3.905	96	137353	41.563	ug/L	98
34) Trichloroethene	5.912	95	56461	18.542	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028818.D
Acq On : 01 Nov 2022 16:27
Operator : SY/MD
Sample : N5321-12DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN6DL

Manual IntegrationsAPPROVED

Quant Time: Nov 02 05:13:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 02 05:10:28 2022
Response via : Initial Calibration

Reviewed By : John Carlone 11/03/2022
Supervised By : Mahesh Dadoda 11/03/2022

