

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110122\
 Data File : VW028808.D
 Acq On : 01 Nov 2022 12:02
 Operator : SY/MD
 Sample : N5321-05DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBXA4DL

Quant Time: Nov 02 05:11:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 02 05:10:28 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	407456	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	371330	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	158569	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	126817	32.832	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	65.660%	
7) Chloroethane-d5	1.564	69	131382	39.789	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.580%	
11) 1,1-Dichloroethene-d2	2.105	63	206191	28.063	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	56.120%#	
21) 2-Butanone-d5	3.876	46	280829	99.878	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	99.880%	
24) Chloroform-d	4.343	84	248456	42.649	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.300%	
26) 1,2-Dichloroethane-d4	5.027	65	175449	45.538	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.080%	
32) Benzene-d6	5.047	84	511488	44.124	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.240%	
36) 1,2-Dichloropropane-d6	6.066	67	182578	45.877	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	91.760%	
41) Toluene-d8	7.310	98	433186	42.508	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	85.020%	
43) trans-1,3-Dichloroprop...	7.619	79	64629	42.283	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.560%	
47) 2-Hexanone-d5	8.085	63	170237	94.656	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	94.660%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	236898	45.142	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.280%	
66) 1,2-Dichlorobenzene-d4	11.616	152	145125	46.366	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.740%	
Target Compounds						
17) trans-1,2-Dichloroethene	2.761	96	3967	1.350	ug/L	96
20) cis-1,2-Dichloroethene	3.908	96	29589	9.123	ug/L #	99
34) Trichloroethene	5.908	95	134178	43.890	ug/L	97
46) Tetrachloroethene	7.973	164	20046	9.461	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028808.D
Acq On : 01 Nov 2022 12:02
Operator : SY/MD
Sample : N5321-05DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBXA4DL

Quant Time: Nov 02 05:11:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 02 05:10:28 2022
Response via : Initial Calibration




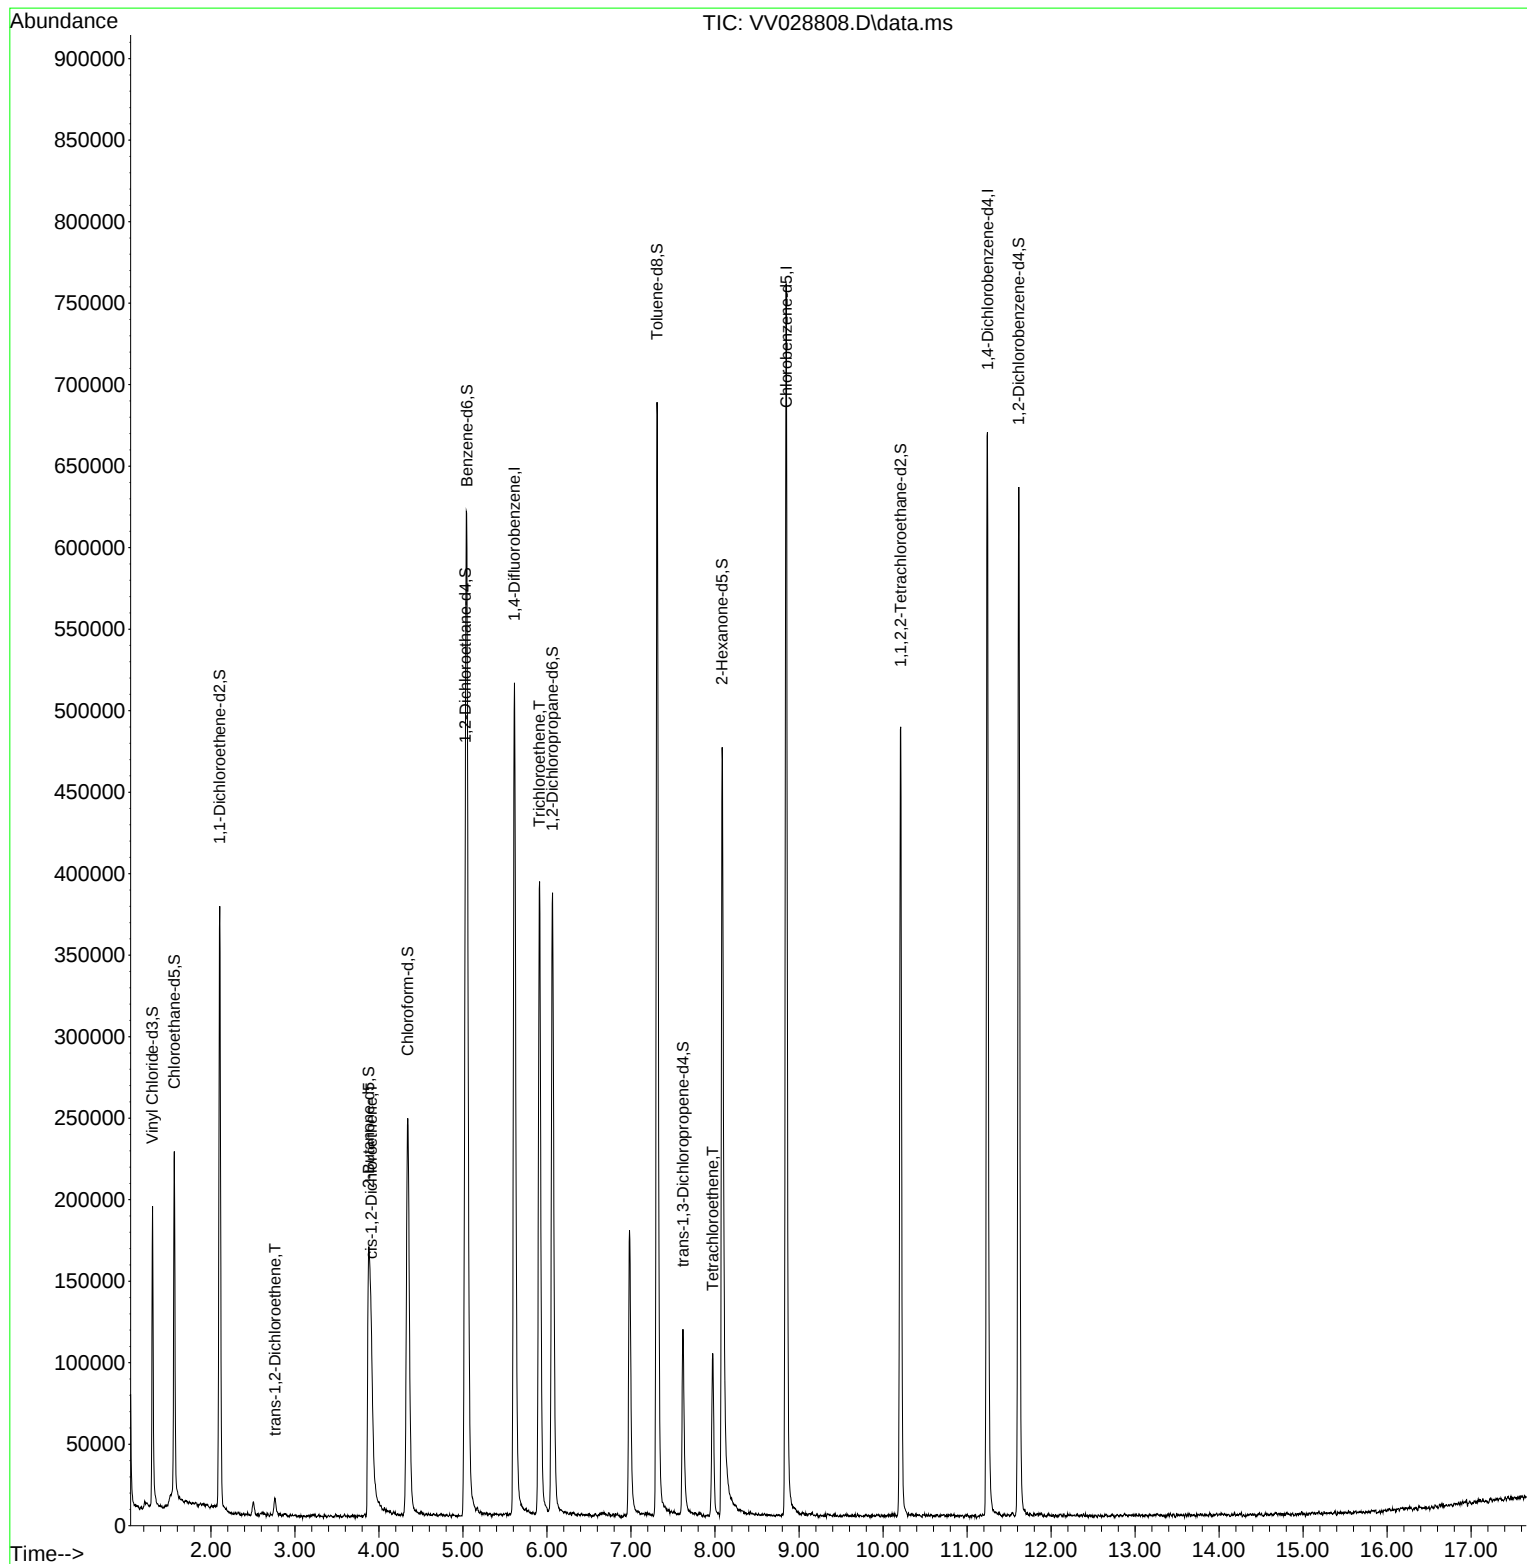


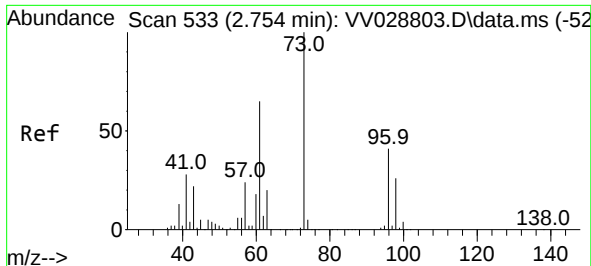

#17
trans-1,2-Dichloroethene
Concen: 1.350 ug/L
RT: 2.761 min Scan# 51
Delta R.T. 0.006 min
Lab File: VV028808.D
Acq: 01 Nov 2022 12:02




Instrument :
MSVOA_V
ClientSampleId :
DBXA4DL


Tgt Ion: 96 Resp: 3967
Ion Ratio Lower Upper
96 100
61 151.8 109.4 203.2
98 65.0 43.3 80.5

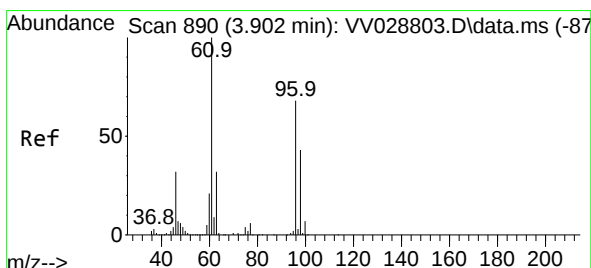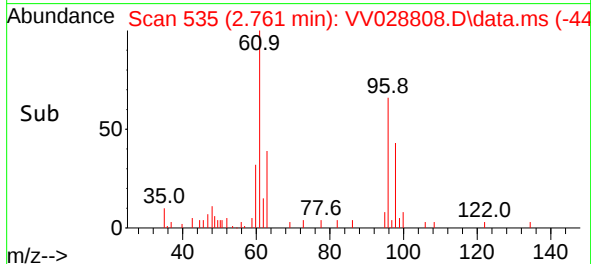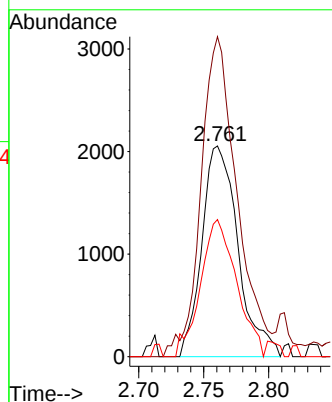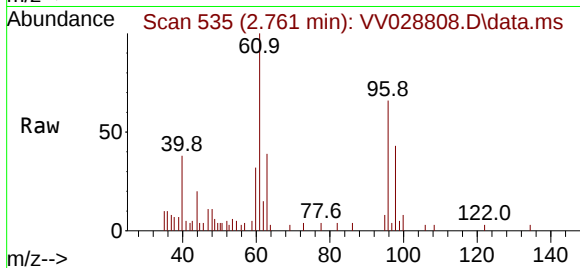

#20
cis-1,2-Dichloroethene
Concen: 9.123 ug/L
RT: 3.908 min Scan# 892
Delta R.T. 0.006 min
Lab File: VV028808.D
Acq: 01 Nov 2022 12:02

Tgt Ion: 96 Resp: 29589
Ion Ratio Lower Upper
96 100
61 147.0 102.3 190.1
68 0.0 0.1 0.3#

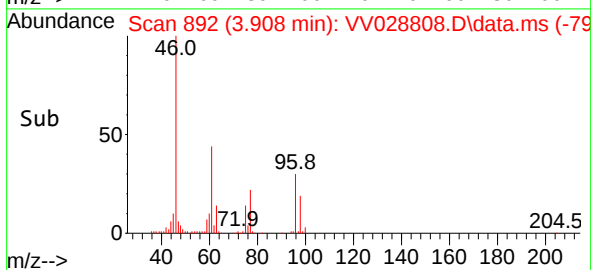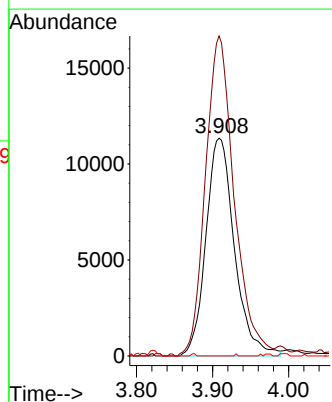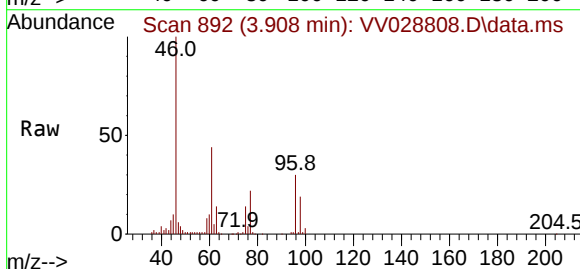

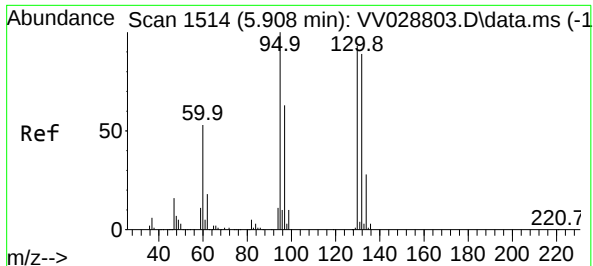

#34

Trichloroethene

Concen: 43.890 ug/L

RT: 5.908 min Scan# 1

Delta R.T. -0.000 min

Lab File: VV028808.D

Acq: 01 Nov 2022 12:02

Instrument :

MSVOA_V

ClientSampleId :

DBXA4DL

Tgt Ion: 95 Resp: 134178





Ion Ratio Lower Upper

95 100

97 63.3 46.2 85.8

132 86.9 63.2 117.4

130 91.6 66.2 123.0

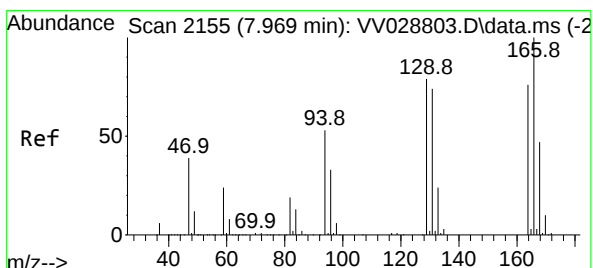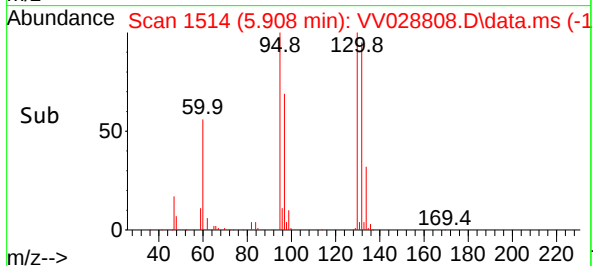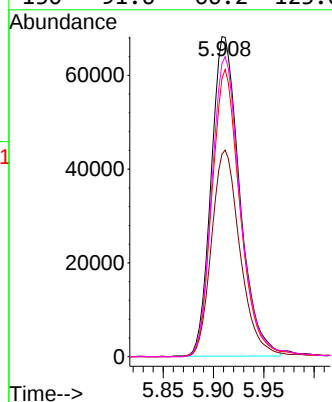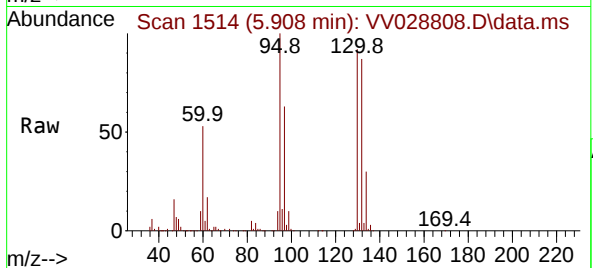

#46

Tetrachloroethene

Concen: 9.461 ug/L

RT: 7.973 min Scan# 2156

Delta R.T. 0.003 min

Lab File: VV028808.D

Acq: 01 Nov 2022 12:02

Tgt Ion:164 Resp: 20046

Ion Ratio Lower Upper

164 100

129 105.6 69.5 129.1

131 98.8 66.4 123.2

166 130.3 88.5 164.3

