

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028804.D
 Acq On : 01 Nov 2022 10:27
 Operator : SY/MD
 Sample : VV1101WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK283

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rBV	265864	286000	15.63%	2.116%
2	1.565	157	163	188	rVB	268952	315704	17.25%	2.335%
3	2.105	322	331	347	rVB	480248	686547	37.51%	5.079%
4	2.468	442	444	446	rBV3	1449	682	0.04%	0.005%
5	2.571	474	476	481	rVB6	1577	1074	0.06%	0.008%
6	2.593	481	483	485	rBV3	1180	696	0.04%	0.005%
7	2.889	570	575	576	rBV4	1052	821	0.04%	0.006%
8	2.921	583	585	589	rVB5	1847	1255	0.07%	0.009%
9	2.941	589	591	596	rVB6	1741	1266	0.07%	0.009%
10	3.021	614	616	619	rVB4	1544	807	0.04%	0.006%
11	3.044	619	623	625	rBV5	1638	1371	0.07%	0.010%
12	3.172	660	663	664	rBV2	1611	651	0.04%	0.005%
13	3.314	703	707	709	rBV5	1100	667	0.04%	0.005%
14	3.359	717	721	725	rVB5	1689	1314	0.07%	0.010%
15	3.388	725	730	734	rBV8	2330	2364	0.13%	0.017%
16	3.407	734	736	740	rVB4	1365	995	0.05%	0.007%
17	3.468	752	755	758	rBV4	1669	1321	0.07%	0.010%
18	3.542	774	778	781	rBV5	1252	1128	0.06%	0.008%
19	3.606	795	798	799	rBV3	1283	807	0.04%	0.006%
20	3.635	803	807	812	rVV5	866	906	0.05%	0.007%
21	3.664	812	816	819	rBV6	1411	1211	0.07%	0.009%
22	3.722	829	834	836	rBV6	1760	1537	0.08%	0.011%
23	3.828	862	867	871	rBV8	2073	1964	0.11%	0.015%
24	3.876	871	882	917	rBV2	150204	457250	24.98%	3.382%
25	4.339	1012	1026	1049	rVB	273232	671128	36.67%	4.965%
26	4.751	1150	1154	1158	rVB6	2654	2229	0.12%	0.016%
27	4.767	1158	1159	1161	rBV2	1168	659	0.04%	0.005%
28	4.941	1211	1213	1215	rBV3	1800	882	0.05%	0.007%
29	5.037	1226	1243	1273	rBV2	698924	1830188	100.00%	13.538%
30	5.609	1408	1421	1445	rBV	520462	1054447	57.61%	7.800%
31	6.063	1550	1562	1589	rBV	415933	850452	46.47%	6.291%
32	6.323	1641	1643	1644	rBV2	1228	608	0.03%	0.004%
33	6.506	1697	1700	1703	rBV5	1754	1635	0.09%	0.012%
34	6.632	1733	1739	1740	rBV5	2842	2572	0.14%	0.019%
35	6.886	1816	1818	1820	rBV3	1629	593	0.03%	0.004%
36	6.905	1820	1824	1826	rBV5	1592	1397	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028804.D
 Acq On : 01 Nov 2022 10:27
 Operator : SY/MD
 Sample : VV1101WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK283

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.979	1837	1847	1871	rVV	195923	366771	20.04%	2.713%
38	7.307	1938	1949	1974	rBV	783599	1383341	75.58%	10.233%
39	7.616	2035	2045	2072	rBV	128745	240934	13.16%	1.782%
40	8.011	2166	2168	2170	rVB3	1729	671	0.04%	0.005%
41	8.085	2179	2191	2225	rBV	484474	993622	54.29%	7.350%
42	8.494	2317	2318	2321	rVB3	1659	837	0.05%	0.006%
43	8.516	2321	2325	2327	rBV5	1683	1112	0.06%	0.008%
44	8.686	2373	2378	2386	rVB9	2252	2596	0.14%	0.019%
45	8.844	2415	2427	2450	rBV	742455	1234159	67.43%	9.129%
46	9.307	2569	2571	2574	rBV3	1196	843	0.05%	0.006%
47	9.622	2666	2669	2674	rVB8	1438	1006	0.05%	0.007%
48	9.712	2694	2697	2700	rVB5	2117	1223	0.07%	0.009%
49	9.751	2706	2709	2712	rBV4	1432	1048	0.06%	0.008%
50	9.850	2738	2740	2745	rVB6	1437	849	0.05%	0.006%
51	9.876	2745	2748	2752	rBV5	1308	992	0.05%	0.007%
52	9.928	2760	2764	2769	rBV9	2347	2421	0.13%	0.018%
53	10.114	2820	2822	2826	rBV4	1250	972	0.05%	0.007%
54	10.140	2826	2830	2832	rVB4	1206	723	0.04%	0.005%
55	10.156	2833	2835	2837	rVB3	1762	745	0.04%	0.006%
56	10.207	2839	2851	2867	rBV	506834	809855	44.25%	5.991%
57	10.416	2914	2916	2920	rBV5	1045	658	0.04%	0.005%
58	10.619	2972	2979	2981	rBV8	1802	1977	0.11%	0.015%
59	10.998	3095	3097	3103	rVB7	2002	1238	0.07%	0.009%
60	11.027	3103	3106	3109	rBV4	1322	1007	0.06%	0.007%
61	11.239	3162	3172	3190	rBV	695201	1090527	59.59%	8.067%
62	11.500	3250	3253	3255	rBV4	1705	924	0.05%	0.007%
63	11.616	3278	3289	3307	rVV	689453	1106680	60.47%	8.186%
64	11.960	3394	3396	3400	rVB5	1784	698	0.04%	0.005%
65	12.133	3446	3450	3451	rVV3	1279	745	0.04%	0.006%
66	12.156	3455	3457	3460	rVB4	1487	757	0.04%	0.006%
67	12.194	3467	3469	3473	rBV6	1134	657	0.04%	0.005%
68	12.394	3527	3531	3535	rBV7	1474	1408	0.08%	0.010%
69	12.423	3537	3540	3548	rVB9	1782	2159	0.12%	0.016%
70	12.464	3548	3553	3554	rBV4	974	907	0.05%	0.007%
71	12.545	3576	3578	3579	rBV2	1513	590	0.03%	0.004%
72	12.612	3595	3599	3600	rBV4	850	580	0.03%	0.004%
73	12.789	3649	3654	3655	rBV5	1935	1766	0.10%	0.013%
74	12.850	3670	3673	3674	rBV3	1342	687	0.04%	0.005%
75	12.882	3681	3683	3686	rBV3	1447	705	0.04%	0.005%
76	12.934	3696	3699	3702	rBV4	1945	1409	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028804.D
 Acq On : 01 Nov 2022 10:27
 Operator : SY/MD
 Sample : VV1101WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK283

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.960	3704	3707	3710	rVB4	2415	1576	0.09%	0.012%
78	12.982	3710	3714	3716	rBV5	1043	960	0.05%	0.007%
79	13.079	3742	3744	3745	rBV2	1575	713	0.04%	0.005%
80	13.181	3772	3776	3778	rBV3	1080	996	0.05%	0.007%
81	13.214	3784	3786	3790	rBV5	1435	1052	0.06%	0.008%
82	13.262	3792	3801	3810	rVB10	8323	14638	0.80%	0.108%
83	13.435	3851	3855	3858	rBV6	1692	1477	0.08%	0.011%
84	13.458	3858	3862	3866	rBV6	1667	1431	0.08%	0.011%
85	13.497	3866	3874	3886	rBV	16881	30920	1.69%	0.229%
86	13.574	3896	3898	3902	rBV4	1129	927	0.05%	0.007%
87	13.616	3908	3911	3915	rVB5	2173	1389	0.08%	0.010%
88	13.677	3927	3930	3933	rBV4	2075	1580	0.09%	0.012%
89	13.905	3997	4001	4002	rBV4	1466	1165	0.06%	0.009%
90	14.075	4052	4054	4058	rBV5	1596	1008	0.06%	0.007%
91	14.201	4090	4093	4094	rBV3	1205	666	0.04%	0.005%
92	14.394	4148	4153	4155	rBV5	1890	1652	0.09%	0.012%
93	14.458	4171	4173	4177	rBV4	1465	1135	0.06%	0.008%
94	14.477	4177	4179	4182	rVV4	987	576	0.03%	0.004%
95	14.680	4240	4242	4244	rBV3	1441	819	0.04%	0.006%
96	14.738	4256	4260	4264	rVB6	1994	1796	0.10%	0.013%
97	14.763	4264	4268	4271	rBV5	2693	2189	0.12%	0.016%
98	14.779	4271	4273	4274	rBV2	1175	581	0.03%	0.004%
99	14.960	4325	4329	4332	rBV6	1704	1563	0.09%	0.012%
100	15.664	4546	4548	4554	rVB6	2687	1706	0.09%	0.013%




Sum of corrected areas: 13518442

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028804.D
Acq On : 01 Nov 2022 10:27
Operator : SY/MD
Sample : VV1101WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK283

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

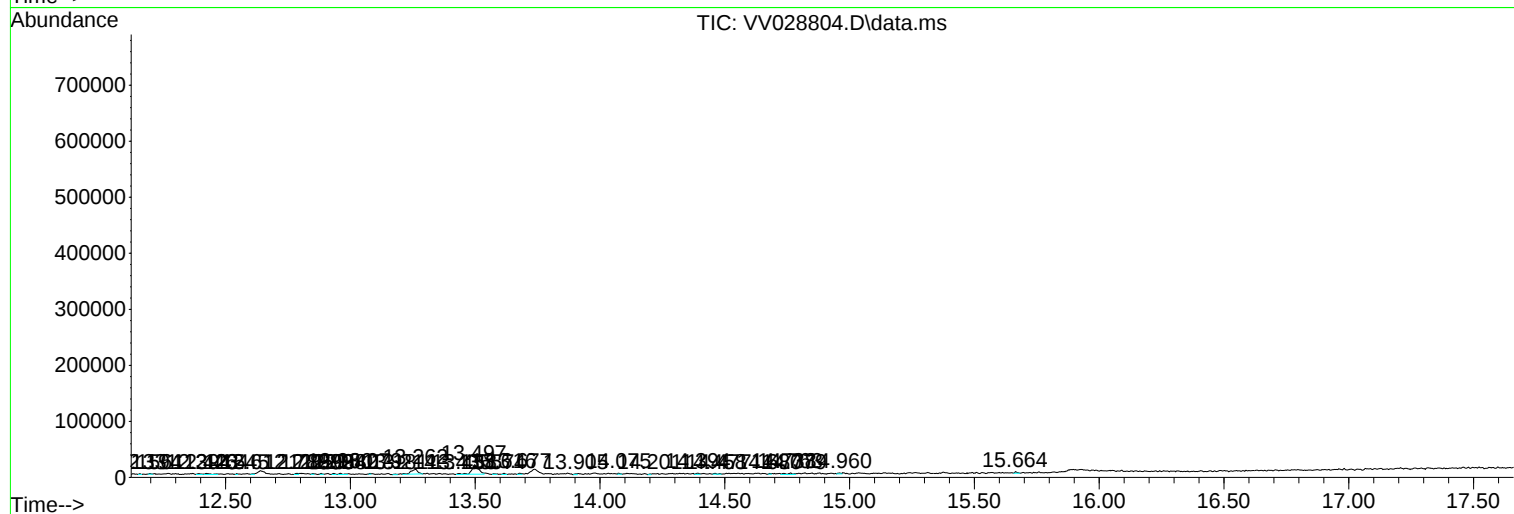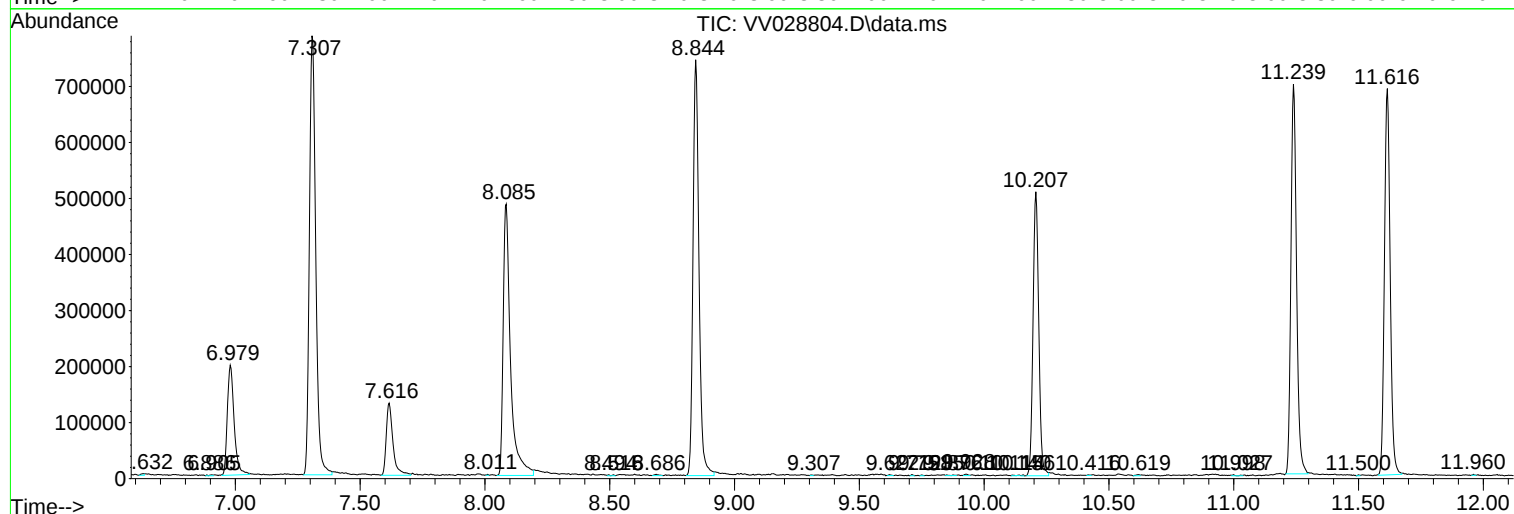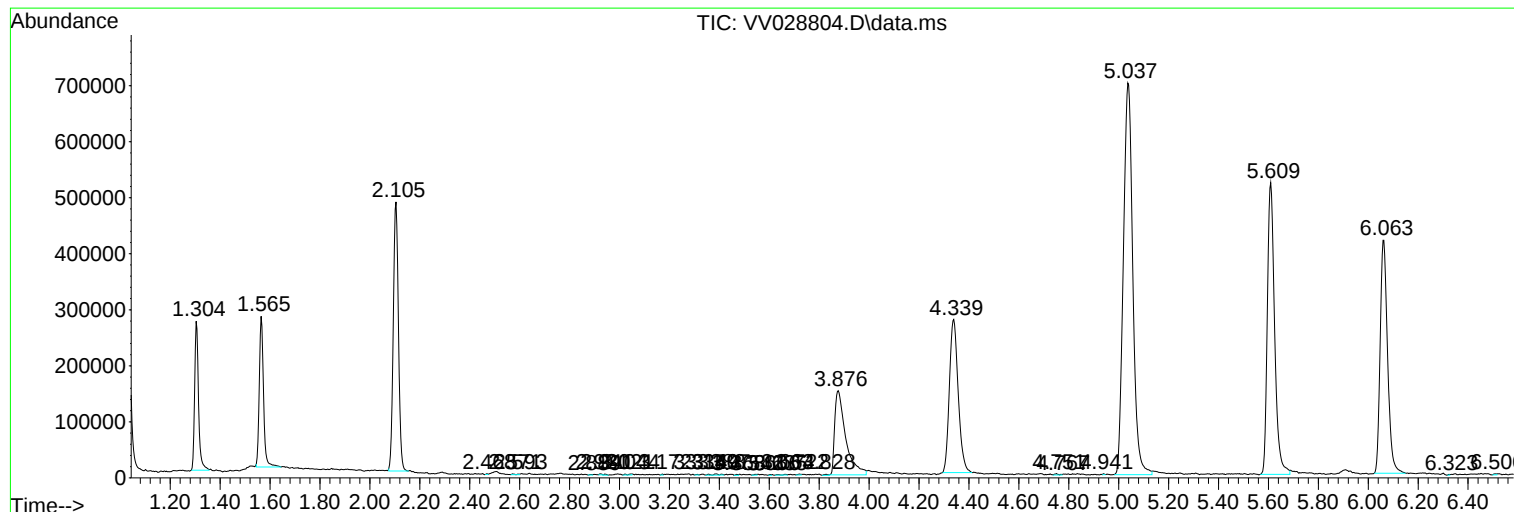

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028804.D
Acq On : 01 Nov 2022 10:27
Operator : SY/MD
Sample : VV1101WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK283

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028804.D
Acq On : 01 Nov 2022 10:27
Operator : SY/MD
Sample : VV1101WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK283

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc