

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028805.D
 Acq On : 01 Nov 2022 10:51
 Operator : SY/MD
 Sample : N5321-03DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWW1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rVB	213924	240061	14.81%	1.721%
2	1.565	157	163	178	rVB	225024	259188	15.99%	1.858%
3	2.105	322	331	344	rVB	389654	558983	34.48%	4.008%
4	2.677	507	509	510	rBV2	1307	511	0.03%	0.004%
5	2.757	525	534	555	rVB	75719	136974	8.45%	0.982%
6	2.899	576	578	579	rBV2	1260	558	0.03%	0.004%
7	3.124	641	648	650	rBV7	2077	2146	0.13%	0.015%
8	3.224	677	679	680	rBV2	1145	433	0.03%	0.003%
9	3.249	685	687	689	rVB3	1183	387	0.02%	0.003%
10	3.304	700	704	706	rVB4	1183	869	0.05%	0.006%
11	3.323	706	710	711	rBV4	1851	1224	0.08%	0.009%
12	3.352	717	719	722	rBV4	1887	1241	0.08%	0.009%
13	3.410	733	737	740	rBV5	1471	1104	0.07%	0.008%
14	3.426	740	742	745	rVV4	1353	779	0.05%	0.006%
15	3.458	747	752	755	rBV5	2082	2028	0.13%	0.015%
16	3.481	755	759	761	rBV3	1575	834	0.05%	0.006%
17	3.529	772	774	778	rBV5	998	608	0.04%	0.004%
18	3.593	792	794	797	rBV4	1489	1122	0.07%	0.008%
19	3.626	802	804	808	rVB3	1276	743	0.05%	0.005%
20	3.648	808	811	815	rBV6	1793	1781	0.11%	0.013%
21	3.706	825	829	834	rBV8	1867	1848	0.11%	0.013%
22	3.754	842	844	846	rBV3	1970	920	0.06%	0.007%
23	3.802	857	859	861	rBV3	947	392	0.02%	0.003%
24	3.828	865	867	868	rBV3	1065	306	0.02%	0.002%
25	3.899	872	889	916	rBV2	224849	837079	51.64%	6.001%
26	4.343	1013	1027	1055	rBV2	248903	617143	38.07%	4.425%
27	4.764	1157	1158	1162	rBV4	1003	820	0.05%	0.006%
28	4.892	1194	1198	1202	rBV6	2009	1861	0.11%	0.013%
29	4.963	1218	1220	1222	rVB4	1266	476	0.03%	0.003%
30	5.040	1228	1244	1271	rBV2	624712	1621127	100.00%	11.623%
31	5.613	1408	1422	1444	rBV	530053	1082764	66.79%	7.763%
32	5.912	1502	1515	1534	rBV	306523	617489	38.09%	4.427%
33	6.066	1551	1563	1587	rBV	376903	764922	47.18%	5.484%
34	6.487	1691	1694	1697	rBV5	1752	1343	0.08%	0.010%
35	6.503	1697	1699	1701	rVB3	1348	440	0.03%	0.003%
36	6.625	1735	1737	1738	rBV2	2280	986	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028805.D
 Acq On : 01 Nov 2022 10:51
 Operator : SY/MD
 Sample : N5321-03DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWW1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.847	1800	1806	1813	rVB2	1751	2247	0.14%	0.016%
38	6.918	1826	1828	1831	rBV4	1012	494	0.03%	0.004%
39	6.982	1838	1848	1874	rBV	177560	330267	20.37%	2.368%
40	7.310	1939	1950	1973	rBV	681534	1205329	74.35%	8.642%
41	7.619	2036	2046	2063	rBV	113077	208237	12.85%	1.493%
42	7.889	2128	2130	2131	rBV2	887	384	0.02%	0.003%
43	7.969	2143	2155	2174	rBV	169871	294350	18.16%	2.110%
44	8.085	2181	2191	2225	rBV	475223	938489	57.89%	6.729%
45	8.847	2414	2428	2456	rBV	769133	1286725	79.37%	9.225%
46	9.313	2572	2573	2574	rBV	722	251	0.02%	0.002%
47	9.326	2575	2577	2582	rVB6	1660	1092	0.07%	0.008%
48	9.349	2582	2584	2586	rBV3	1289	703	0.04%	0.005%
49	9.378	2590	2593	2594	rBV3	1650	1058	0.07%	0.008%
50	9.481	2620	2625	2626	rBV4	1436	884	0.05%	0.006%
51	9.519	2635	2637	2639	rBV3	1734	939	0.06%	0.007%
52	9.635	2671	2673	2677	rBV5	1357	808	0.05%	0.006%
53	9.677	2684	2686	2688	rBV3	963	547	0.03%	0.004%
54	9.754	2707	2710	2713	rBV5	1655	1215	0.07%	0.009%
55	9.793	2720	2722	2723	rBV2	1909	875	0.05%	0.006%
56	9.821	2729	2731	2732	rBV2	1172	504	0.03%	0.004%
57	9.834	2733	2735	2737	rVV3	1304	586	0.04%	0.004%
58	9.857	2740	2742	2744	rBV3	1075	478	0.03%	0.003%
59	10.040	2796	2799	2802	rBV4	1677	1254	0.08%	0.009%
60	10.053	2802	2803	2805	rVB2	1574	429	0.03%	0.003%
61	10.095	2814	2816	2818	rBV3	1150	691	0.04%	0.005%
62	10.124	2821	2825	2827	rBV5	1142	952	0.06%	0.007%
63	10.207	2840	2851	2873	rBV	478400	765668	47.23%	5.489%
64	10.477	2930	2935	2939	rBV7	2437	2292	0.14%	0.016%
65	10.513	2945	2946	2947	rVB	771	149	0.01%	0.001%
66	10.526	2947	2950	2953	rBV4	1869	1392	0.09%	0.010%
67	10.542	2953	2955	2961	rVV6	1940	1697	0.10%	0.012%
68	10.612	2974	2977	2979	rBV3	2130	1518	0.09%	0.011%
69	10.667	2991	2994	2996	rBV4	1014	733	0.05%	0.005%
70	10.702	3004	3005	3007	rBV2	1013	349	0.02%	0.003%
71	10.744	3015	3018	3023	rBV7	1778	1559	0.10%	0.011%
72	10.796	3031	3034	3035	rBV3	1539	684	0.04%	0.005%
73	10.905	3065	3068	3071	rBV4	2469	2062	0.13%	0.015%
74	10.982	3090	3092	3093	rBV2	1170	521	0.03%	0.004%
75	11.075	3119	3121	3124	rVB4	1572	683	0.04%	0.005%
76	11.130	3136	3138	3139	rBV2	1279	576	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110122\
 Data File : VW028805.D
 Acq On : 01 Nov 2022 10:51
 Operator : SY/MD
 Sample : N5321-03DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWW1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	11.149	3142	3144	3146	rVB3	982	318	0.02%	0.002%
78	11.239	3162	3172	3197	rBV	688789	1109970	68.47%	7.958%
79	11.526	3258	3261	3264	rBV5	2440	2157	0.13%	0.015%
80	11.571	3272	3275	3276	rBV3	1645	884	0.05%	0.006%
81	11.616	3278	3289	3309	rVV	617570	995051	61.38%	7.134%
82	11.973	3396	3400	3401	rBV5	1793	907	0.06%	0.007%
83	12.069	3427	3430	3431	rBV3	1009	511	0.03%	0.004%
84	12.355	3517	3519	3522	rBV4	1080	989	0.06%	0.007%
85	12.619	3599	3601	3602	rBV3	1290	421	0.03%	0.003%
86	12.760	3643	3645	3649	rVB5	1575	938	0.06%	0.007%
87	12.780	3649	3651	3654	rBV4	1386	999	0.06%	0.007%
88	12.886	3679	3684	3688	rVB8	1628	1585	0.10%	0.011%
89	12.908	3688	3691	3695	rBV5	1580	1639	0.10%	0.012%
90	12.956	3700	3706	3707	rBV5	1903	1207	0.07%	0.009%
91	12.992	3715	3717	3719	rBV3	1634	858	0.05%	0.006%
92	13.066	3738	3740	3742	rBV3	1085	415	0.03%	0.003%
93	13.088	3744	3747	3749	rBV5	1340	692	0.04%	0.005%
94	13.407	3844	3846	3848	rBV4	1351	730	0.05%	0.005%
95	13.493	3868	3873	3874	rBV4	2350	2010	0.12%	0.014%
96	13.796	3965	3967	3973	rVB6	1760	1584	0.10%	0.011%
97	13.831	3975	3978	3981	rBV5	1693	1125	0.07%	0.008%
98	14.066	4049	4051	4054	rBV3	1388	802	0.05%	0.006%
99	14.204	4092	4094	4096	rBV3	1060	508	0.03%	0.004%
100	14.323	4129	4131	4132	rBV2	1324	466	0.03%	0.003%




Sum of corrected areas: 13947927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028805.D
Acq On : 01 Nov 2022 10:51
Operator : SY/MD
Sample : N5321-03DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWW1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

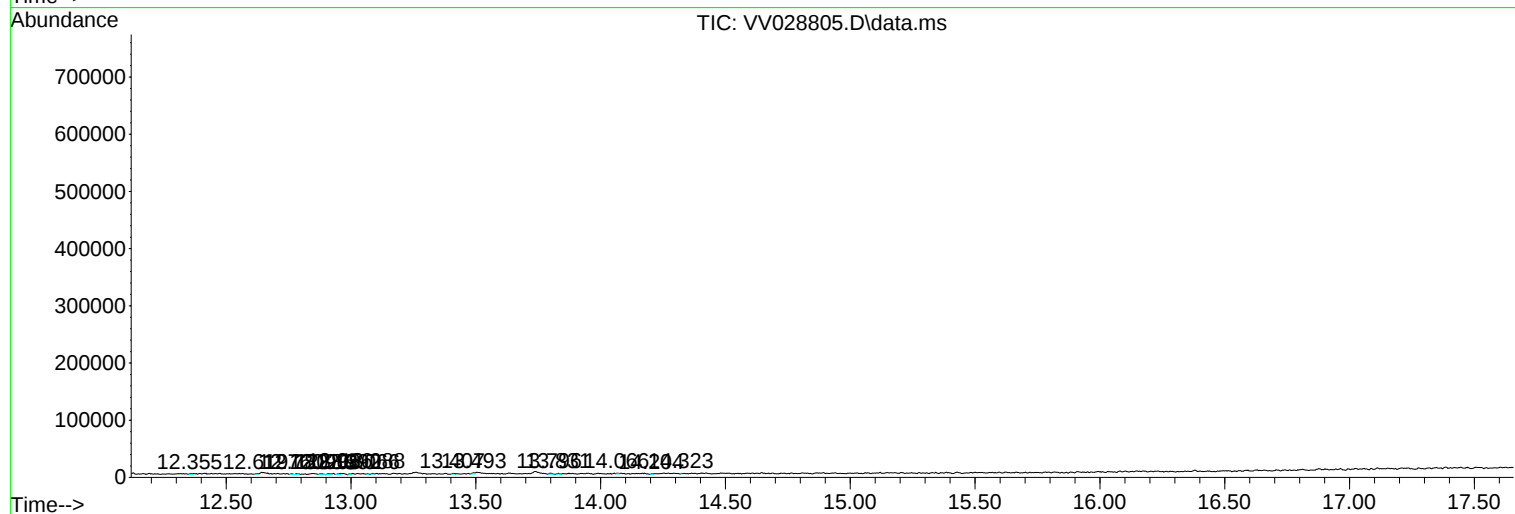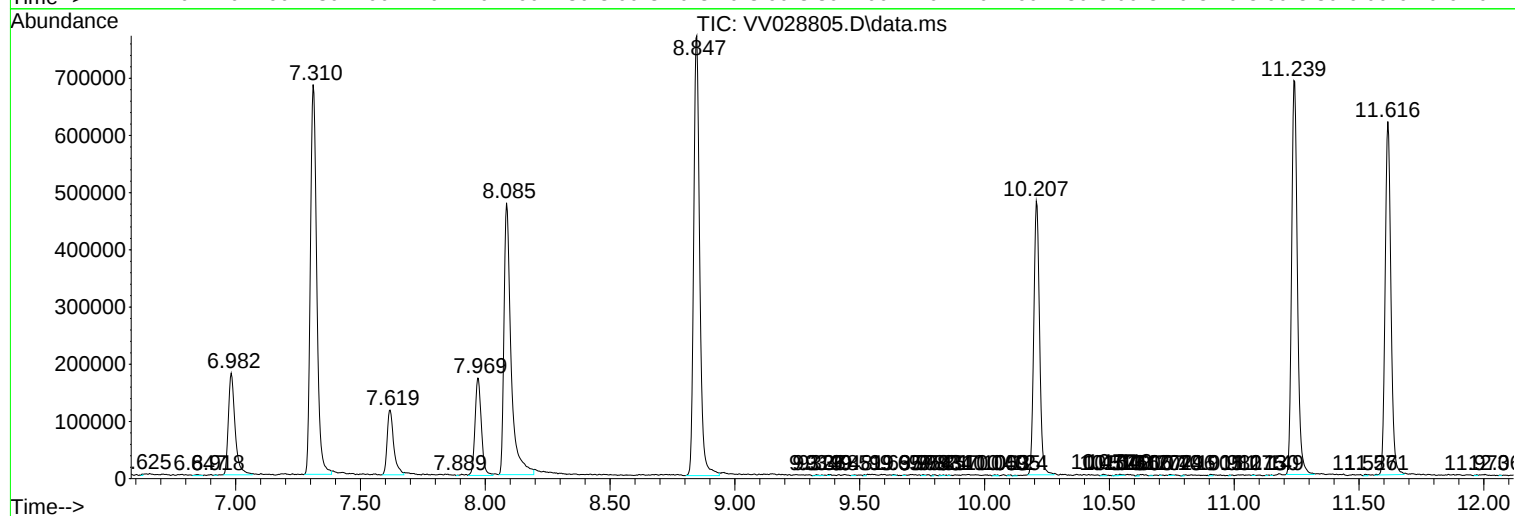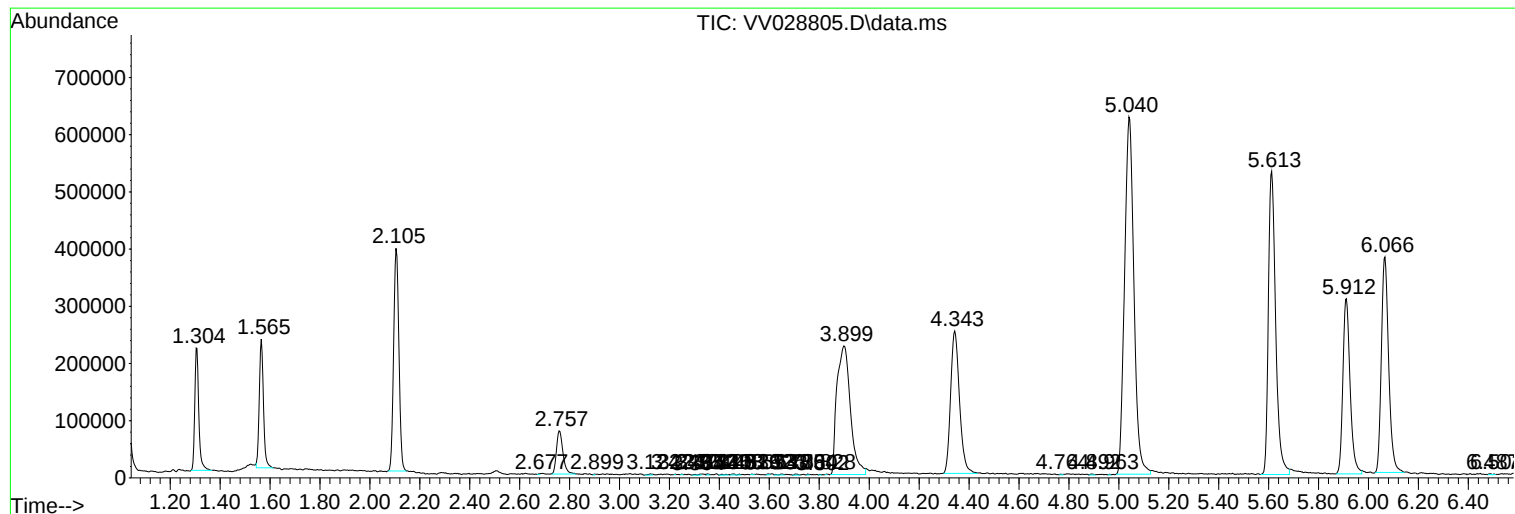

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028805.D
Acq On : 01 Nov 2022 10:51
Operator : SY/MD
Sample : N5321-03DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWW1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028805.D
Acq On : 01 Nov 2022 10:51
Operator : SY/MD
Sample : N5321-03DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWW1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------