

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028810.D
 Acq On : 01 Nov 2022 12:50
 Operator : SY/MD
 Sample : N5301-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWP1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rBV	175933	198509	12.32%	1.514%
2	1.561	156	162	177	rVB	189326	224384	13.92%	1.711%
3	2.105	322	331	345	rVB	370943	524982	32.58%	4.003%
4	2.465	439	443	445	rBV5	2006	2008	0.12%	0.015%
5	2.481	445	448	449	rBV3	2283	1264	0.08%	0.010%
6	2.590	480	482	483	rBV2	1300	446	0.03%	0.003%
7	2.757	524	534	552	rBV	130005	230032	14.27%	1.754%
8	2.892	574	576	577	rBV2	1287	516	0.03%	0.004%
9	2.966	595	599	602	rBV5	1325	1484	0.09%	0.011%
10	3.088	634	637	639	rBV4	2522	1507	0.09%	0.011%
11	3.153	654	657	660	rBV5	2265	1323	0.08%	0.010%
12	3.169	660	662	666	rBV5	1691	1494	0.09%	0.011%
13	3.249	685	687	691	rVB5	1220	766	0.05%	0.006%
14	3.272	691	694	700	rVB7	1741	2031	0.13%	0.015%
15	3.297	700	702	705	rBV4	1493	728	0.05%	0.006%
16	3.349	713	718	719	rBV4	1376	1150	0.07%	0.009%
17	3.365	719	723	725	rBV5	1741	1287	0.08%	0.010%
18	3.410	735	737	739	rVB3	1450	480	0.03%	0.004%
19	3.490	760	762	766	rVB4	1025	629	0.04%	0.005%
20	3.539	775	777	778	rBV2	1566	699	0.04%	0.005%
21	3.571	785	787	791	rBV5	894	649	0.04%	0.005%
22	3.600	792	796	799	rVB7	1180	1001	0.06%	0.008%
23	3.625	801	804	806	rBV4	1191	840	0.05%	0.006%
24	3.648	809	811	814	rVB3	1683	840	0.05%	0.006%
25	3.667	814	817	820	rBV4	628	407	0.03%	0.003%
26	3.690	822	824	825	rBV2	1676	689	0.04%	0.005%
27	3.728	832	836	839	rBV6	1454	1436	0.09%	0.011%
28	3.809	858	861	865	rBV5	1364	1407	0.09%	0.011%
29	3.838	868	870	871	rBV2	1300	436	0.03%	0.003%
30	3.902	871	890	920	rBV2	262015	975689	60.54%	7.440%
31	4.217	986	988	989	rBV	1341	438	0.03%	0.003%
32	4.342	1013	1027	1052	rBV	241875	599880	37.22%	4.575%
33	4.748	1151	1153	1154	rBV2	1129	429	0.03%	0.003%
34	4.825	1173	1177	1179	rBV5	1658	1447	0.09%	0.011%
35	4.850	1182	1185	1187	rBV4	1471	887	0.06%	0.007%
36	5.040	1228	1244	1272	rBV2	612789	1611519	100.00%	12.289%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110122\
 Data File : VW028810.D
 Acq On : 01 Nov 2022 12:50
 Operator : SY/MD
 Sample : N5301-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWP1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	5.612	1410	1422	1448	rBV	516261	1057197	65.60%	8.062%
38	5.915	1503	1516	1531	rBV3	62396	135184	8.39%	1.031%
39	6.066	1551	1563	1591	rBV	377351	763229	47.36%	5.820%
40	6.387	1661	1663	1665	rBV2	1962	939	0.06%	0.007%
41	6.509	1699	1701	1702	rBV2	1068	443	0.03%	0.003%
42	6.747	1772	1775	1777	rBV4	1708	1030	0.06%	0.008%
43	6.809	1791	1794	1796	rBV3	1808	1208	0.07%	0.009%
44	6.889	1816	1819	1820	rBV3	930	501	0.03%	0.004%
45	6.927	1828	1831	1832	rBV3	2158	1360	0.08%	0.010%
46	6.982	1838	1848	1865	rBV	174677	320168	19.87%	2.442%
47	7.310	1940	1950	1977	rBV	682552	1197979	74.34%	9.136%
48	7.619	2037	2046	2060	rBV	112319	196510	12.19%	1.499%
49	7.837	2112	2114	2118	rBV5	1370	845	0.05%	0.006%
50	7.915	2135	2138	2139	rBV3	1418	792	0.05%	0.006%
51	8.085	2181	2191	2220	rBV	464544	902249	55.99%	6.880%
52	8.458	2304	2307	2308	rBV2	1312	670	0.04%	0.005%
53	8.779	2403	2407	2409	rBV5	1298	843	0.05%	0.006%
54	8.847	2417	2428	2452	rBV	757688	1240611	76.98%	9.461%
55	9.143	2518	2520	2523	rBV4	1629	1195	0.07%	0.009%
56	9.529	2638	2640	2641	rBV3	1016	412	0.03%	0.003%
57	9.603	2660	2663	2666	rBV4	1156	1118	0.07%	0.009%
58	9.644	2672	2676	2677	rBV3	1489	1160	0.07%	0.009%
59	9.718	2697	2699	2701	rBV2	2057	1196	0.07%	0.009%
60	9.767	2712	2714	2715	rBV2	1490	384	0.02%	0.003%
61	9.796	2720	2723	2724	rBV4	1030	580	0.04%	0.004%
62	9.995	2783	2785	2789	rBV4	1629	1183	0.07%	0.009%
63	10.207	2839	2851	2869	rBV	482208	770178	47.79%	5.873%
64	10.541	2953	2955	2960	rBV6	1630	1171	0.07%	0.009%
65	10.715	3007	3009	3012	rBV4	1290	724	0.04%	0.006%
66	10.905	3065	3068	3070	rBV4	1090	622	0.04%	0.005%
67	10.918	3070	3072	3076	rVB4	1666	991	0.06%	0.008%
68	10.937	3076	3078	3081	rBV4	1519	711	0.04%	0.005%
69	10.953	3081	3083	3087	rVB4	1973	988	0.06%	0.008%
70	10.985	3090	3093	3097	rBV6	1875	1290	0.08%	0.010%
71	11.008	3097	3100	3101	rBV4	1145	521	0.03%	0.004%
72	11.056	3111	3115	3121	rVB9	1422	1425	0.09%	0.011%
73	11.159	3145	3147	3150	rBV3	1304	717	0.04%	0.005%
74	11.239	3162	3172	3199	rBV	676047	1078031	66.90%	8.221%
75	11.615	3278	3289	3315	rBV	626096	1009146	62.62%	7.696%
76	11.812	3348	3350	3352	rBV3	1220	560	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028810.D
 Acq On : 01 Nov 2022 12:50
 Operator : SY/MD
 Sample : N5301-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWP1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	11.985	3401	3404	3406	rBV4	1317	804	0.05%	0.006%
78	12.033	3416	3419	3420	rBV3	1409	704	0.04%	0.005%
79	12.062	3426	3428	3430	rBV2	750	448	0.03%	0.003%
80	12.094	3435	3438	3439	rBV4	1196	565	0.04%	0.004%
81	12.143	3450	3453	3456	rBV5	1282	1025	0.06%	0.008%
82	12.246	3483	3485	3487	rBV3	1415	706	0.04%	0.005%
83	12.339	3512	3514	3516	rBV3	1608	837	0.05%	0.006%
84	12.368	3521	3523	3526	rVV4	1718	968	0.06%	0.007%
85	12.384	3526	3528	3533	rVB5	1542	1337	0.08%	0.010%
86	12.467	3551	3554	3555	rBV2	1411	670	0.04%	0.005%
87	12.500	3562	3564	3565	rBV2	1326	582	0.04%	0.004%
88	12.741	3636	3639	3641	rBV3	1120	760	0.05%	0.006%
89	12.850	3669	3673	3676	rBV6	1873	1427	0.09%	0.011%
90	13.056	3735	3737	3739	rBV3	1121	692	0.04%	0.005%
91	13.130	3756	3760	3762	rBV4	1329	851	0.05%	0.006%
92	13.258	3794	3800	3803	rBV9	1906	2195	0.14%	0.017%
93	13.397	3841	3843	3845	rBV3	1475	862	0.05%	0.007%
94	13.429	3850	3853	3856	rVB4	1169	728	0.05%	0.006%
95	13.442	3856	3857	3863	rBV5	2007	1914	0.12%	0.015%
96	13.493	3870	3873	3876	rBV4	2047	1448	0.09%	0.011%
97	14.037	4041	4042	4045	rBV2	1239	700	0.04%	0.005%
98	14.101	4060	4062	4067	rBV6	2158	1641	0.10%	0.013%
99	14.368	4143	4145	4146	rBV2	1264	526	0.03%	0.004%
100	14.914	4313	4315	4318	rVB4	2282	1171	0.07%	0.009%




Sum of corrected areas: 13113335

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028810.D
Acq On : 01 Nov 2022 12:50
Operator : SY/MD
Sample : N5301-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

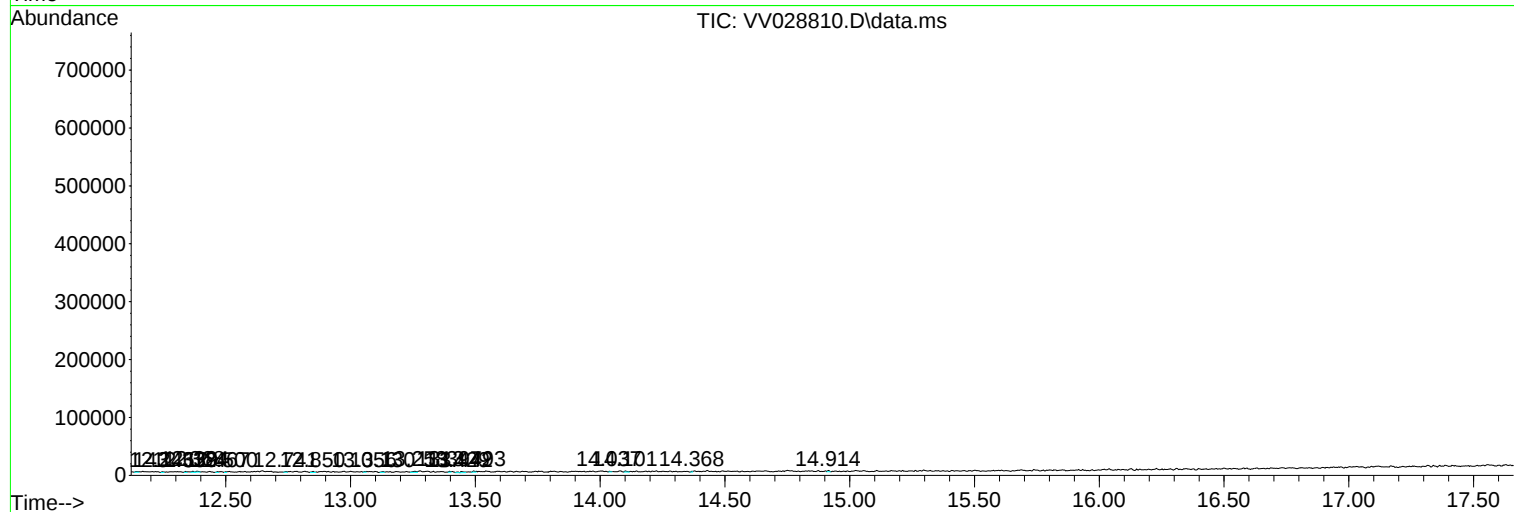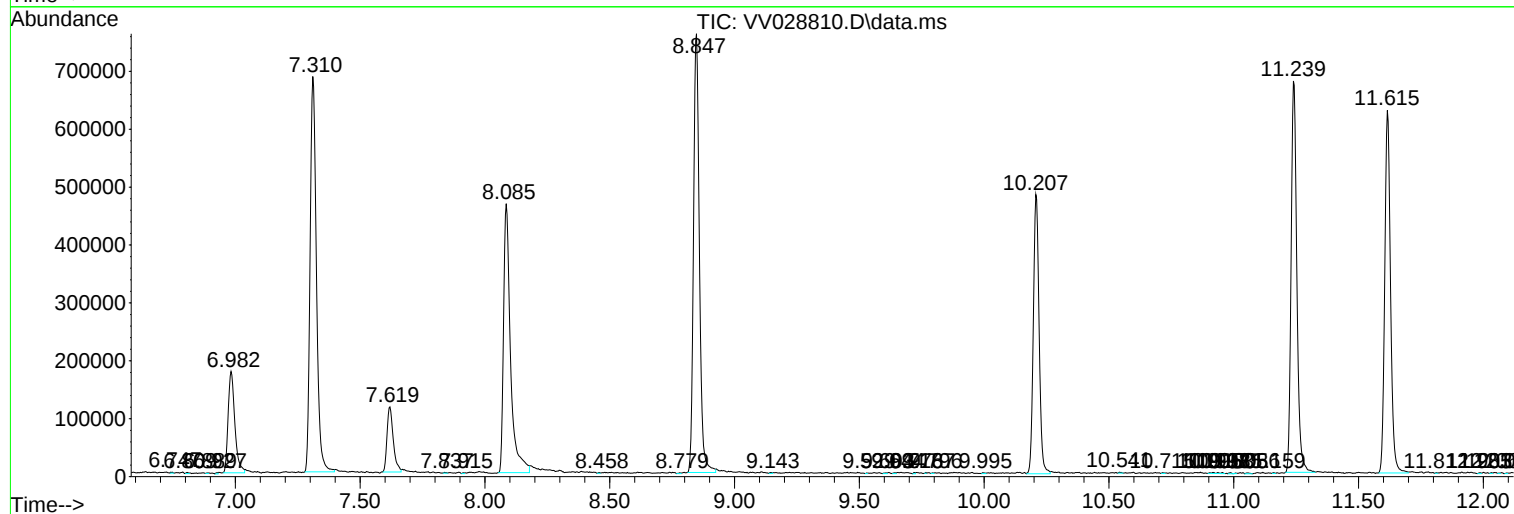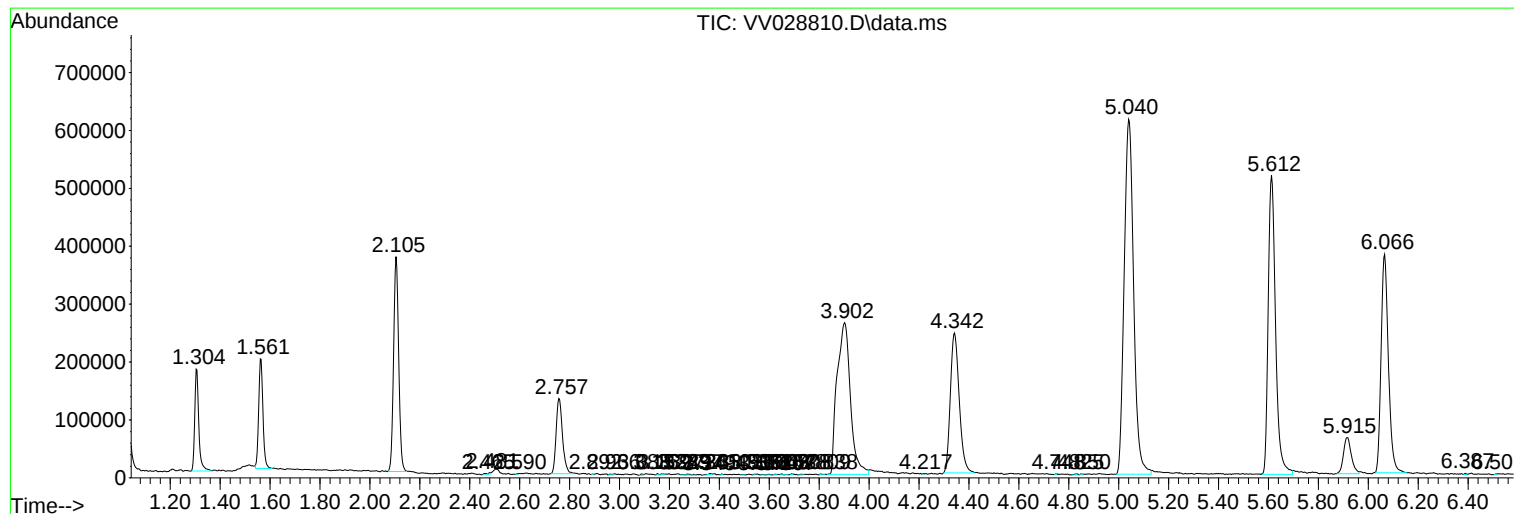

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028810.D
Acq On : 01 Nov 2022 12:50
Operator : SY/MD
Sample : N5301-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028810.D
Acq On : 01 Nov 2022 12:50
Operator : SY/MD
Sample : N5301-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------