

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028813.D
 Acq On : 01 Nov 2022 14:02
 Operator : SY/MD
 Sample : N5301-14DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBXB4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M

Title : VOC Analysis

Signal : TIC: VV028813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	164179	182327	12.19%	1.339%
2	1.564	156	163	178	rVB	176724	208527	13.94%	1.531%
3	2.105	322	331	345	rVB	344133	492500	32.92%	3.616%
4	2.506	447	456	467	rVB	12880	22797	1.52%	0.167%
5	3.011	611	613	616	rVB4	1295	560	0.04%	0.004%
6	3.056	624	627	628	rBV3	1781	815	0.05%	0.006%
7	3.104	640	642	645	rBV4	1556	744	0.05%	0.005%
8	3.140	651	653	655	rVB3	1744	772	0.05%	0.006%
9	3.153	655	657	660	rVB4	1025	626	0.04%	0.005%
10	3.178	660	665	669	rBV8	2045	2212	0.15%	0.016%
11	3.256	686	689	692	rBV4	1183	948	0.06%	0.007%
12	3.301	701	703	706	rVB4	1035	430	0.03%	0.003%
13	3.342	714	716	719	rVB4	1103	677	0.05%	0.005%
14	3.358	719	721	725	rBV5	1417	1126	0.08%	0.008%
15	3.439	742	746	747	rBV4	1274	985	0.07%	0.007%
16	3.506	764	767	770	rBV5	757	611	0.04%	0.004%
17	3.632	802	806	808	rBV5	1133	830	0.06%	0.006%
18	3.703	826	828	830	rBV2	1163	683	0.05%	0.005%
19	3.735	835	838	839	rBV3	1368	613	0.04%	0.005%
20	3.757	842	845	848	rVB5	1678	1131	0.08%	0.008%
21	3.773	848	850	854	rBV3	1122	816	0.05%	0.006%
22	3.812	858	862	864	rBV5	1840	1051	0.07%	0.008%
23	3.902	873	890	915	rBV3	200690	771103	51.54%	5.662%
24	4.194	978	981	987	rBV7	1964	1819	0.12%	0.013%
25	4.236	992	994	996	rBV3	1961	1125	0.08%	0.008%
26	4.342	1015	1027	1055	rVB	230242	569399	38.06%	4.181%
27	4.754	1153	1155	1159	rBV6	2740	2064	0.14%	0.015%
28	4.924	1206	1208	1210	rBV2	793	326	0.02%	0.002%
29	5.043	1229	1245	1275	rBV2	568932	1496196	100.00%	10.985%
30	5.612	1411	1422	1446	rBV	507533	1016285	67.92%	7.462%
31	5.911	1504	1515	1543	rVB	351830	696164	46.53%	5.111%
32	6.066	1552	1563	1586	rVB	351663	706346	47.21%	5.186%
33	6.815	1793	1796	1798	rBV3	1719	917	0.06%	0.007%
34	6.895	1819	1821	1824	rVB4	1142	578	0.04%	0.004%
35	6.911	1824	1826	1827	rBV2	1145	593	0.04%	0.004%
36	6.927	1829	1831	1832	rVB2	1350	409	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028813.D
 Acq On : 01 Nov 2022 14:02
 Operator : SY/MD
 Sample : N5301-14DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBXB4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.982	1839	1848	1873	rBV	157858	292182	19.53%	2.145%
38	7.310	1940	1950	1975	rBV	626767	1105611	73.89%	8.118%
39	7.619	2038	2046	2064	rBV	98824	177981	11.90%	1.307%
40	7.773	2091	2094	2095	rBV3	1485	864	0.06%	0.006%
41	7.915	2137	2138	2141	rBV3	1372	715	0.05%	0.005%
42	7.969	2141	2155	2177	rBV	651913	1089135	72.79%	7.997%
43	8.085	2182	2191	2225	rBV	423950	826979	55.27%	6.072%
44	8.587	2345	2347	2348	rBV	720	313	0.02%	0.002%
45	8.599	2348	2351	2354	rVV5	1628	1020	0.07%	0.007%
46	8.741	2390	2395	2397	rBV5	2305	1634	0.11%	0.012%
47	8.776	2400	2406	2410	rVV7	1709	2005	0.13%	0.015%
48	8.847	2417	2428	2457	rBV	743206	1217388	81.37%	8.938%
49	9.365	2583	2589	2594	rBV9	2611	2622	0.18%	0.019%
50	9.394	2594	2598	2600	rBV5	1205	1037	0.07%	0.008%
51	9.426	2605	2608	2610	rBV4	946	664	0.04%	0.005%
52	9.493	2627	2629	2632	rVB3	1129	407	0.03%	0.003%
53	9.612	2664	2666	2668	rBV3	1004	451	0.03%	0.003%
54	9.879	2746	2749	2750	rBV3	1342	744	0.05%	0.005%
55	9.911	2757	2759	2761	rBV2	1303	543	0.04%	0.004%
56	9.953	2770	2772	2773	rBV2	828	314	0.02%	0.002%
57	9.985	2780	2782	2785	rBV3	1575	1097	0.07%	0.008%
58	10.043	2797	2800	2802	rBV4	1106	527	0.04%	0.004%
59	10.066	2802	2807	2811	rBV7	2101	2482	0.17%	0.018%
60	10.143	2829	2831	2833	rBV3	1192	677	0.05%	0.005%
61	10.210	2840	2852	2871	rBV	436262	706097	47.19%	5.184%
62	10.599	2971	2973	2975	rBV2	1721	681	0.05%	0.005%
63	10.657	2989	2991	2994	rBV4	903	769	0.05%	0.006%
64	10.831	3042	3045	3047	rBV4	1153	858	0.06%	0.006%
65	10.950	3080	3082	3084	rVB3	1360	532	0.04%	0.004%
66	10.963	3084	3086	3089	rBV4	1346	912	0.06%	0.007%
67	11.082	3121	3123	3125	rBV2	958	350	0.02%	0.003%
68	11.130	3136	3138	3140	rBV3	1059	394	0.03%	0.003%
69	11.242	3161	3173	3192	rBV	661245	1055694	70.56%	7.751%
70	11.615	3279	3289	3307	rBV	573213	916932	61.28%	6.732%
71	11.828	3353	3355	3356	rBV	1287	481	0.03%	0.004%
72	12.049	3423	3424	3425	rBV2	1190	364	0.02%	0.003%
73	12.072	3429	3431	3432	rBV2	1317	530	0.04%	0.004%
74	12.194	3465	3469	3470	rBV3	1038	780	0.05%	0.006%
75	12.204	3470	3472	3475	rVB4	1891	729	0.05%	0.005%
76	12.297	3500	3501	3503	rBV2	1048	451	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
 Data File : VV028813.D
 Acq On : 01 Nov 2022 14:02
 Operator : SY/MD
 Sample : N5301-14DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBXB4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.316	3503	3507	3510	rVV5	2193	1743	0.12%	0.013%
78	12.374	3520	3525	3526	rBV5	1434	1023	0.07%	0.008%
79	12.445	3545	3547	3548	rBV2	1042	427	0.03%	0.003%
80	12.641	3606	3608	3611	rBV4	1493	934	0.06%	0.007%
81	12.696	3623	3625	3628	rBV3	1419	751	0.05%	0.006%
82	12.734	3634	3637	3641	rBV6	1469	1277	0.09%	0.009%
83	12.786	3648	3653	3654	rBV6	1245	972	0.06%	0.007%
84	12.869	3678	3679	3681	rVB2	1232	385	0.03%	0.003%
85	12.943	3699	3702	3705	rBV5	1185	909	0.06%	0.007%
86	12.963	3705	3708	3710	rVB3	1444	704	0.05%	0.005%
87	12.982	3710	3714	3715	rBV3	915	562	0.04%	0.004%
88	13.065	3738	3740	3744	rVB5	1742	779	0.05%	0.006%
89	13.220	3786	3788	3791	rVB4	1952	1060	0.07%	0.008%
90	13.249	3795	3797	3798	rBV2	1198	553	0.04%	0.004%
91	13.352	3826	3829	3833	rBV6	1670	1434	0.10%	0.011%
92	13.400	3843	3844	3846	rBV2	1225	635	0.04%	0.005%
93	13.715	3940	3942	3945	rVB3	1498	482	0.03%	0.004%
94	13.747	3948	3952	3954	rBV5	1792	1244	0.08%	0.009%
95	13.959	4016	4018	4019	rBV2	1324	727	0.05%	0.005%
96	14.114	4064	4066	4067	rBV2	1525	642	0.04%	0.005%
97	14.175	4083	4085	4089	rVB4	2239	1219	0.08%	0.009%
98	14.194	4089	4091	4093	rBV3	1732	934	0.06%	0.007%
99	15.075	4363	4365	4368	rBV5	1338	916	0.06%	0.007%
100	15.139	4383	4385	4386	rBV2	1711	592	0.04%	0.004%




Sum of corrected areas: 13619955

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028813.D
Acq On : 01 Nov 2022 14:02
Operator : SY/MD
Sample : N5301-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBXB4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

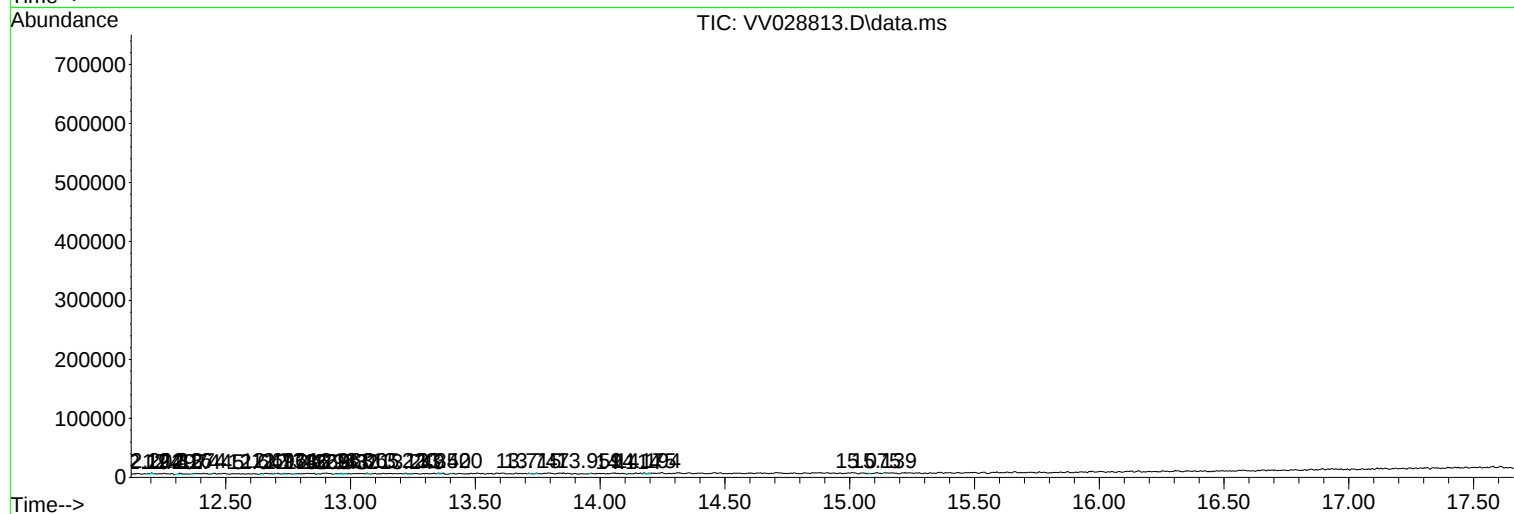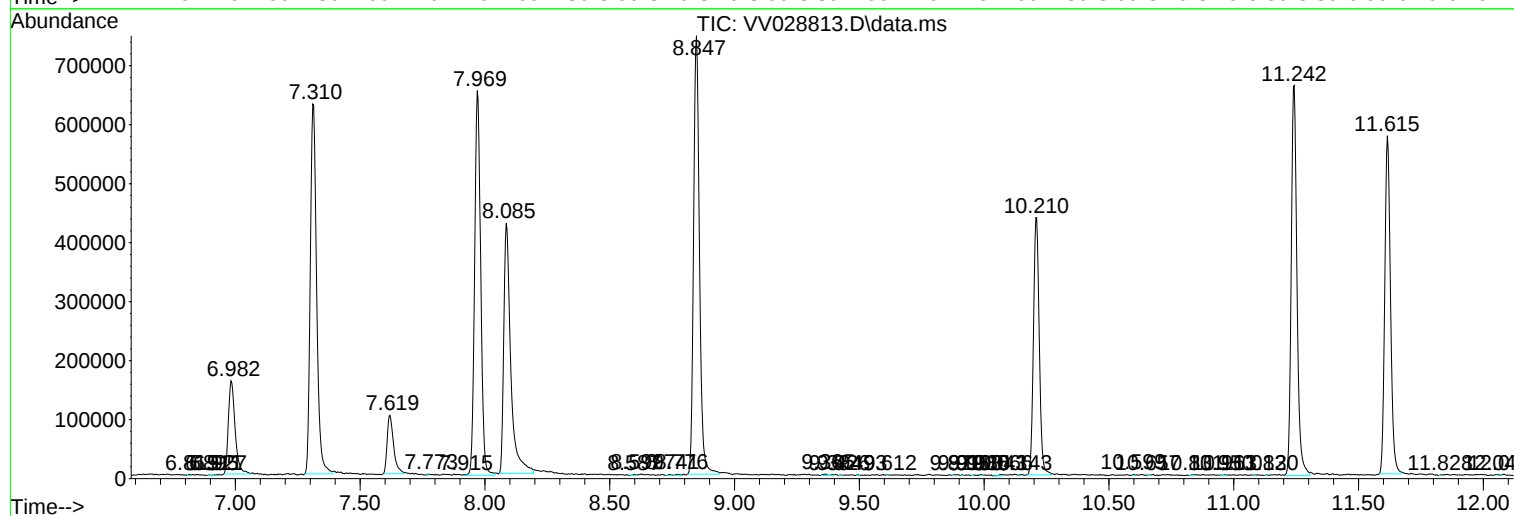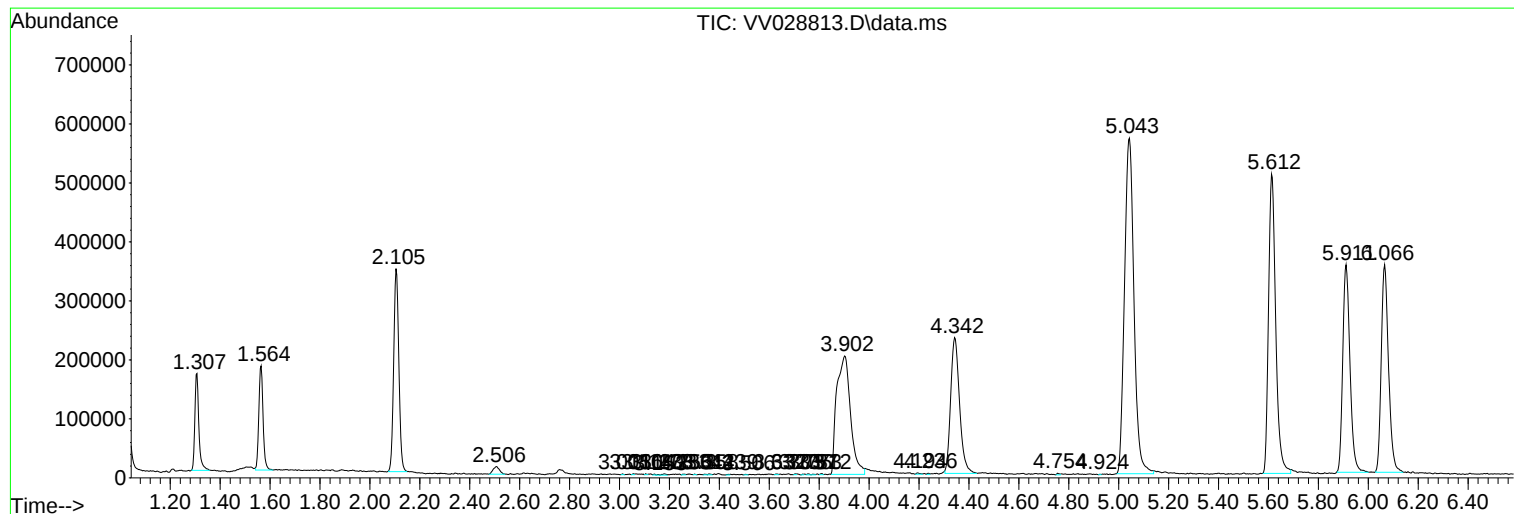

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028813.D
Acq On : 01 Nov 2022 14:02
Operator : SY/MD
Sample : N5301-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBXB4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110122\
Data File : VV028813.D
Acq On : 01 Nov 2022 14:02
Operator : SY/MD
Sample : N5301-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBXB4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------